


Data Path : Z:\voasrv\HPCHEM1\MSVOA_F\Data\VF112718\
 Data File : VF060834.D
 Acq On : 27 Nov 2018 12:33
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F112618S.M
 Title : SW846 8260
 Last Update : Tue Nov 27 01:36:26 2018

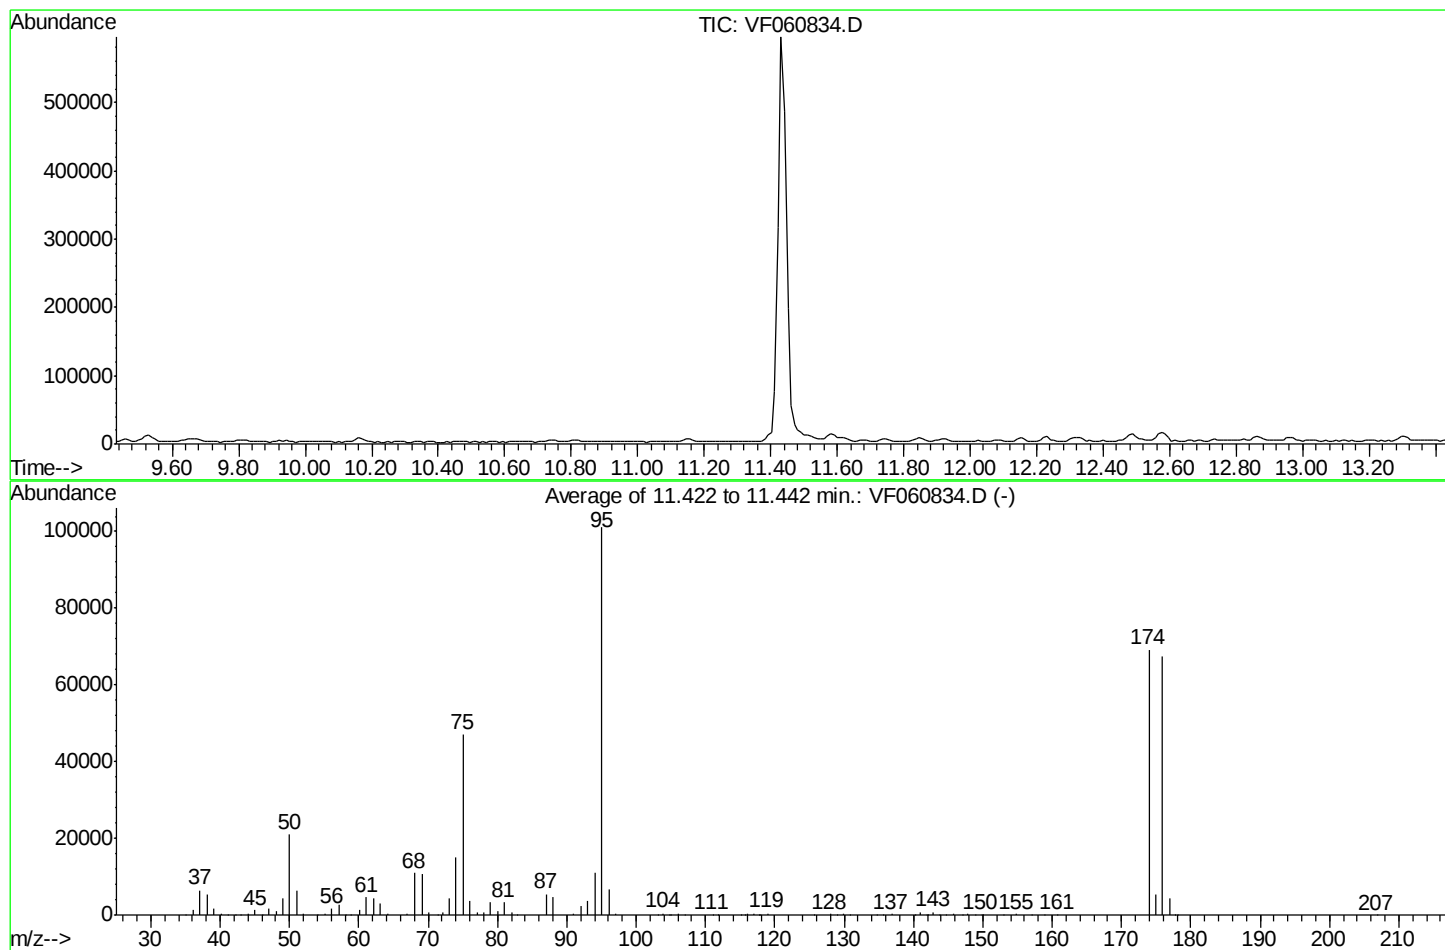

AutoFind: Scans 1094, 1095, 1096; Background Corrected with Scan 1089

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	20933	PASS
75	95	30	60	46.5	46986	PASS
95	95	100	100	100.0	101109	PASS
96	95	5	9	6.7	6764	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	68.5	69269	PASS
175	174	5	9	7.8	5409	PASS
176	174	95	101	97.4	67474	PASS
177	176	5	9	6.6	4485	PASS