


Data Path : Z:\voasrv\HPCHEM1\MSVOA_F\Data\VF112818\
Data File : VF060849.D
Acq On : 28 Nov 2018 9:45
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F112618S.M
Title : SW846 8260
Last Update : Tue Nov 27 01:36:26 2018

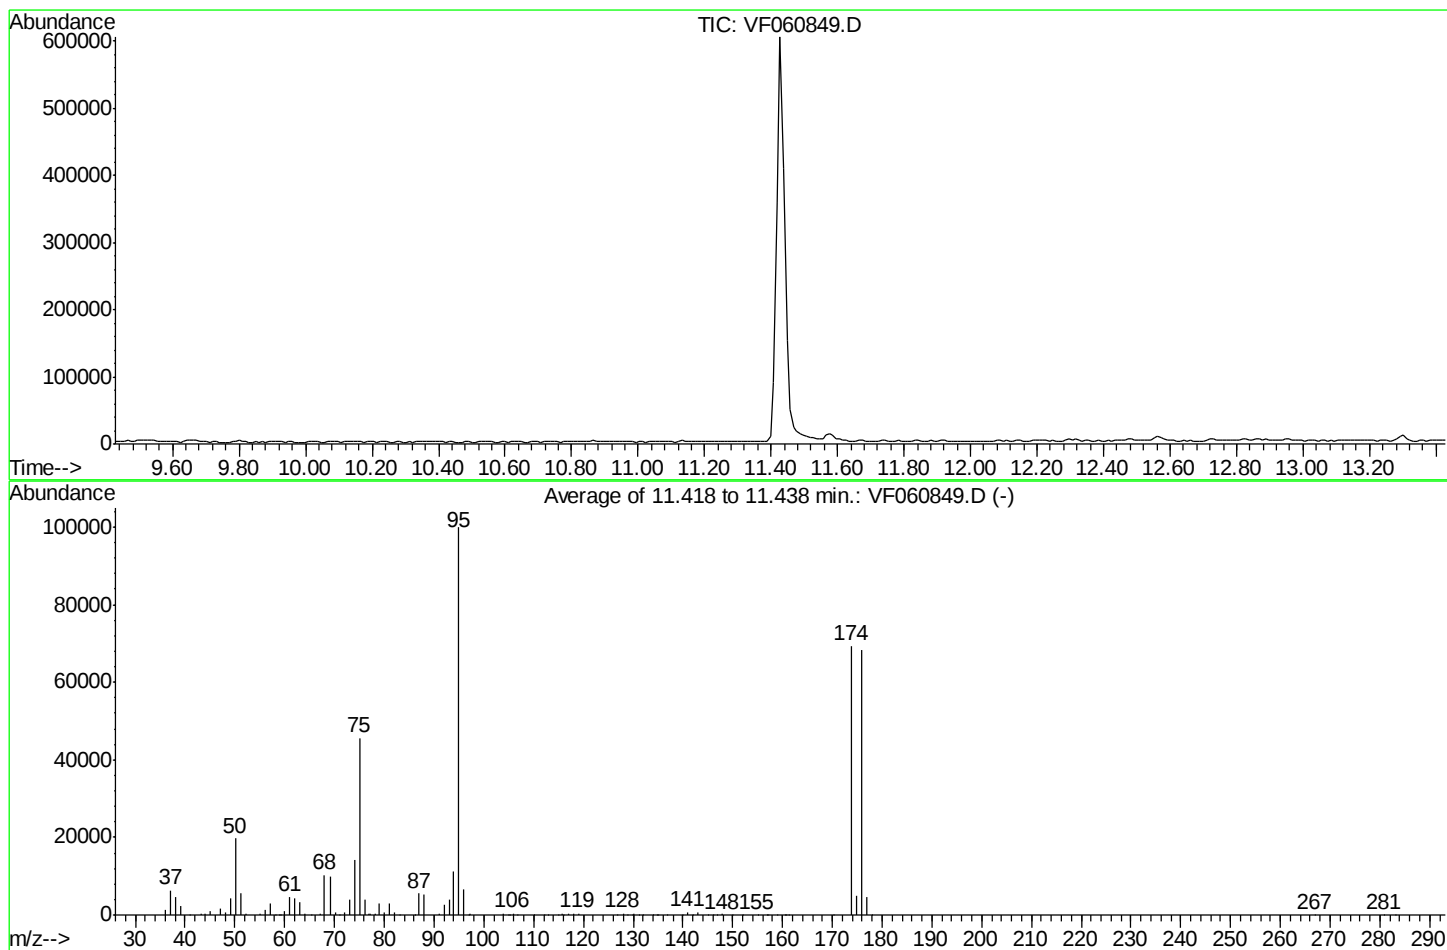

AutoFind: Scans 1094, 1095, 1096; Background Corrected with Scan 1089

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	19763	PASS
75	95	30	60	45.6	45549	PASS
95	95	100	100	100.0	99944	PASS
96	95	5	9	6.5	6504	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.4	69378	PASS
175	174	5	9	7.3	5063	PASS
176	174	95	101	98.5	68312	PASS
177	176	5	9	6.6	4507	PASS