


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF112918\
Data File : VF060865.D
Acq On : 29 Nov 2018 13:04
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F112618S.M
Title : SW846 8260
Last Update : Tue Nov 27 01:36:26 2018

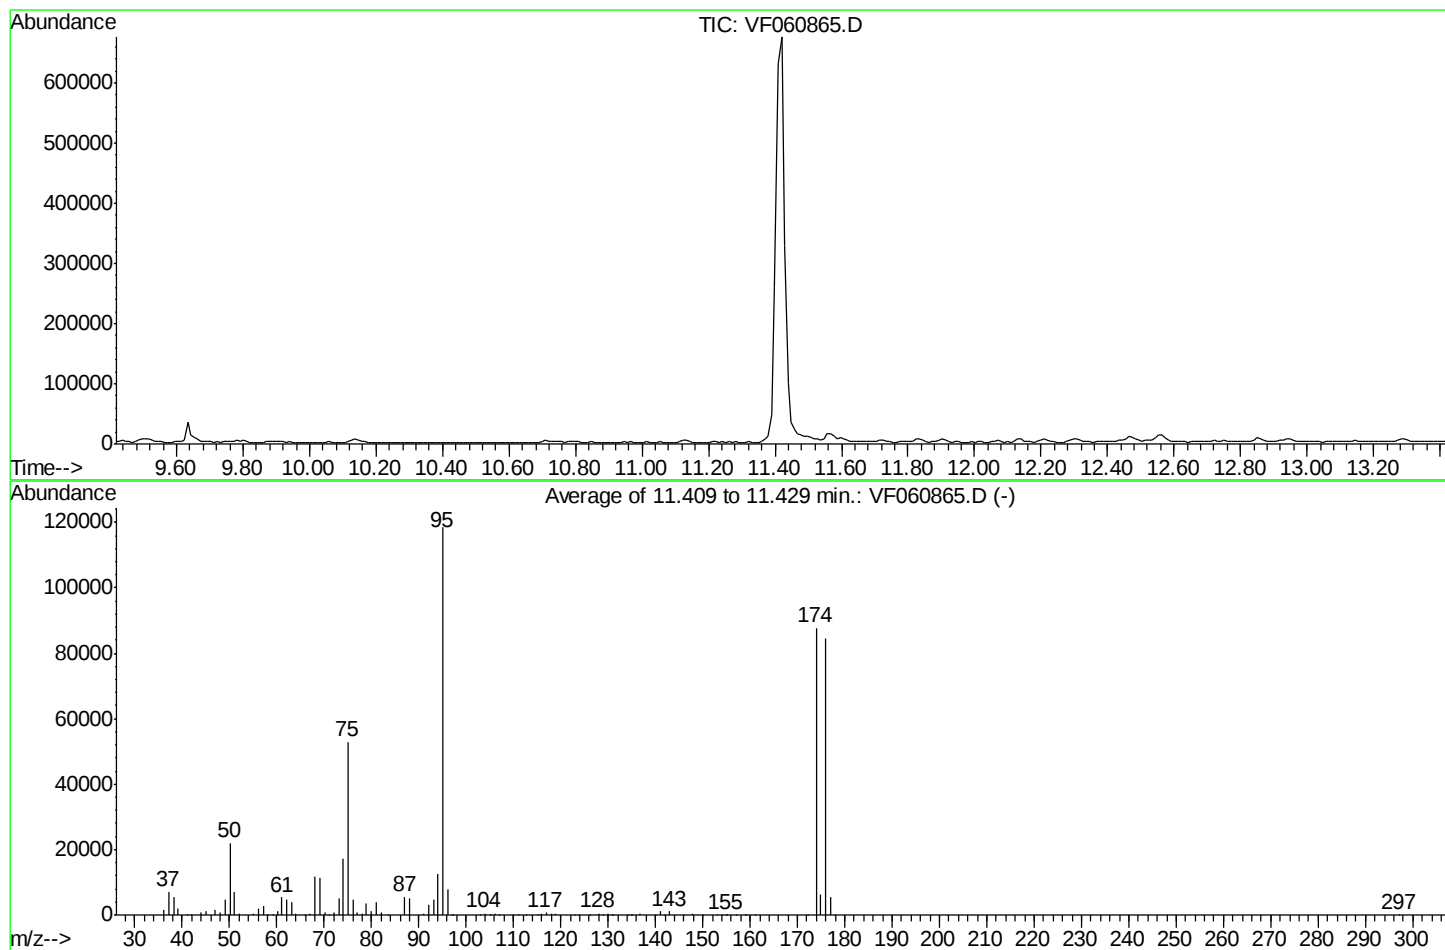

AutoFind: Scans 1093, 1094, 1095; Background Corrected with Scan 1087

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	22011	PASS
75	95	30	60	44.7	52962	PASS
95	95	100	100	100.0	118488	PASS
96	95	5	9	6.7	7906	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.1	87826	PASS
175	174	5	9	7.3	6402	PASS
176	174	95	101	96.2	84453	PASS
177	176	5	9	6.5	5501	PASS