

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_F\DATA\VF121018\
 Data File : VF060957.D
 Acq On : 10 Dec 2018 16:54
 Operator : VA/AP
 Sample : J6327-02RE
 Misc : 5.07g/5mL/MSVOA-F/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 STOCK-PILERE


Quant Time: Dec 11 04:57:34 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F112618S.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 27 01:36:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.88	168	14581	50.00	ug/l	-0.03
34) 1,4-Difluorobenzene	5.60	114	17358	50.00	ug/l	-0.04
63) Chlorobenzene-d5	9.77	117	11384	50.00	ug/l	-0.04
72) 1,4-Dichlorobenzene-d4	12.55	152	4059	50.00	ug/l	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	4.84	65	2134	12.42	ug/l	-0.04
Spiked Amount			Recovery	=	24.84%	
35) Dibromofluoromethane	4.10	113	3233	23.48	ug/l	-0.05
Spiked Amount			Recovery	=	46.96%	
50) Toluene-d8	7.55	98	14241	35.11	ug/l	-0.04
Spiked Amount			Recovery	=	70.22%	
62) 4-Bromofluorobenzene	11.41	95	3495	18.96	ug/l	-0.03
Spiked Amount			Recovery	=	37.92%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.08	50	351	2.474	ug/l #	41
5) Bromomethane	1.34	94	291	3.119	ug/l #	63
6) Chloroethane	1.40	64	60	1.049	ug/l #	1
8) Diethyl Ether	1.55	74	154	3.772	ug/l	46
11) Tert butyl alcohol	2.48	59	85	12.072	ug/l #	1
13) Acrolein	2.09	56	329	49.315	ug/l	94
14) Allyl chloride	2.12	41	518	3.600	ug/l #	64
15) Acrylonitrile	2.94	53	835	52.895	ug/l #	26
16) Acetone	2.30	43	797	25.162	ug/l	98
18) Methyl Acetate	2.38	43	837	14.581	ug/l #	61
23) Vinyl Acetate	3.22	43	726	4.055	ug/l #	80
25) 2-Butanone	4.37	43	990	18.070	ug/l #	57
26) 2,2-Dichloropropane	3.68	77	310	2.052	ug/l #	60
29) Tetrahydrofuran	4.08	42	153	6.588	ug/l #	37
37) Ethyl Acetate	4.16	43	223	2.850	ug/l #	14
41) Methacrylonitrile	4.73	41	383	6.045	ug/l #	39
43) Isopropyl Acetate	6.90	43	982	7.882	ug/l #	49
48) Methyl methacrylate	6.72	41	376	5.309	ug/l #	40
49) 1,4-Dioxane	6.81	88	71	136.984	ug/l #	17
51) 4-Methyl-2-Pentanone	8.25	43	586	8.122	ug/l #	38
59) 2-Hexanone	9.47	43	398	7.863	ug/l #	27
74) N-amyl acetate	11.39	43	732	9.883	ug/l #	48
75) 1,1,2,2-Tetrachloroethane	11.67	83	65	1.231	ug/l #	25
92) 1,2-Dibromo-3-Chloropropan	13.63	75	59	5.781	ug/l #	1
95) Naphthalene	14.46	128	861	1.627	ug/l #	59

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.88 min Scan# 431

Delta R.T. -0.03 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54

Instrument :

MSVOA_F

ClientSampleId :


STOCK-PILERE

Tgt Ion:168 Resp: 14581

Ion Ratio Lower Upper

168 100

99 78.9 52.6 79.0



Abundance Ion 168.00 (167.70 to 168.70): VF0

Ion 99.00 (98.70 to 99.70): VF0

4.88

4000

3000

2000

1000



0

4.80

4.90

5.00

Time-->



#3

Chloromethane

Concen: 2.474 ug/l

RT: 1.08 min Scan# 46

Delta R.T. -0.02 min

Lab File: VF060957.D


Acq: 10 Dec 2018 16:54

Tgt Ion: 50 Resp: 351

Ion Ratio Lower Upper

50 100

52 0.0 27.0 40.4#



Abundance Ion 50.00 (49.70 to 50.70): VF0

Ion 52.00 (51.70 to 52.70): VF0

1.08

300

200

100


0


1.06

1.08

1.10

Time-->





#5

Bromomethane

Concen: 3.119 ug/l

RT: 1.34 min Scan# 72

Delta R.T. -0.00 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54

Instrument :

MSVOA_F

ClientSampleId :


STOCK-PILERE

Tgt Ion: 94 Resp: 291

Ion Ratio Lower Upper



94 100

96 58.8 75.9 113.9#

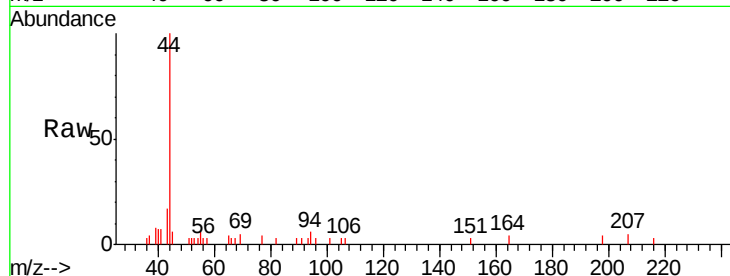


Abundance Ion 94.00 (93.70 to 94.70): VF0

Ion 96.00 (95.70 to 96.70): VF0

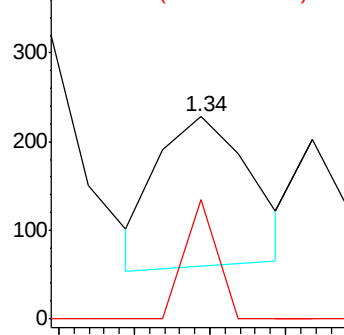

Time-->



#6

Chloroethane

Concen: 1.049 ug/l

RT: 1.40 min Scan# 78

Delta R.T. 0.01 min

Lab File: VF060957.D


Acq: 10 Dec 2018 16:54

Tgt Ion: 64 Resp: 60

Ion Ratio Lower Upper



64 100

66 161.8 28.1 42.1#




Abundance Ion 64.00 (63.70 to 64.70): VF0

Ion 66.00 (65.70 to 66.70): VF0

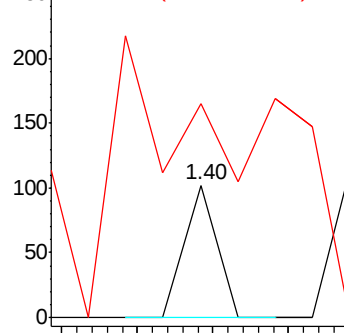





Time-->



#8
Diethyl Ether
Concen: 3.772 ug/l
RT: 1.55 min Scan# 94
Delta R.T. -0.09 min
Lab File: VF060957.D
Acq: 10 Dec 2018 16:54




Instrument :
MSVOA_F
ClientSampleId :
STOCK-PILERE


Tgt Ion: 74 Resp: 154
Ion Ratio Lower Upper
74 100
45 207.6 71.0 212.8

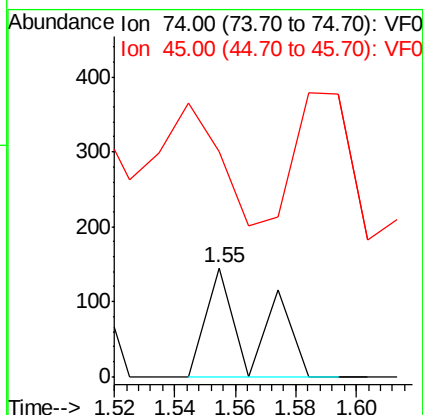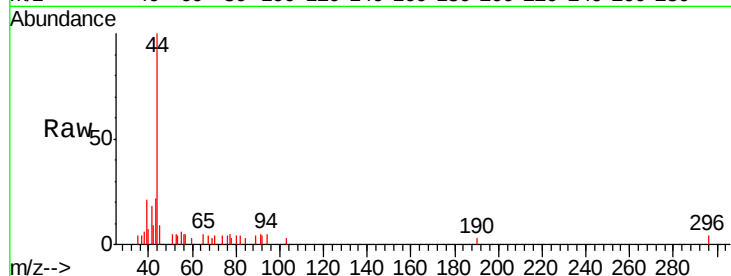

#11
Tert butyl alcohol
Concen: 12.072 ug/l
RT: 2.48 min Scan# 188
Delta R.T. -0.10 min
Lab File: VF060957.D
Acq: 10 Dec 2018 16:54

Tgt Ion: 59 Resp: 85
Ion Ratio Lower Upper
59 100
57 131.5 12.7 19.1#

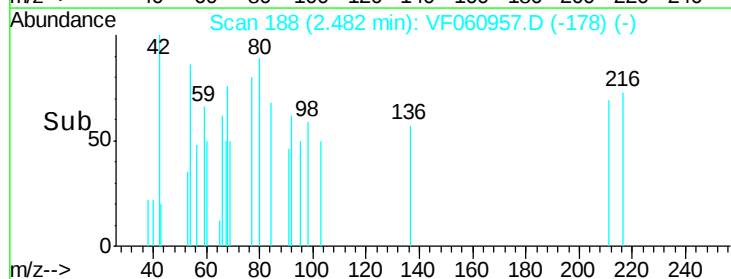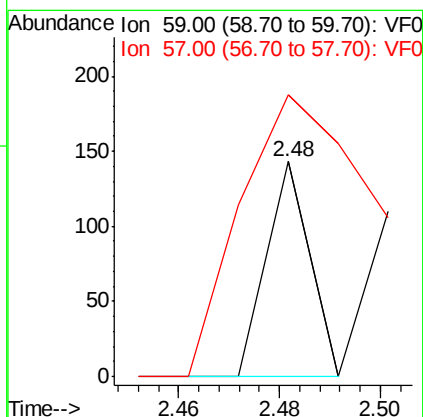

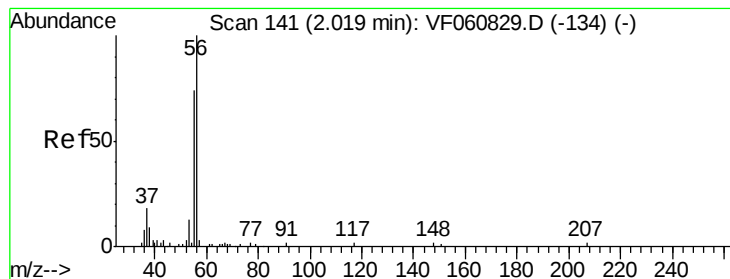

#13

Acrolein

Concen: 49.315 ug/l

RT: 2.09 min Scan# 148

Delta R.T. 0.07 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54

Instrument :

MSVOA_F

ClientSampleId :





STOCK-PILERE

Tgt Ion: 56 Resp: 329

Ion Ratio Lower Upper

56 100

55 71.2 61.2 91.8

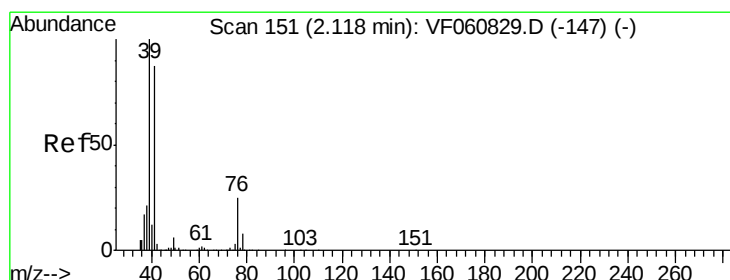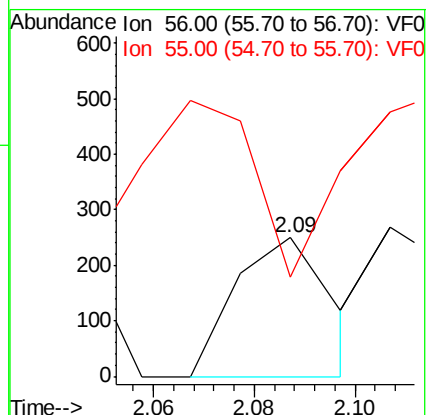

#14

Allyl chloride

Concen: 3.600 ug/l

RT: 2.12 min Scan# 151

Delta R.T. -0.00 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54




Tgt Ion: 41 Resp: 518


Ion Ratio Lower Upper

41 100

39 80.5 91.7 137.5#

76 0.0 23.5 35.3#

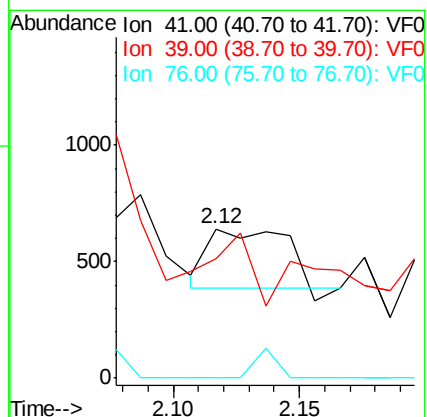



#15

Acrylonitrile

Concen: 52.895 ug/l

RT: 2.94 min Scan# 234

Delta R.T. -0.03 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54

Instrument :

MSVOA_F

ClientSampleId :

STOCK-PILERE


Tgt Ion: 53 Resp: 835

Ion Ratio Lower Upper

53 100

52 0.0 76.5 114.7#




51 30.1 40.7 61.1#



Abundance Ion 53.00 (52.70 to 53.70): VF0

Ion 52.00 (51.70 to 52.70): VF0

Ion 51.00 (50.70 to 51.70): VF0

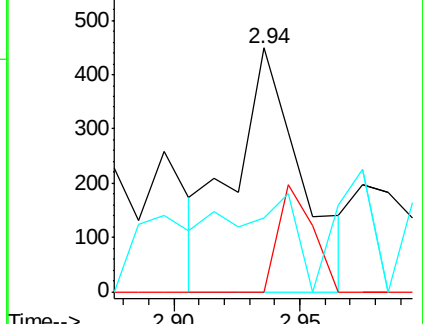

#16

Acetone

Concen: 25.162 ug/l

RT: 2.30 min Scan# 170

Delta R.T. 0.05 min

Lab File: VF060957.D


Acq: 10 Dec 2018 16:54

Tgt Ion: 43 Resp: 797

Ion Ratio Lower Upper



43 100


58 15.2 11.4 17.2



Abundance Ion 43.00 (42.70 to 43.70): VF0

Ion 58.00 (57.70 to 58.70): VF0




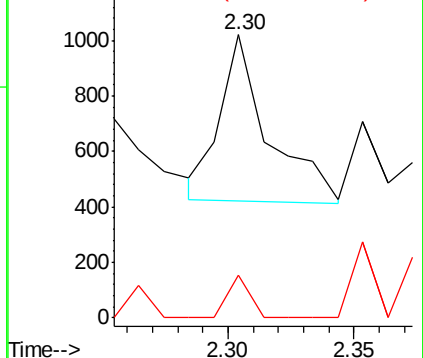




#18
Methyl Acetate
Concen: 14.581 ug/l
RT: 2.38 min Scan# 178
Delta R.T. 0.02 min
Lab File: VF060957.D
Acq: 10 Dec 2018 16:54




Instrument :
MSVOA_F
ClientSampleId :
STOCK-PILERE


Tgt Ion: 43 Resp: 837
Ion Ratio Lower Upper
43 100
74 0.0 13.3 19.9#

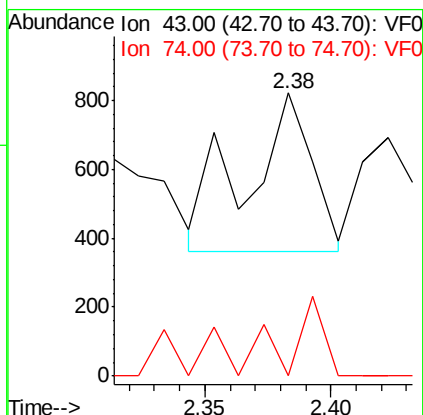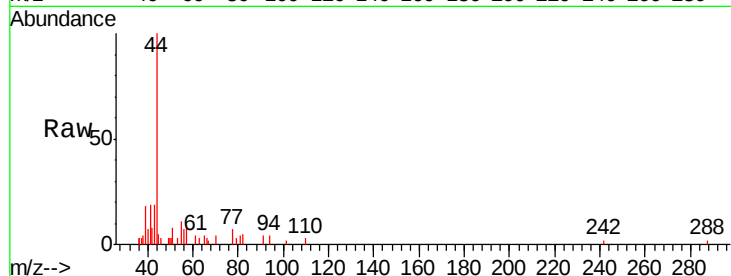

#23
Vinyl Acetate
Concen: 4.055 ug/l
RT: 3.22 min Scan# 263
Delta R.T. 0.01 min
Lab File: VF060957.D
Acq: 10 Dec 2018 16:54

Tgt Ion: 43 Resp: 726
Ion Ratio Lower Upper
43 100
86 0.0 5.4 8.0#

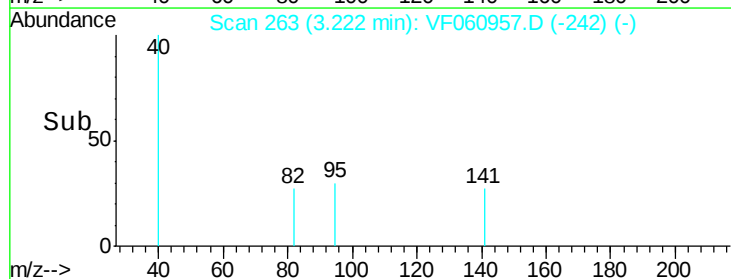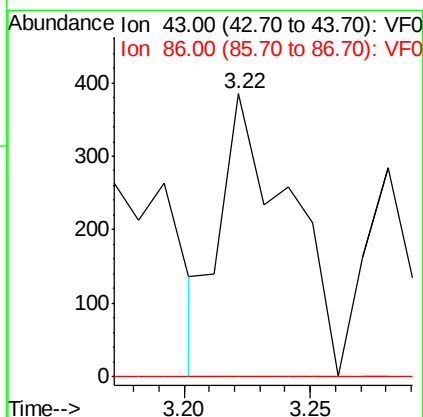

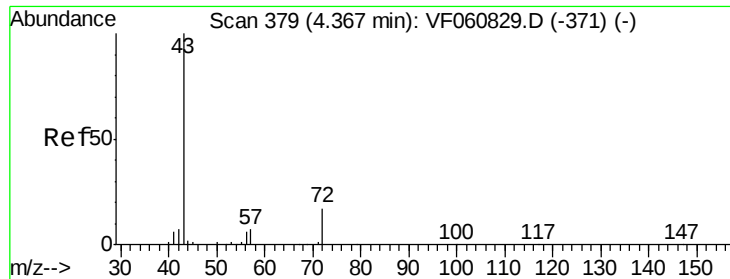

#25

2-Butanone

Concen: 18.070 ug/l

RT: 4.37 min Scan# 379

Delta R.T. -0.00 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54

Instrument :

MSVOA_F

ClientSampleId :


STOCK-PILERE

Tgt Ion: 43 Resp: 990

Ion Ratio Lower Upper

43 100

72 0.0 15.4 23.2#

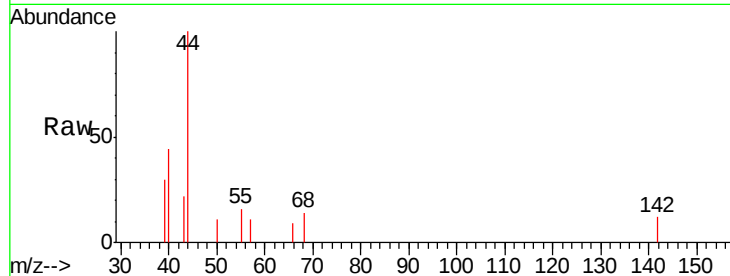

Abundance Ion 43.00 (42.70 to 43.70): VF0

Ion 72.00 (71.70 to 72.70): VF0

300

250

200

150

100

50

0



4.25

4.30

4.35

4.40

Time-->



#26

2,2-Dichloropropane

Concen: 2.052 ug/l

RT: 3.68 min Scan# 309

Delta R.T. 0.04 min

Lab File: VF060957.D


Acq: 10 Dec 2018 16:54

Tgt Ion: 77 Resp: 310

Ion Ratio Lower Upper

77 100

97 0.0 8.6 25.8#



Abundance Ion 77.00 (76.70 to 77.70): VF0

Ion 97.00 (96.70 to 97.70): VF0

200

150

100


50


0

3.65

3.70

Time-->





#29

Tetrahydrofuran

Concen: 6.588 ug/l

RT: 4.08 min Scan# 350

Delta R.T. -0.03 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54

Instrument :

MSVOA_F

ClientSampleId :

STOCK-PILERE


Tgt Ion: 42 Resp: 153

Ion Ratio Lower Upper

42 100

72 0.0 31.9 47.9#

71 0.0 28.7 43.1#



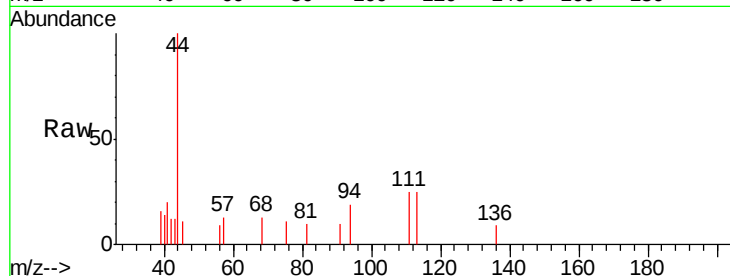


Abundance Ion 42.00 (41.70 to 42.70): VF0

Ion 72.00 (71.70 to 72.70): VF0

Ion 71.00 (70.70 to 71.70): VF0

Time-->

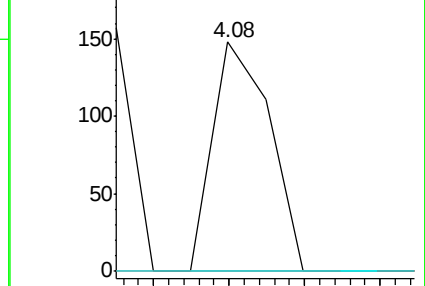

#33

1,2-Dichloroethane-d4

Concen: 12.424 ug/l

RT: 4.84 min Scan# 427

Delta R.T. -0.04 min

Lab File: VF060957.D


Acq: 10 Dec 2018 16:54

Tgt Ion: 65 Resp: 2134

Ion Ratio Lower Upper

65 100



67 37.1 0.0 96.4




Abundance Ion 65.00 (64.70 to 65.70): VF0

Ion 67.00 (66.70 to 67.70): VF0

Time-->

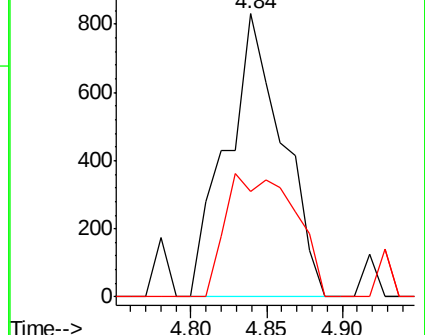



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.60 min Scan# 504

Delta R.T. -0.04 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54

Instrument :

MSVOA_F

ClientSampleId :

STOCK-PILERE


Tgt Ion:114 Resp: 17358

Ion Ratio Lower Upper

114 100

63 22.0 0.0 41.6




88 9.8 0.0 36.6

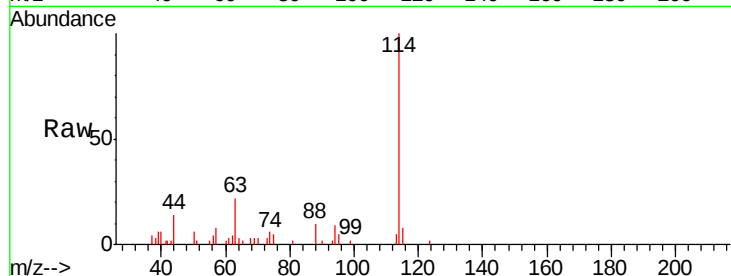

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 63.00 (62.70 to 63.70): VF0

Ion 88.00 (87.70 to 88.70): VF0

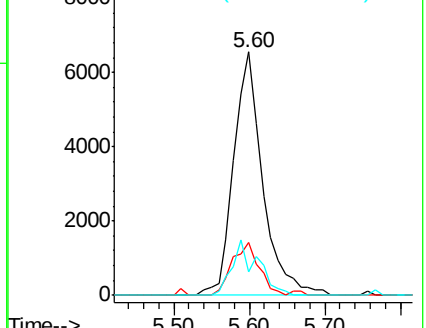

#35

Dibromofluoromethane

Concen: 23.478 ug/l

RT: 4.10 min Scan# 352

Delta R.T. -0.05 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54


Tgt Ion:113 Resp: 3233

Ion Ratio Lower Upper

113 100

111 97.2 83.0 124.6



192 15.2 12.3 18.5




Abundance Ion 113.00 (112.70 to 113.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 192.00 (191.70 to 192.70): V




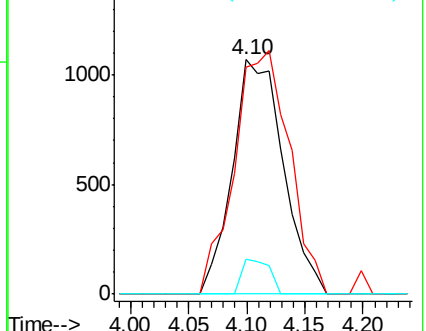




#37
Ethyl Acetate
Concen: 2.850 ug/l
RT: 4.16 min Scan# 358
Delta R.T. 0.01 min
Lab File: VF060957.D
Acq: 10 Dec 2018 16:54




Instrument :
MSVOA_F
ClientSampleId :
STOCK-PILERE


Tgt Ion: 43 Resp: 223
Ion Ratio Lower Upper
43 100
61 0.0 68.6 103.0#
70 0.0 9.0 13.4#

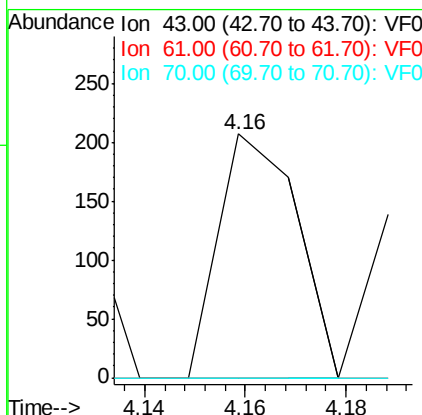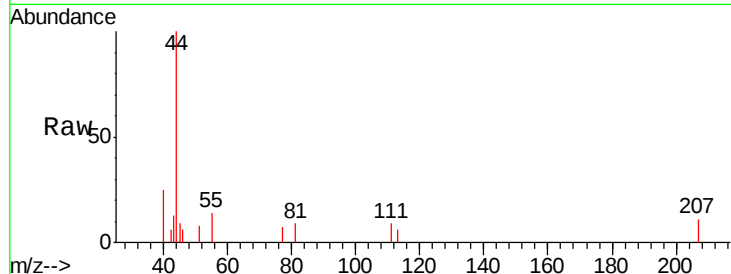

#41
Methacrylonitrile
Concen: 6.045 ug/l
RT: 4.73 min Scan# 416
Delta R.T. -0.05 min
Lab File: VF060957.D
Acq: 10 Dec 2018 16:54

Tgt Ion: 41 Resp: 383
Ion Ratio Lower Upper
41 100
39 100.0 53.0 79.6#
67 0.0 43.8 65.6#
52 0.0 37.8 56.8#

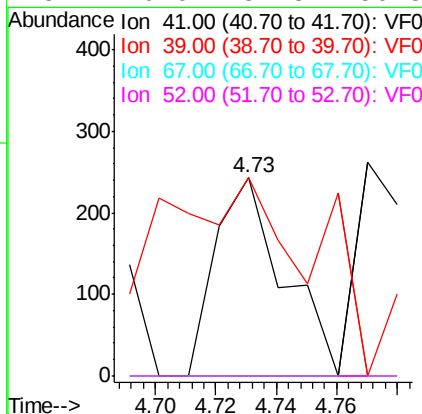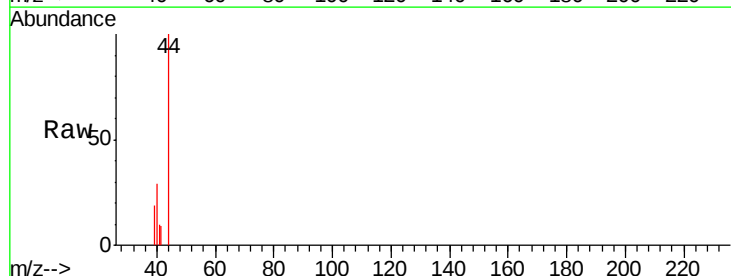

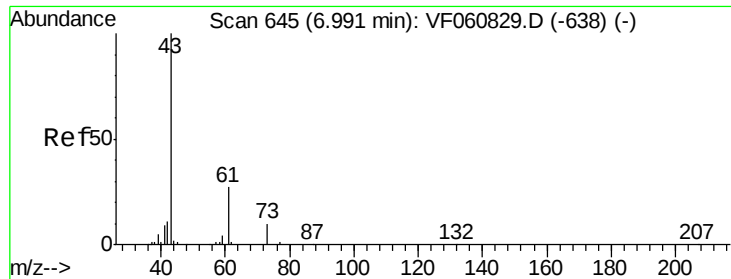

#43

Isopropyl Acetate

Concen: 7.882 ug/l

RT: 6.90 min Scan# 636

Delta R.T. -0.09 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54

Instrument :

MSVOA_F

ClientSampleId :

STOCK-PILERE


Tgt Ion: 43 Resp: 982

Ion Ratio Lower Upper

43 100

61 0.0 21.4 32.0#




87 0.0 0.2 0.4#

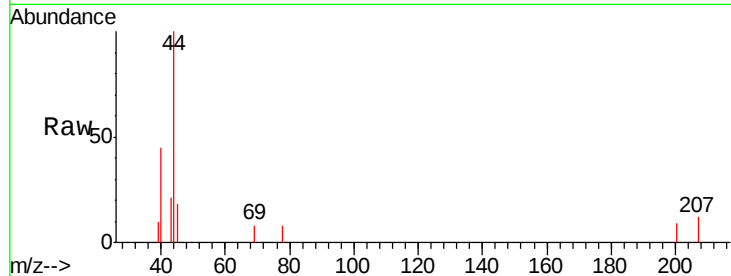

Abundance Ion 43.00 (42.70 to 43.70): VF0

Ion 61.00 (60.70 to 61.70): VF0

Ion 87.00 (86.70 to 87.70): VF0

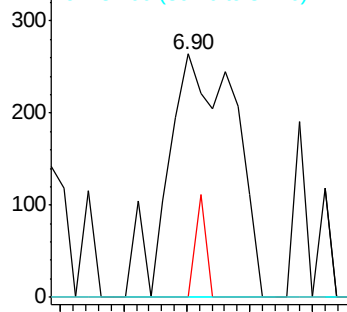

#48

Methyl methacrylate

Concen: 5.309 ug/l

RT: 6.72 min Scan# 618

Delta R.T. -0.03 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54


Tgt Ion: 41 Resp: 376

Ion Ratio Lower Upper

41 100

69 0.0 53.9 80.9#



39 87.8 49.0 73.6#




Abundance Ion 41.00 (40.70 to 41.70): VF0

Ion 69.00 (68.70 to 69.70): VF0

Ion 39.00 (38.70 to 39.70): VF0

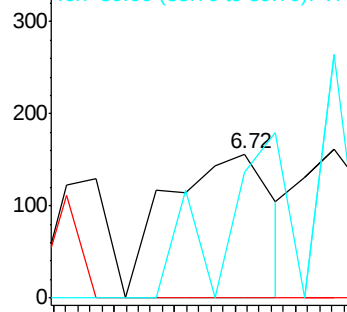

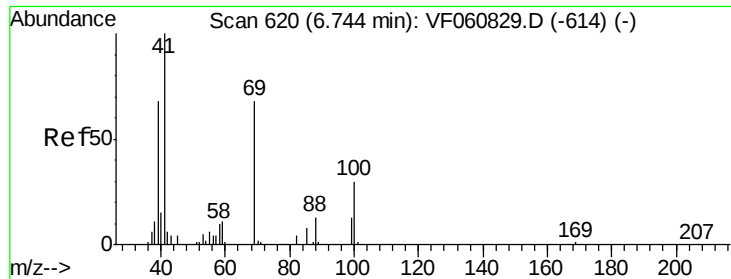

#49

1,4-Dioxane

Concen: 136.984 ug/l

RT: 6.81 min Scan# 627

Delta R.T. 0.07 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54

Instrument :
MSVOA_F
ClientSampleId :
STOCK-PILERE





Tgt Ion: 88 Resp: 71

Ion Ratio Lower Upper

88 100

43 0.0 42.0 63.0#

58 0.0 61.8 92.8#

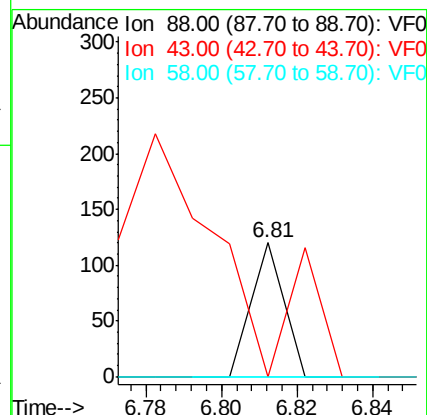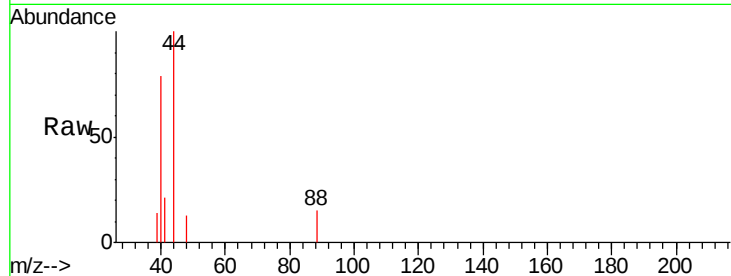

#50

Toluene-d8

Concen: 35.108 ug/l

RT: 7.55 min Scan# 702

Delta R.T. -0.04 min

Lab File: VF060957.D




Acq: 10 Dec 2018 16:54


Tgt Ion: 98 Resp: 14241

Ion Ratio Lower Upper

98 100

100 66.7 59.3 88.9

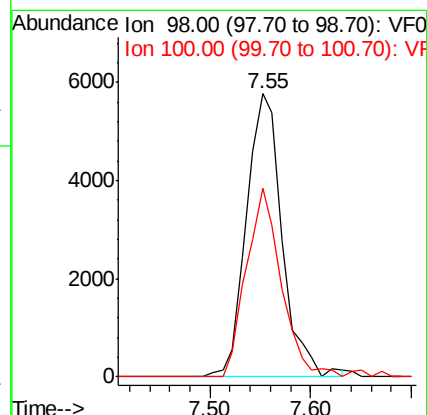

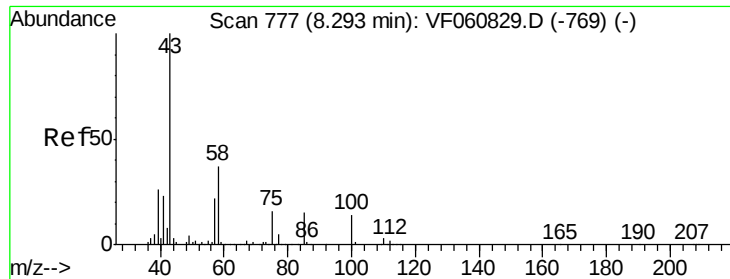

#51

4-Methyl-2-Pentanone

Concen: 8.122 ug/l

RT: 8.25 min Scan# 773

Delta R.T. -0.04 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54

Instrument :

MSVOA_F

ClientSampleId :


STOCK-PILERE

Tgt Ion: 43 Resp: 586

Ion Ratio Lower Upper

43 100

58 0.0 29.7 44.5#

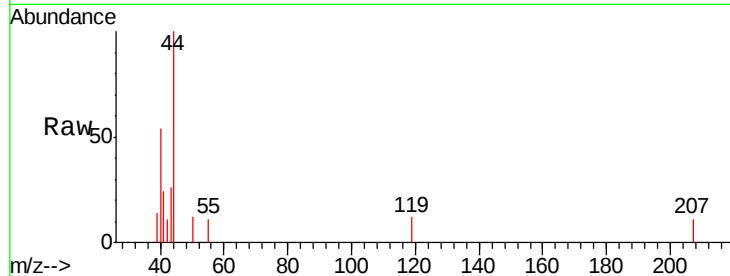

Abundance Ion 43.00 (42.70 to 43.70): VF0

Ion 58.00 (57.70 to 58.70): VF0

8.25

250

200



150

100

50

0

Time-->



#59

2-Hexanone

Concen: 7.863 ug/l

RT: 9.47 min Scan# 896

Delta R.T. -0.06 min

Lab File: VF060957.D


Acq: 10 Dec 2018 16:54

Tgt Ion: 43 Resp: 398

Ion Ratio Lower Upper

43 100

58 0.0 25.6 76.6#



Abundance Ion 43.00 (42.70 to 43.70): VF0

Ion 58.00 (57.70 to 58.70): VF0

9.47

250

200


150


100

50

0

Time-->









#62
4-Bromofluorobenzene
Concen: 18.958 ug/l
RT: 11.41 min Scan# 1093
Delta R.T. -0.03 min
Lab File: VF060957.D
Acq: 10 Dec 2018 16:54




Instrument :
MSVOA_F
ClientSampleId :
STOCK-PILERE


Tgt Ion: 95 Resp: 3495
Ion Ratio Lower Upper
95 100
174 75.8 0.0 138.2
176 60.8 0.0 146.2

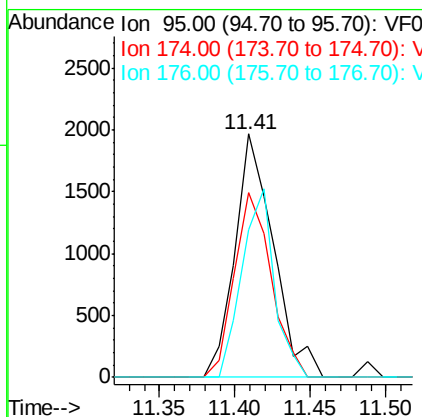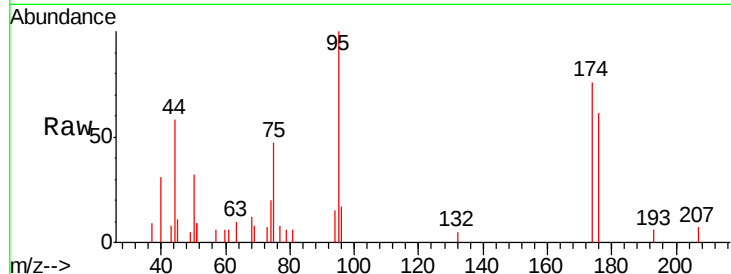

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.77 min Scan# 927
Delta R.T. -0.04 min
Lab File: VF060957.D
Acq: 10 Dec 2018 16:54

Tgt Ion: 117 Resp: 11384
Ion Ratio Lower Upper
117 100
82 56.0 46.6 69.8
119 36.3 26.4 39.6

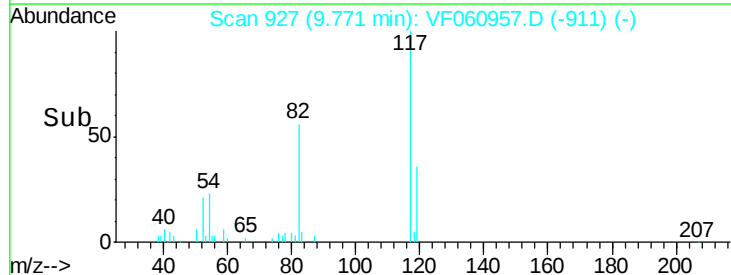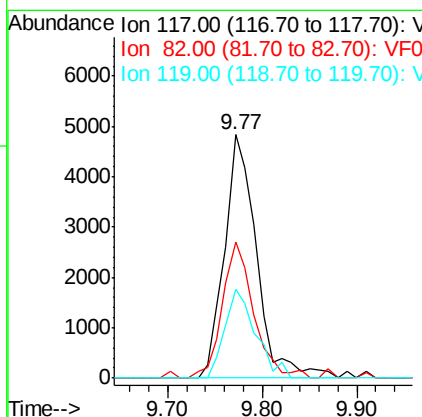

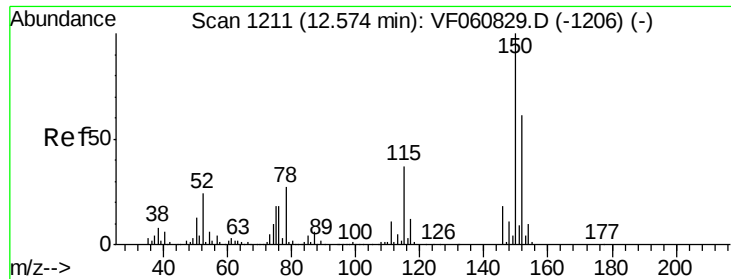

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.55 min Scan# 1209

Delta R.T. -0.02 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54

Instrument :

MSVOA_F

ClientSampleId :

STOCK-PILERE


Tgt Ion: 152 Resp: 4059

Ion Ratio Lower Upper

152 100

115 52.6 30.1 90.5




150 154.5 0.0 327.6

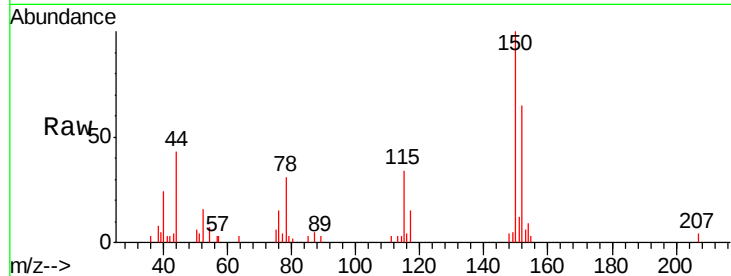

Abundance Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

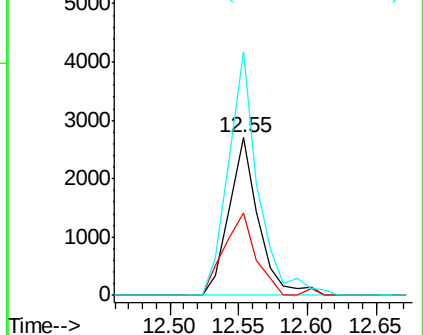

#74

N-ethyl acetate

Concen: 9.883 ug/l

RT: 11.39 min Scan# 1091

Delta R.T. -0.01 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54

Tgt Ion: 43 Resp: 732


Ion Ratio Lower Upper

43 100

70 0.0 29.6 44.4#

55 38.4 17.2 25.8#

61 0.0 21.8 32.6#






Abundance Ion 43.00 (42.70 to 43.70): VF0

Ion 70.00 (69.70 to 70.70): VF0

Ion 55.00 (54.70 to 55.70): VF0

Ion 61.00 (60.70 to 61.70): VF0

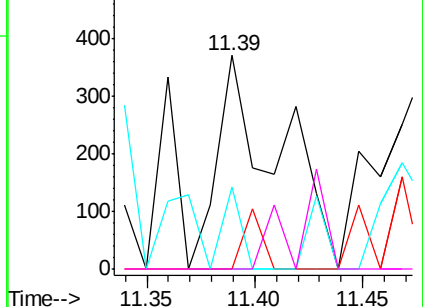

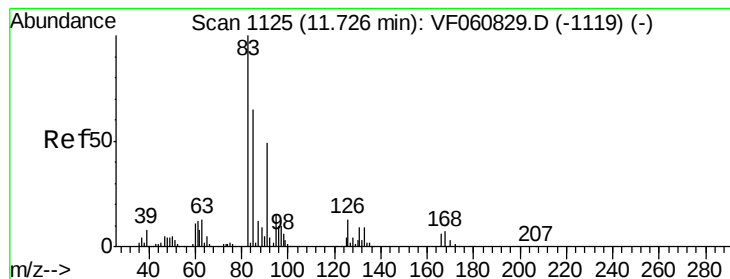

#75

1,1,2,2-Tetrachloroethane

Concen: 1.231 ug/l

RT: 11.67 min Scan# 1119

Delta R.T. -0.06 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54

Instrument :

MSVOA_F

ClientSampleId :

STOCK-PILERE


Tgt Ion: 83 Resp: 65

Ion Ratio Lower Upper

83 100

131 0.0 4.7 14.1#




85 0.0 32.6 97.8#

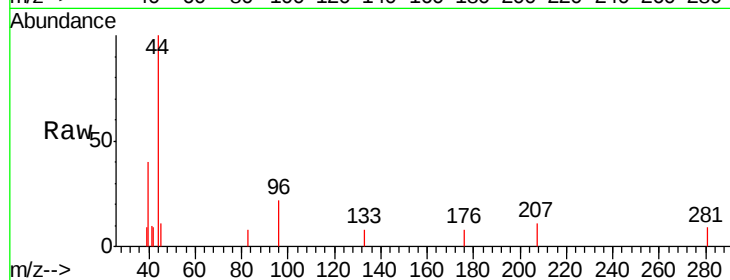

Abundance Ion 83.00 (82.70 to 83.70): VF0

Ion 131.00 (130.70 to 131.70): V

Ion 85.00 (84.70 to 85.70): VF0

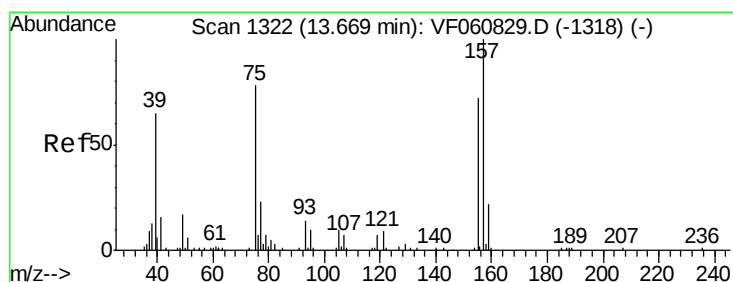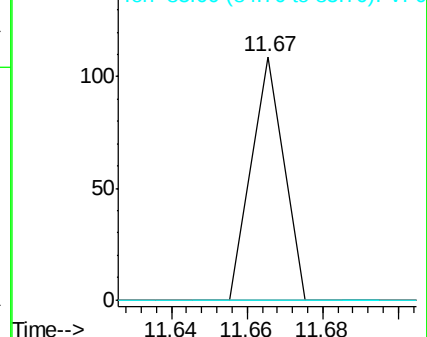

#92

1,2-Dibromo-3-Chloropropane

Concen: 5.781 ug/l

RT: 13.63 min Scan# 1318

Delta R.T. -0.04 min

Lab File: VF060957.D

Acq: 10 Dec 2018 16:54


Tgt Ion: 75 Resp: 59

Ion Ratio Lower Upper

75 100

155 0.0 45.6 136.9#



157 0.0 63.8 191.5#

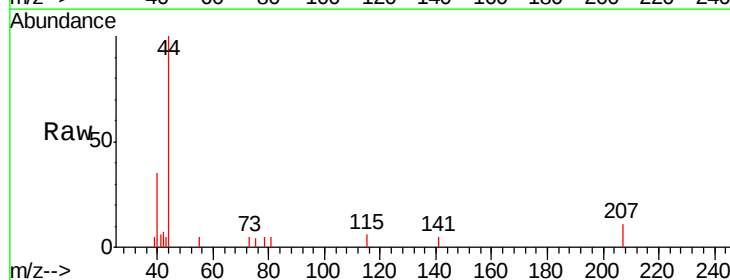


Abundance Ion 75.00 (74.70 to 75.70): VF0

Ion 155.00 (154.70 to 155.70): V

Ion 157.00 (156.70 to 157.70): V

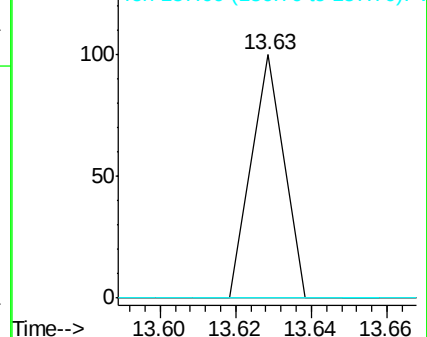



#95

Naphthalene

Concen: 1.627 ug/l

RT: 14.46 min Scan# 1402

Delta R.T. -0.02 min

Lab File: VF060957.D


Acq: 10 Dec 2018 16:54

Instrument :

MSVOA_F

ClientSampleId :

STOCK-PILERE

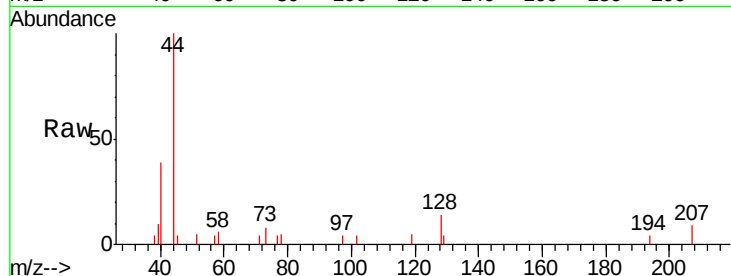


Tgt Ion:128 Resp: 861

Ion Ratio Lower Upper

128 100

127 0.0 9.9 14.9#

129 31.2 9.1 13.7#

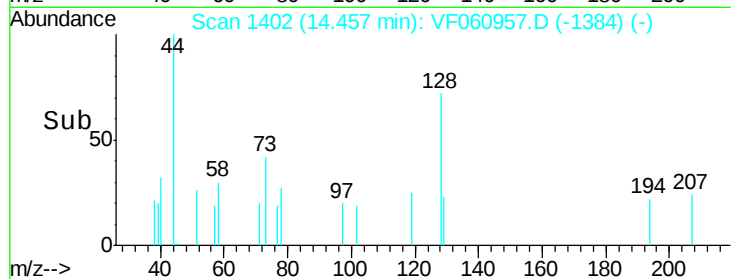

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

