


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_F\DATA\VF121418\
Data File : VF061013.D
Acq On : 14 Dec 2018 10:57
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F112618S.M
Title : SW846 8260
Last Update : Tue Nov 27 01:36:26 2018

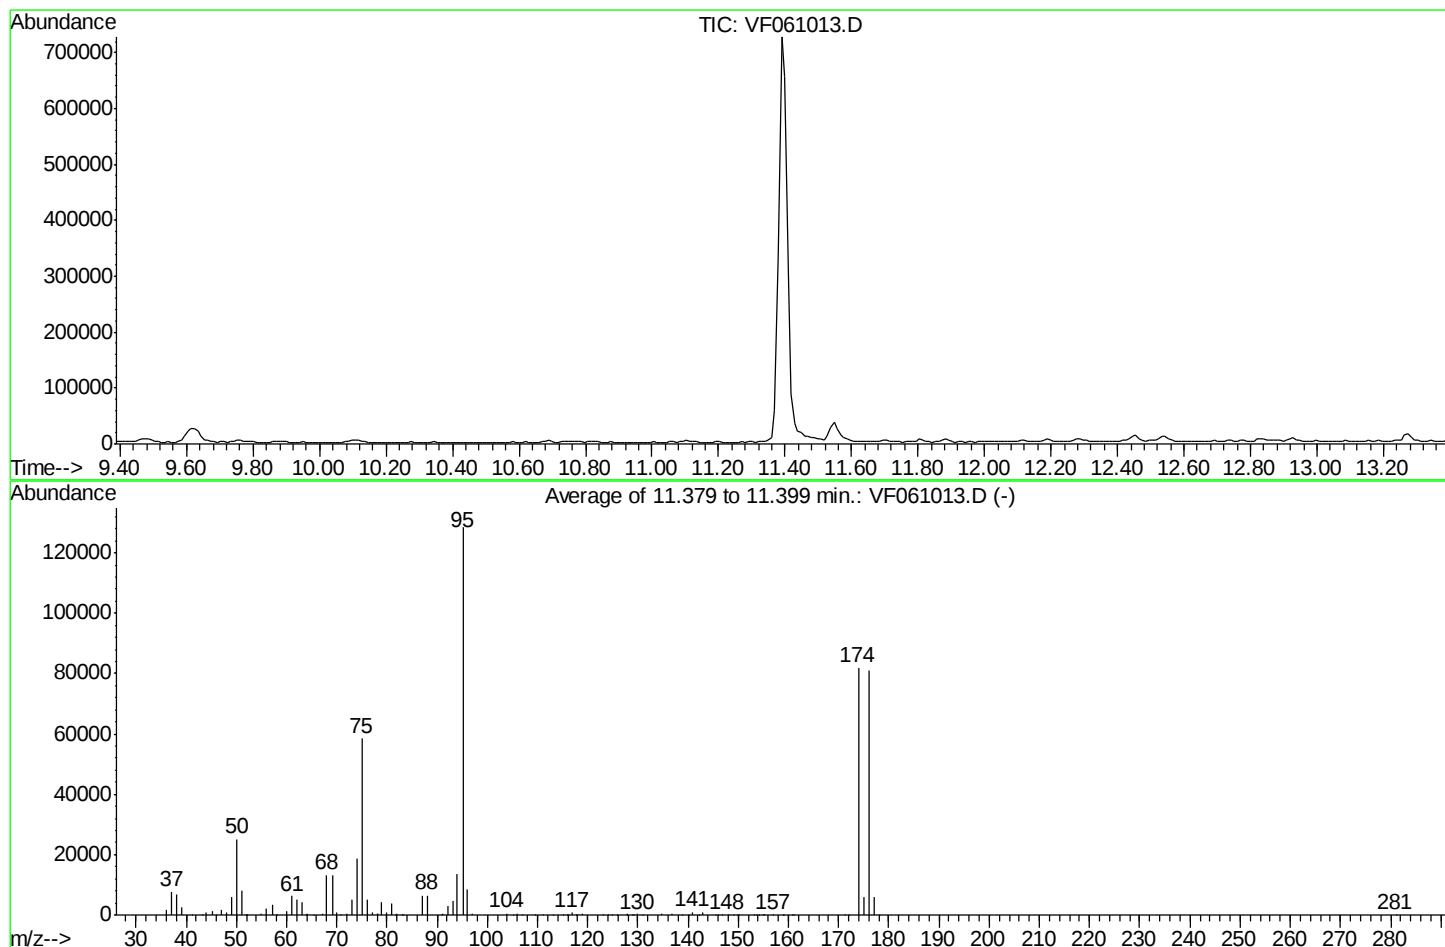

AutoFind: Scans 1090, 1091, 1092; Background Corrected with Scan 1082

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	25096	PASS
75	95	30	60	45.5	58525	PASS
95	95	100	100	100.0	128509	PASS
96	95	5	9	6.5	8300	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	63.8	81994	PASS
175	174	5	9	7.5	6118	PASS
176	174	95	101	98.9	81082	PASS
177	176	5	9	7.1	5745	PASS