

Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF121718\
 Data File : VF061054.D
 Acq On : 17 Dec 2018 21:46
 Operator : VA/AP
 Sample : J6391-17RE
 Misc : 2.75g/5mL/MSVOA-F/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 P001-SS018-0612-01RE

Quant Time: Dec 18 04:09:30 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F112618S.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 27 01:36:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.89	168	74824	50.00	ug/l	-0.02
34) 1,4-Difluorobenzene	5.62	114	121531	50.00	ug/l	-0.02
63) Chlorobenzene-d5	9.79	117	82916	50.00	ug/l	-0.02
72) 1,4-Dichlorobenzene-d4	12.56	152	25734	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	4.87	65	52508	59.57	ug/l	0.00
Spiked Amount						
			Recovery	=	119.14%	
35) Dibromofluoromethane	4.13	113	52026	53.96	ug/l	-0.02
Spiked Amount						
			Recovery	=	107.92%	
50) Toluene-d8	7.57	98	107676	37.91	ug/l	-0.02
Spiked Amount						
			Recovery	=	75.82%	
62) 4-Bromofluorobenzene	11.43	95	33891	26.26	ug/l	0.00
Spiked Amount						
			Recovery	=	52.52%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF121718\
Data File : VF061054.D
Acq On : 17 Dec 2018 21:46
Operator : VA/AP
Sample : J6391-17RE
Misc : 2.75g/5mL/MSVOA-F/SOIL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
P001-SS018-0612-01RE

Quant Time: Dec 18 04:09:30 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F112618S.M
Quant Title : SW846 8260
QLast Update : Tue Nov 27 01:36:26 2018
Response via : Initial Calibration

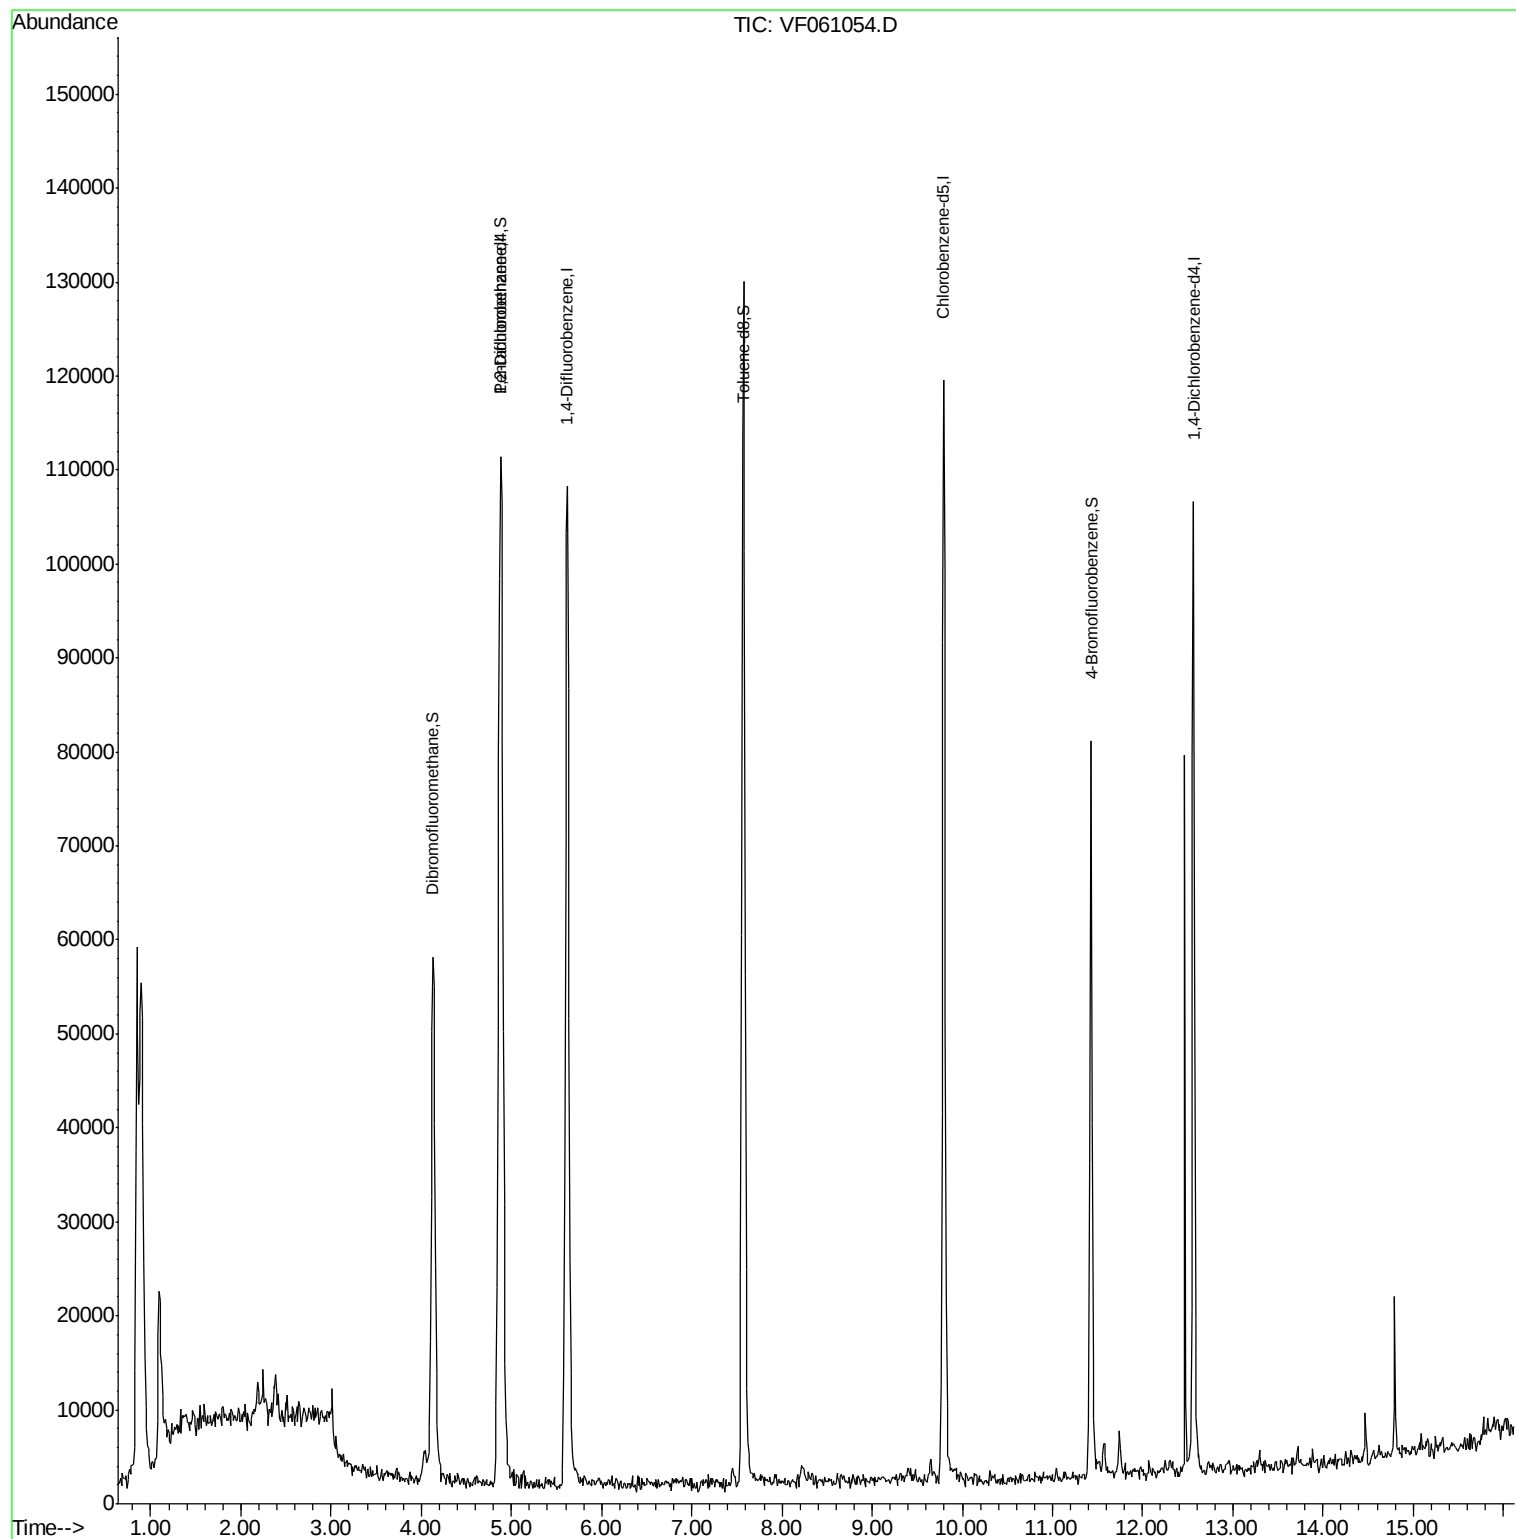

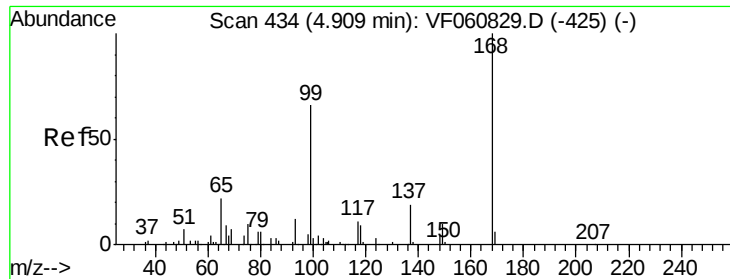

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.89 min Scan# 432

Delta R.T. -0.02 min

Lab File: VF061054.D

Acq: 17 Dec 2018 21:46

Instrument :

MSVOA_F

ClientSampleId :


P001-SS018-0612-01RE

Tot Ion:168 Resp: 74824

Ion Ratio Lower Upper

168 100

99 66.3 52.6 79.0

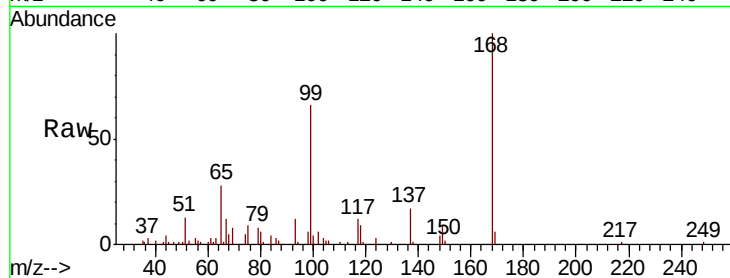

Abundance Ion 168.00 (167.70 to 168.70): VF0

Ion 99.00 (98.70 to 99.70): VF0

4.89

25000

20000



15000

10000

5000

0

Time--> 4.70 4.80 4.90 5.00

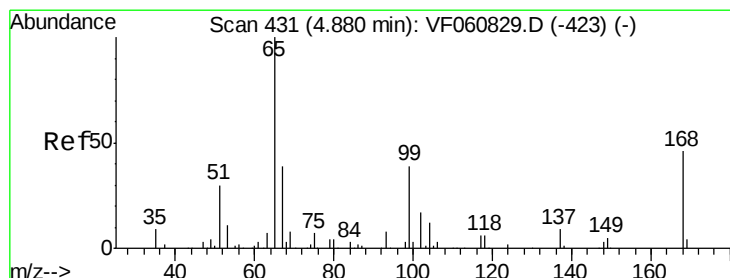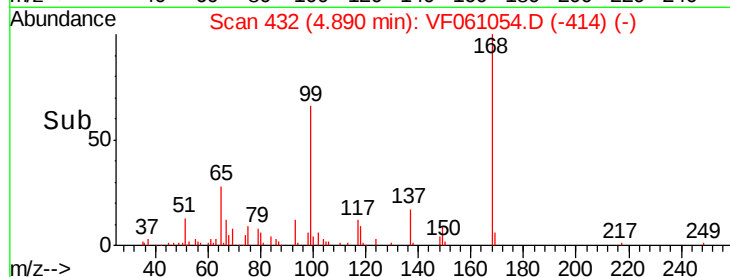

#33

1,2-Dichloroethane-d4

Concen: 59.570 ug/l

RT: 4.87 min Scan# 430

Delta R.T. -0.01 min

Lab File: VF061054.D


Acq: 17 Dec 2018 21:46

Tgt Ion: 65 Resp: 52508

Ion Ratio Lower Upper

65 100

67 46.9 0.0 96.4

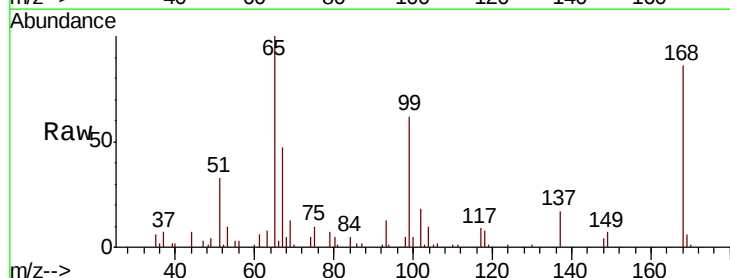

Abundance Ion 65.00 (64.70 to 65.70): VF0

Ion 67.00 (66.70 to 67.70): VF0

20000


15000


10000

5000

0

Time--> 4.70 4.80 4.90 5.00 5.10

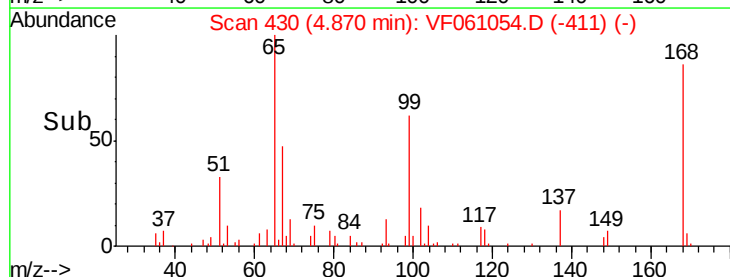

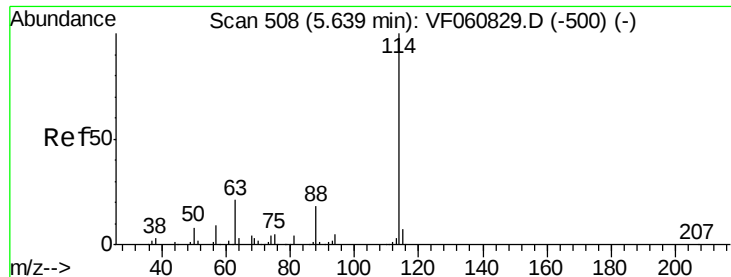

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.62 min Scan# 506

Delta R.T. -0.02 min

Lab File: VF061054.D

Acq: 17 Dec 2018 21:46

Instrument :

MSVOA_F

ClientSampleId :

P001-SS018-0612-01RE


Tot Ion:114 Resp: 121531

Ion Ratio Lower Upper

114 100

63 21.6 0.0 41.6




88 20.8 0.0 36.6

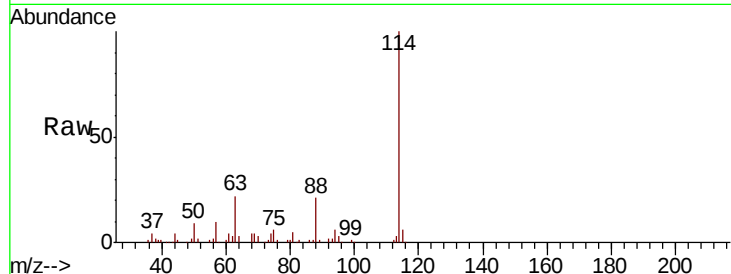

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 63.00 (62.70 to 63.70): VF0

Ion 88.00 (87.70 to 88.70): VF0

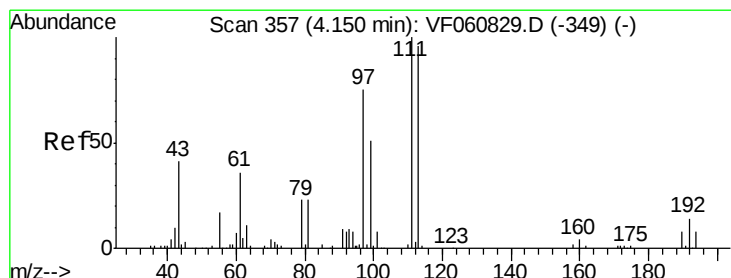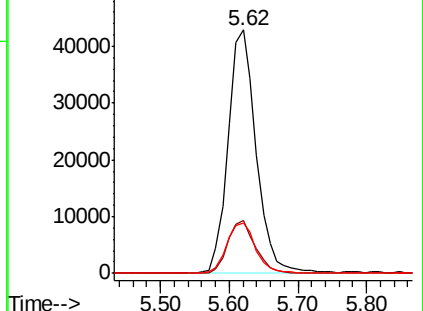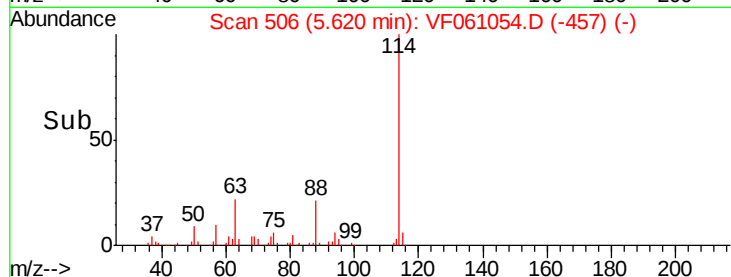

#35

Dibromofluoromethane

Concen: 53.961 ug/l

RT: 4.13 min Scan# 355

Delta R.T. -0.02 min

Lab File: VF061054.D

Acq: 17 Dec 2018 21:46


Tgt Ion:113 Resp: 52026

Ion Ratio Lower Upper

113 100

111 101.4 83.0 124.6



192 14.3 12.3 18.5

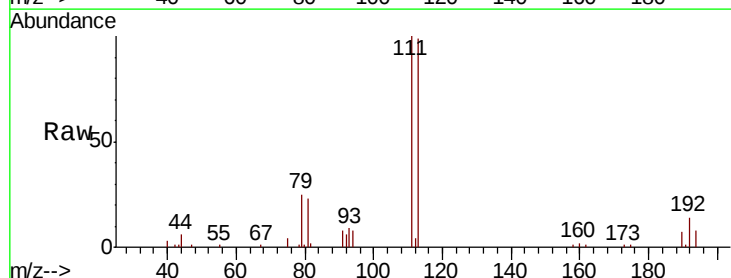


Abundance Ion 113.00 (112.70 to 113.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 192.00 (191.70 to 192.70): V



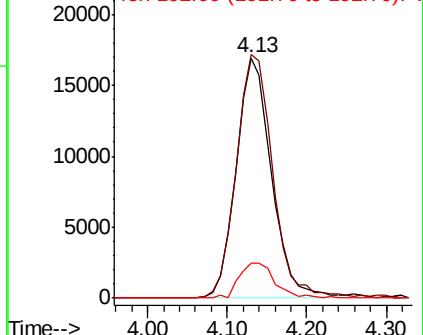
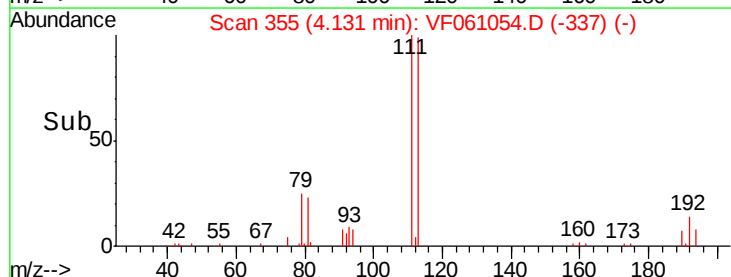


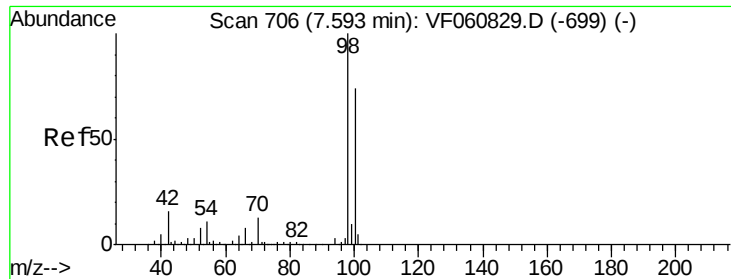

#50
Toluene-d8
Concen: 37.913 ug/l
RT: 7.57 min Scan# 704
Delta R.T. -0.02 min
Lab File: VF061054.D
Acq: 17 Dec 2018 21:46




Instrument :
MSVOA_F
ClientSampleId :
P001-SS018-0612-01RE


Tot Ion: 98 Resp: 107676
Ion Ratio Lower Upper
98 100
100 68.4 59.3 88.9

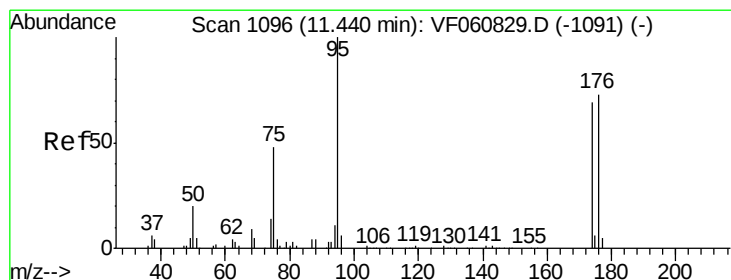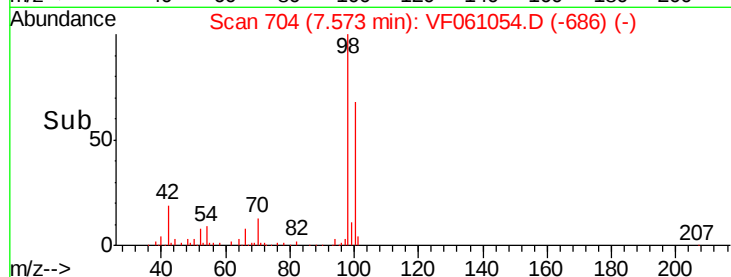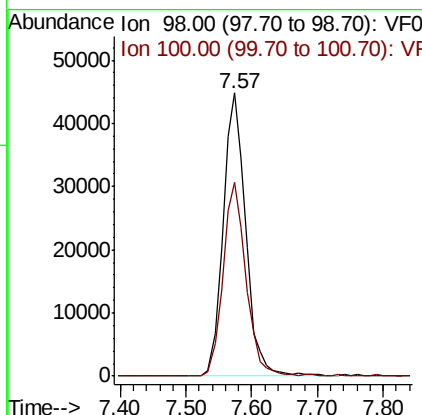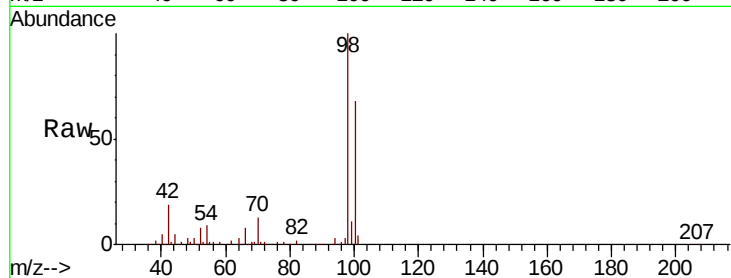

#62
4-Bromofluorobenzene
Concen: 26.257 ug/l
RT: 11.43 min Scan# 1095
Delta R.T. -0.01 min
Lab File: VF061054.D
Acq: 17 Dec 2018 21:46

Tgt Ion: 95 Resp: 33891
Ion Ratio Lower Upper
95 100
174 78.8 0.0 138.2
176 68.5 0.0 146.2

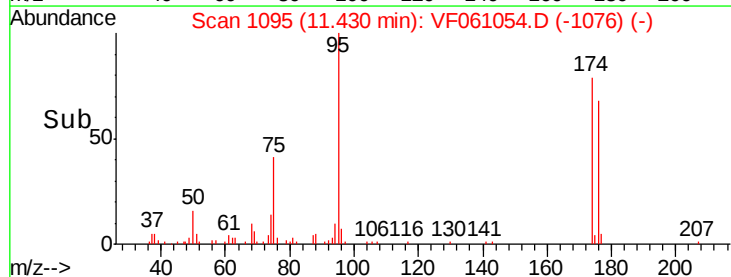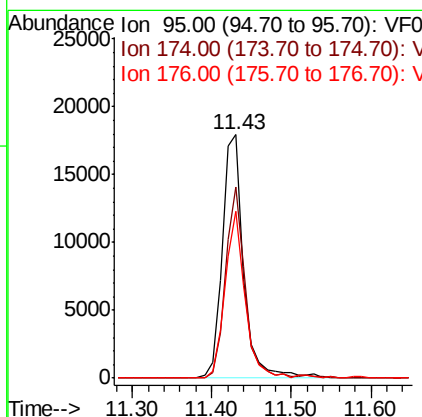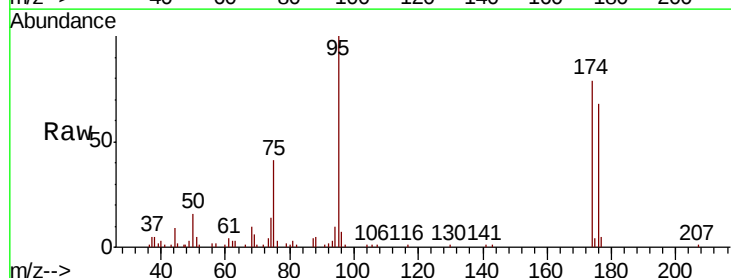


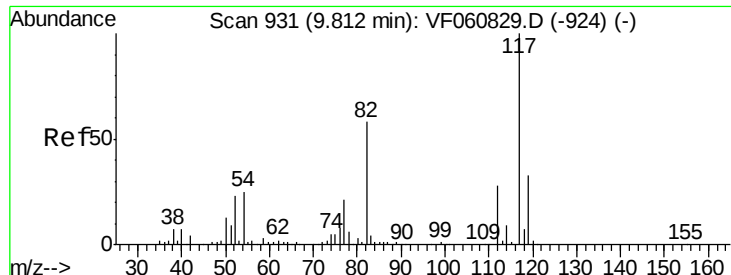




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.79 min Scan# 929
Delta R.T. -0.02 min
Lab File: VF061054.D
Acq: 17 Dec 2018 21:46

Instrument :
MSVOA_F
ClientSampleId :
P001-SS018-0612-01RE

Tot Ion:117 Resp: 82916
Ion Ratio Lower Upper
117 100
82 61.8 46.6 69.8
119 29.5 26.4 39.6

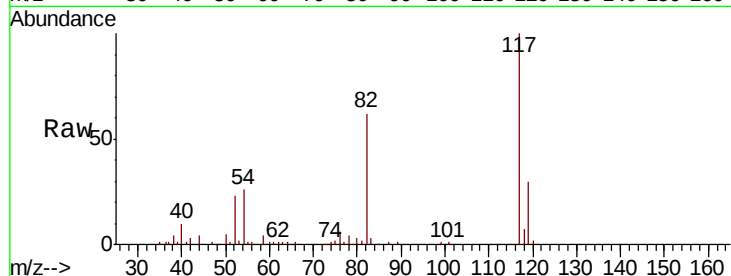


Abundance Ion 117.00 (116.70 to 117.70): V
Ion 82.00 (81.70 to 82.70): VF0
Ion 119.00 (118.70 to 119.70): V

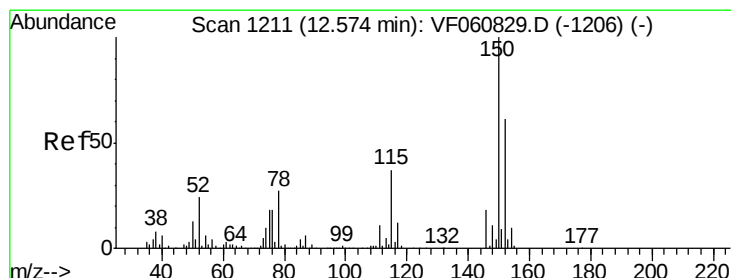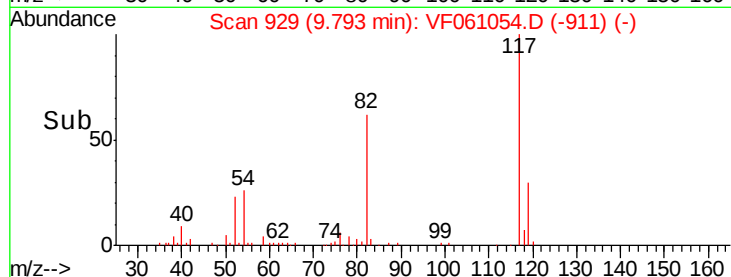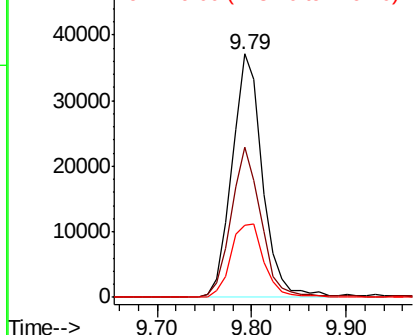

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.56 min Scan# 1210
Delta R.T. -0.01 min
Lab File: VF061054.D
Acq: 17 Dec 2018 21:46

Tgt Ion:152 Resp: 25734
Ion Ratio Lower Upper
152 100
115 54.6 30.1 90.5
150 152.6 0.0 327.6

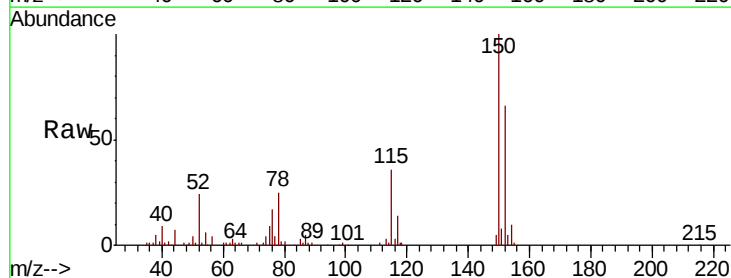

Abundance Ion 152.00 (151.70 to 152.70): V
Ion 115.00 (114.70 to 115.70): V
Ion 150.00 (149.70 to 150.70): V

