


Data Path : Z:\voasrv\HPCHEM1\MSVOA_F\Data\VF121918\
Data File : VF061067.D
Acq On : 18 Dec 2018 17:21
Operator : VA/AP
Sample : BFB
Misc : 5.00G/5mL/MSVOA-F/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F121918S.M
Title : SW846 8260
Last Update : Thu Dec 20 00:56:59 2018

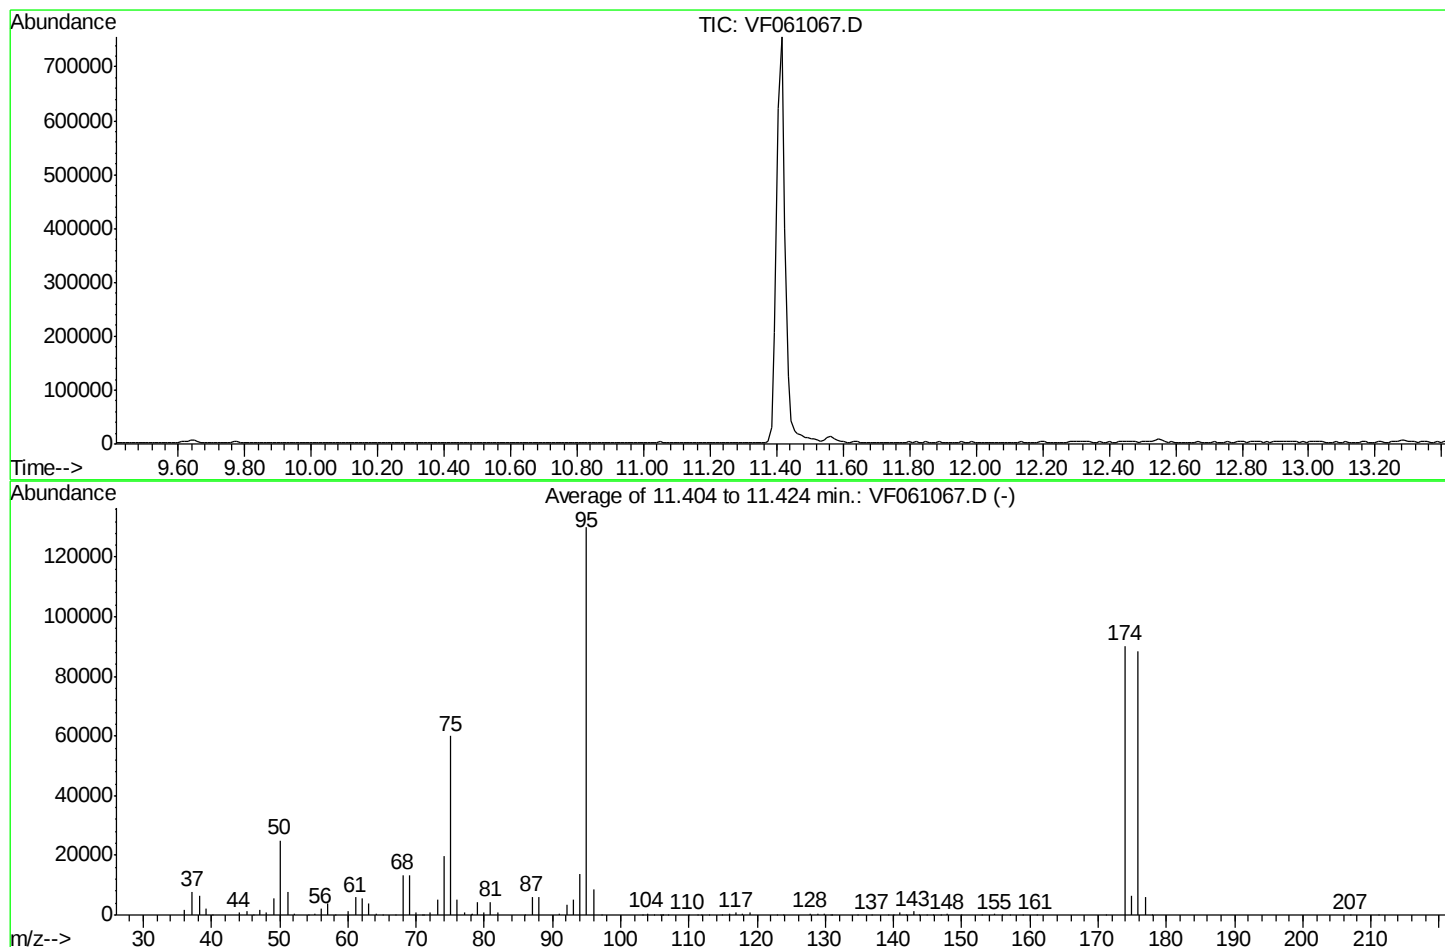

AutoFind: Scans 1092, 1093, 1094; Background Corrected with Scan 1086

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	24906	PASS
75	95	30	60	46.1	59981	PASS
95	95	100	100	100.0	130013	PASS
96	95	5	9	6.7	8748	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.4	90288	PASS
175	174	5	9	7.1	6436	PASS
176	174	95	101	98.2	88656	PASS
177	176	5	9	6.8	6052	PASS