


Data Path : Z:\voasrv\HPCHEM1\MSVOA_F\Data\VF121918\
 Data File : VF061076.D
 Acq On : 19 Dec 2018 9:51
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F121918S.M
 Title : SW846 8260
 Last Update : Thu Dec 20 00:56:59 2018

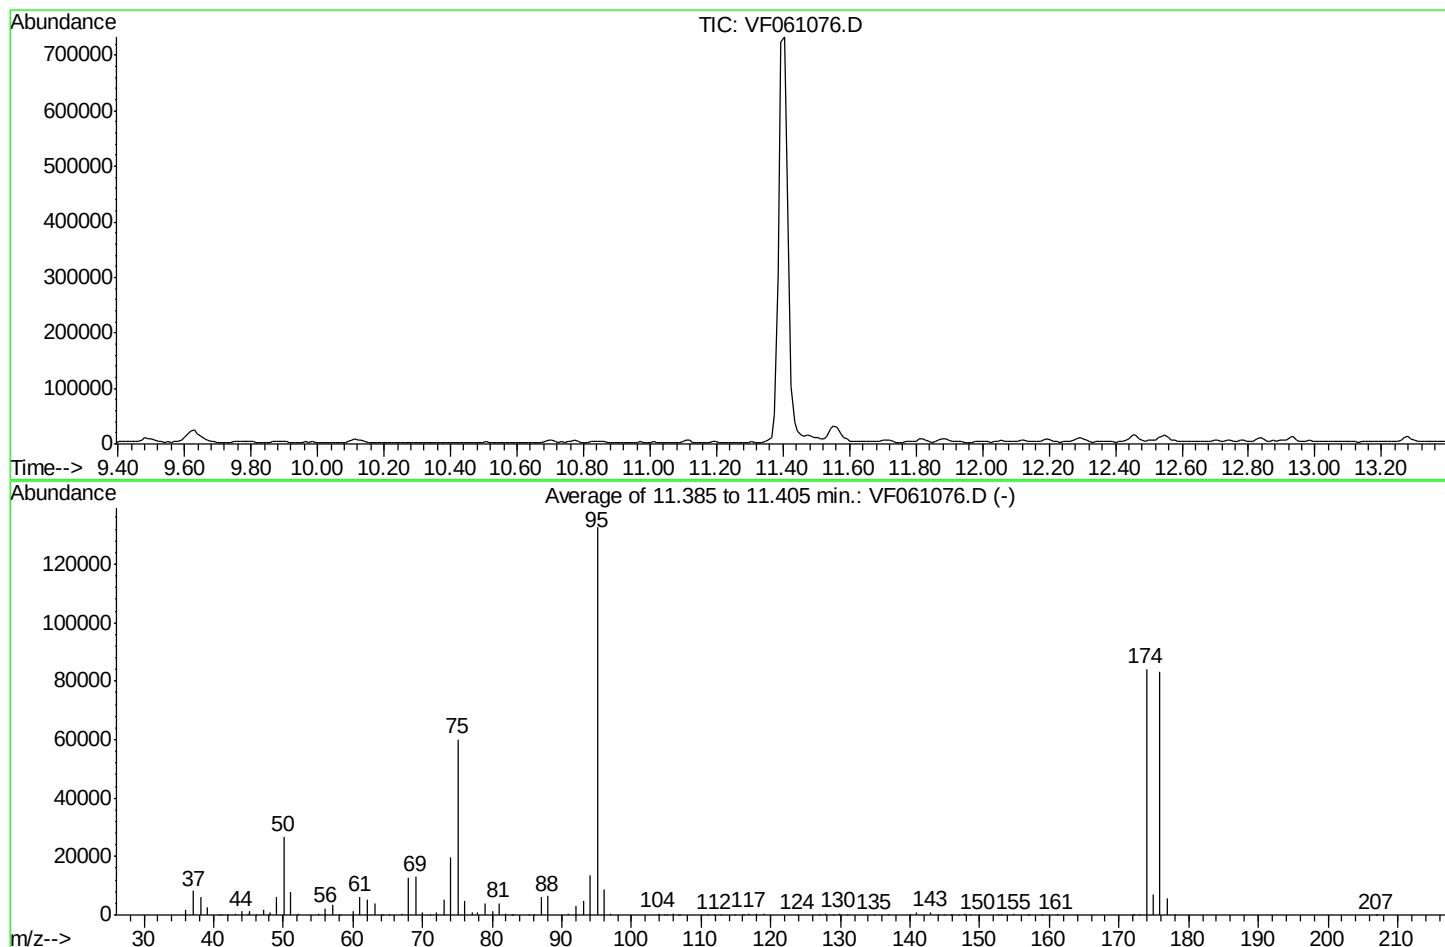

AutoFind: Scans 1090, 1091, 1092; Background Corrected with Scan 1085

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	26722	PASS
75	95	30	60	45.3	60090	PASS
95	95	100	100	100.0	132616	PASS
96	95	5	9	6.7	8896	PASS
173	174	0.00	2	0.3	236	PASS
174	95	50	100	63.4	84093	PASS
175	174	5	9	8.1	6821	PASS
176	174	95	101	99.2	83416	PASS
177	176	5	9	7.0	5875	PASS