


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF122018\
Data File : VF061099.D
Acq On : 20 Dec 2018 9:47
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F121918S.M
Title : SW846 8260
Last Update : Thu Dec 20 00:56:59 2018

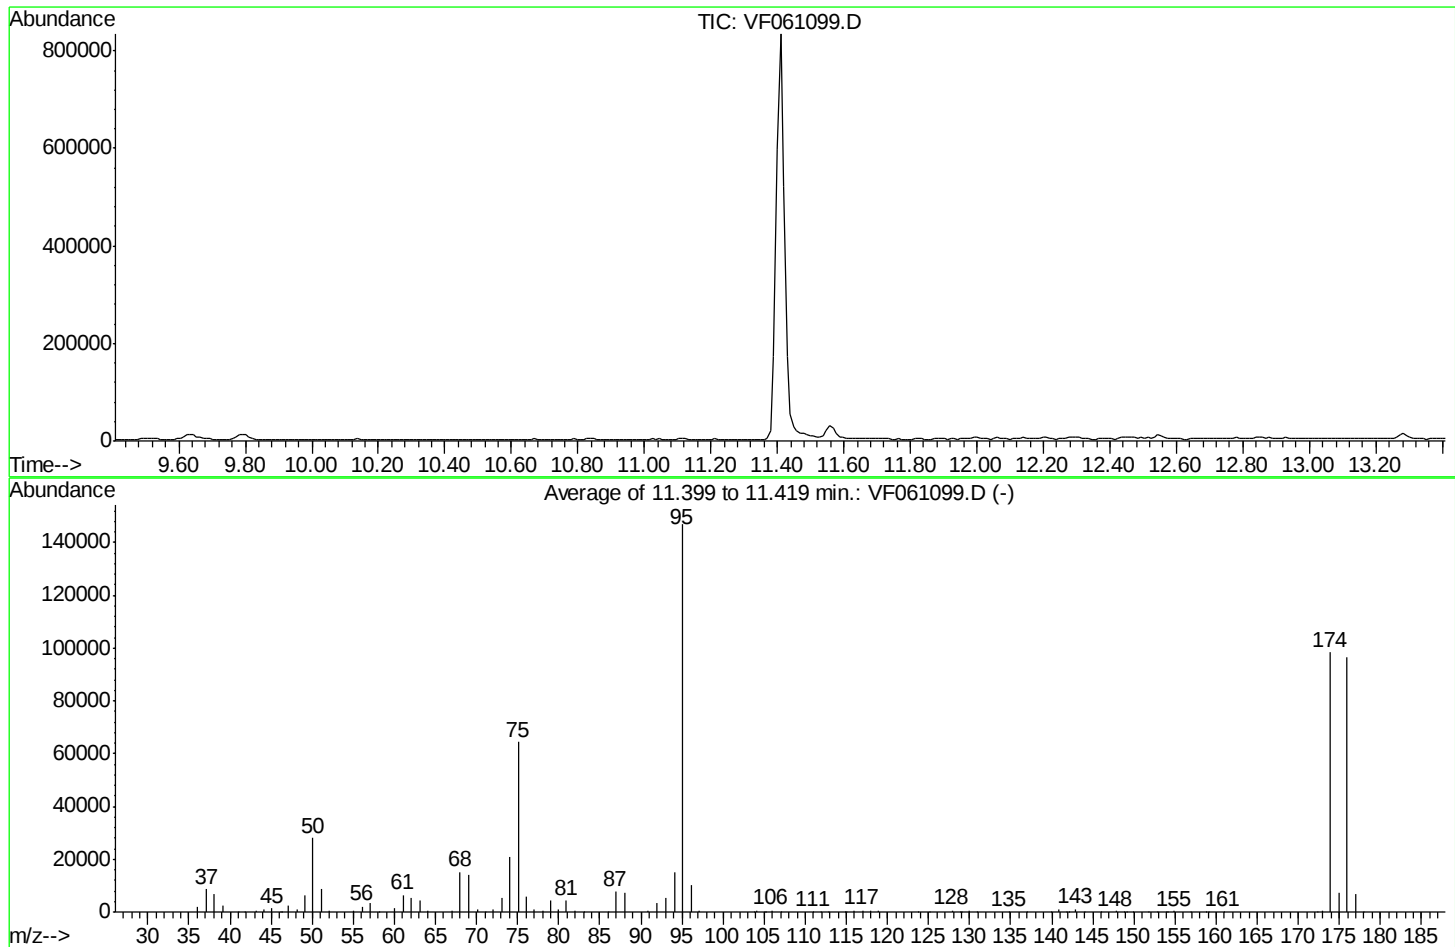

AutoFind: Scans 1092, 1093, 1094; Background Corrected with Scan 1086

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	28069	PASS
75	95	30	60	43.9	64453	PASS
95	95	100	100	100.0	146842	PASS
96	95	5	9	6.8	9992	PASS
173	174	0.00	2	0.4	410	PASS
174	95	50	100	67.0	98386	PASS
175	174	5	9	7.6	7520	PASS
176	174	95	101	97.9	96344	PASS
177	176	5	9	6.9	6631	PASS