


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_F\DATA\VF122218\
Data File : VF061139.D
Acq On : 22 Dec 2018 12:15
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F121918S.M
Title : SW846 8260
Last Update : Thu Dec 20 00:56:59 2018

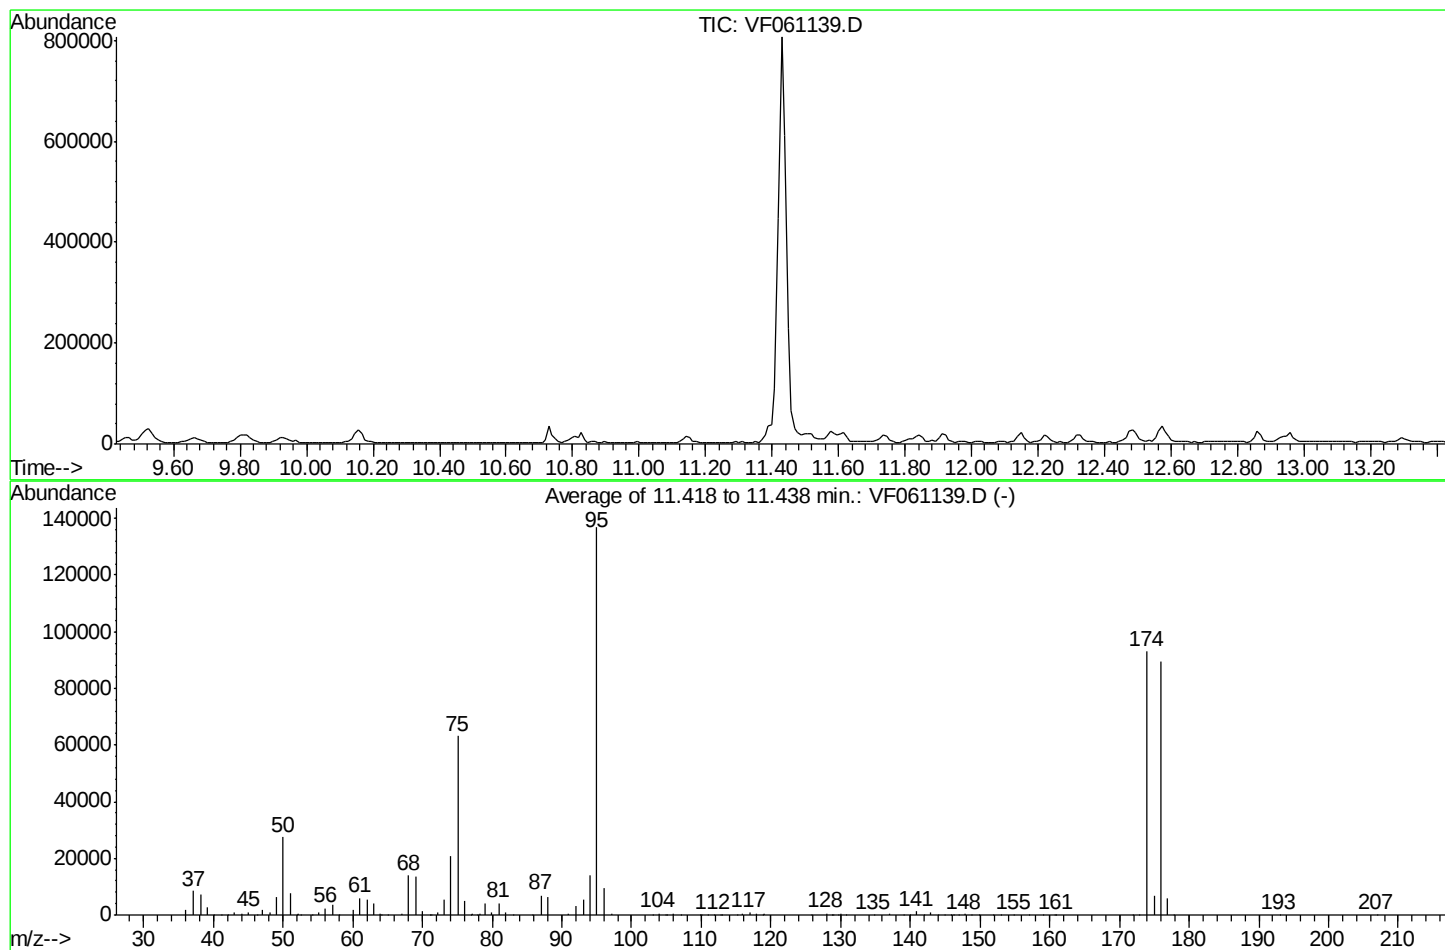

AutoFind: Scans 1094, 1095, 1096; Background Corrected with Scan 1088

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	27448	PASS
75	95	30	60	46.1	63128	PASS
95	95	100	100	100.0	136864	PASS
96	95	5	9	7.0	9562	PASS
173	174	0.00	2	0.1	123	PASS
174	95	50	100	68.0	93018	PASS
175	174	5	9	7.4	6863	PASS
176	174	95	101	96.4	89674	PASS
177	176	5	9	6.6	5957	PASS