


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF122418\
 Data File : VF061156.D
 Acq On : 24 Dec 2018 9:52
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F121918S.M
 Title : SW846 8260
 Last Update : Thu Dec 20 00:56:59 2018

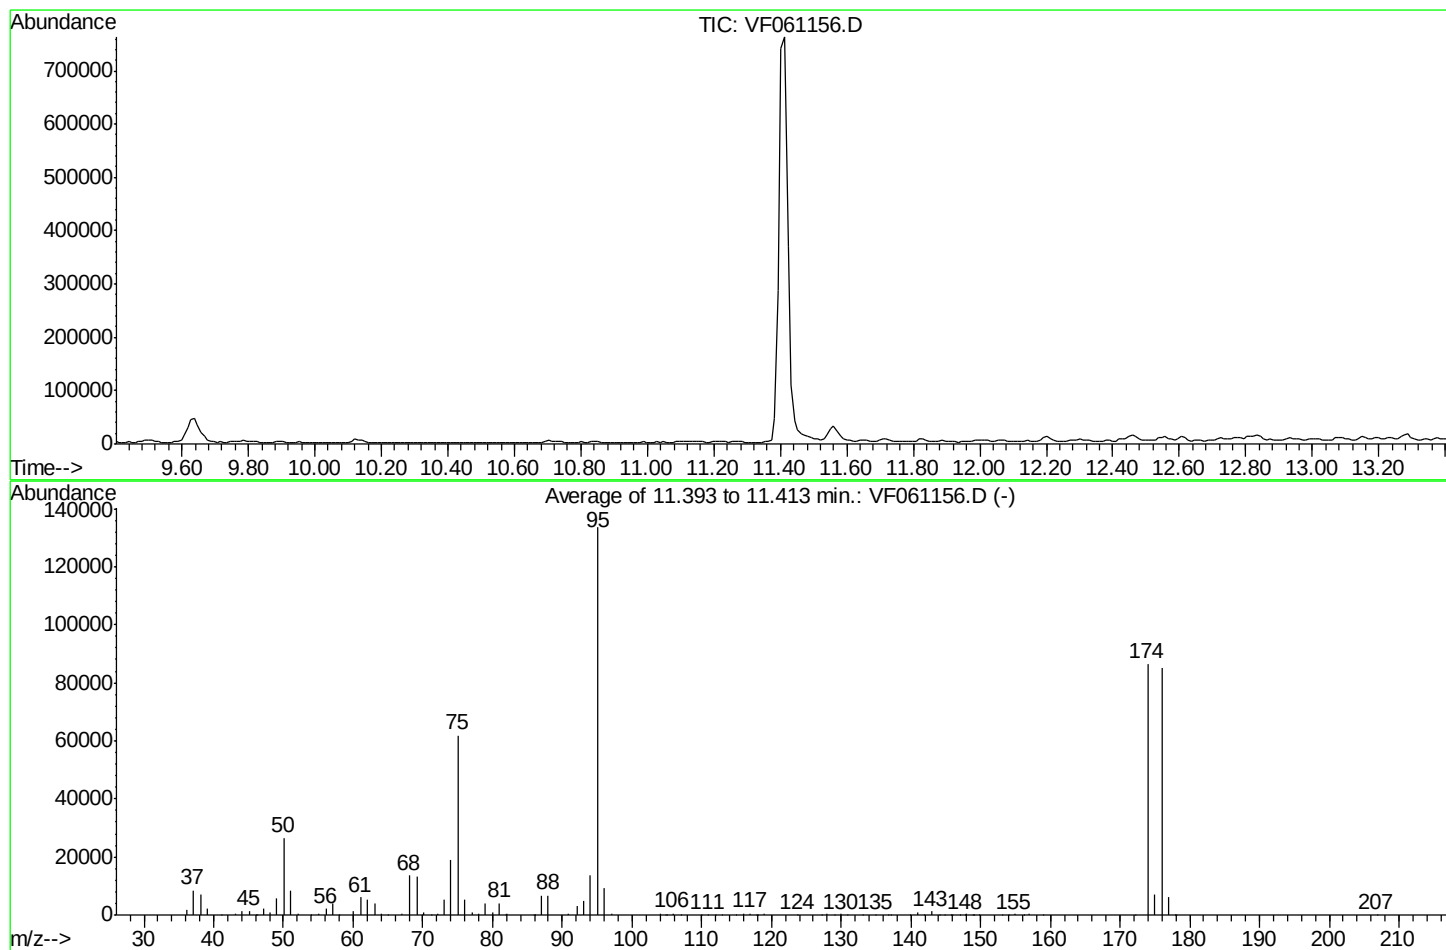

AutoFind: Scans 1091, 1092, 1093; Background Corrected with Scan 1086

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	26668	PASS
75	95	30	60	46.3	61858	PASS
95	95	100	100	100.0	133557	PASS
96	95	5	9	6.9	9231	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	64.7	86450	PASS
175	174	5	9	8.1	6992	PASS
176	174	95	101	98.4	85048	PASS
177	176	5	9	7.2	6138	PASS