


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF122618\  
Data File : VF061179.D  
Acq On : 26 Dec 2018 9:49  
Operator : VA/AP  
Sample : BFB  
Misc : 5.00µ/5mL/MSVOA-F/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_F  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA\_F\METHODS\82F121918S.M  
Title : SW846 8260  
Last Update : Thu Dec 20 00:56:59 2018

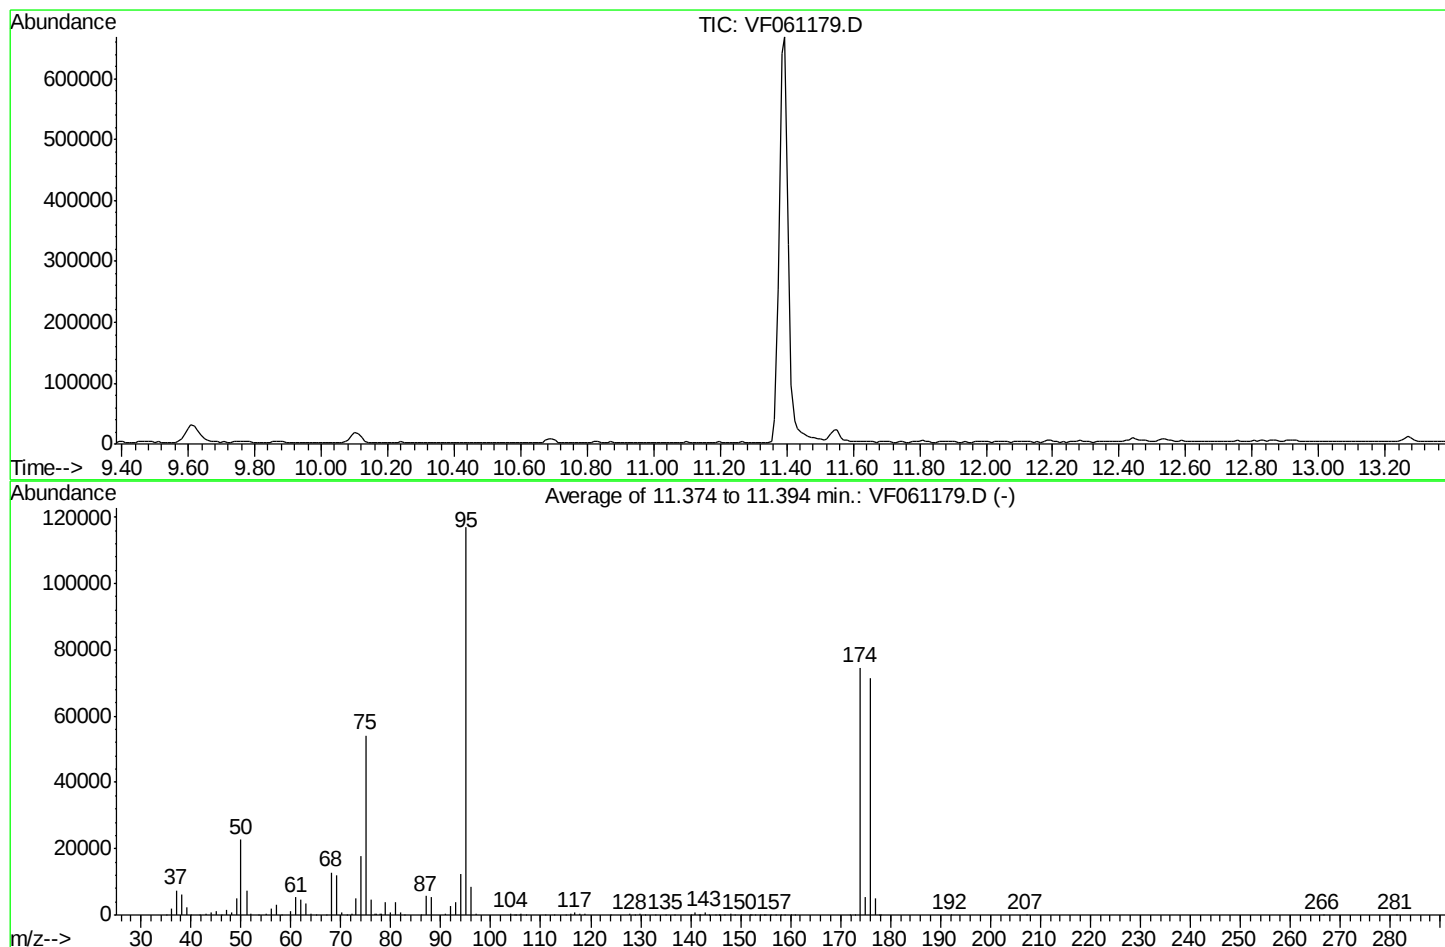

AutoFind: Scans 1089, 1090, 1091; Background Corrected with Scan 1084

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.5      | 22756   | PASS             |
| 75          | 95           | 30           | 60           | 46.3      | 54186   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 116960  | PASS             |
| 96          | 95           | 5            | 9            | 7.2       | 8391    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.1       | 73      | PASS             |
| 174         | 95           | 50           | 100          | 63.9      | 74685   | PASS             |
| 175         | 174          | 5            | 9            | 7.4       | 5511    | PASS             |
| 176         | 174          | 95           | 101          | 95.5      | 71328   | PASS             |
| 177         | 176          | 5            | 9            | 7.0       | 4968    | PASS             |