


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF122718\
Data File : VF061201.D
Acq On : 27 Dec 2018 11:31
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F121918S.M
Title : SW846 8260
Last Update : Thu Dec 20 00:56:59 2018

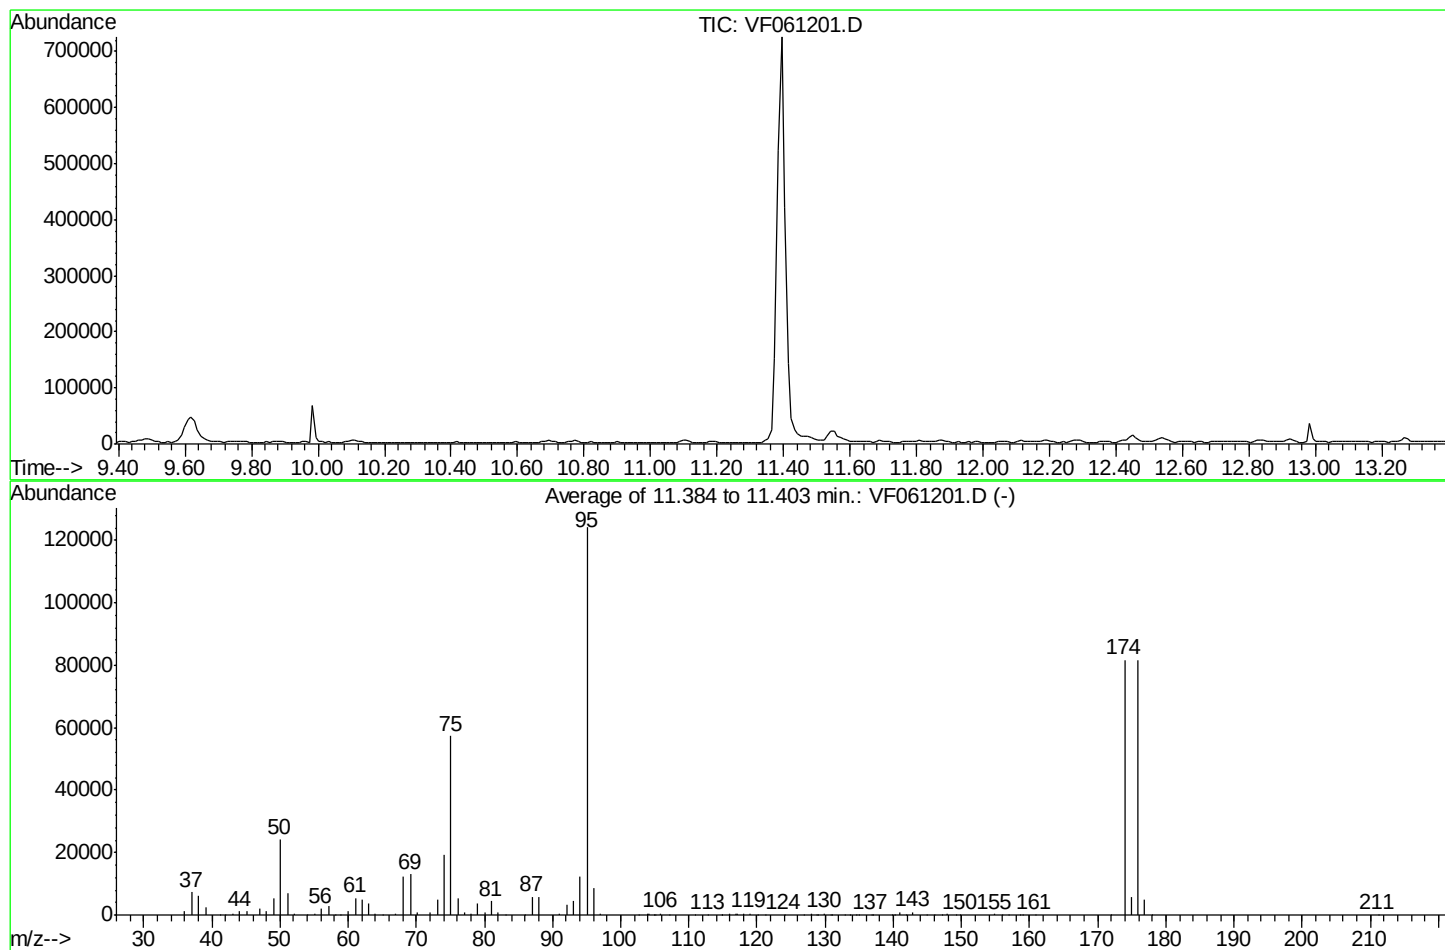

AutoFind: Scans 1090, 1091, 1092; Background Corrected with Scan 1084

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	24151	PASS
75	95	30	60	46.1	57309	PASS
95	95	100	100	100.0	124184	PASS
96	95	5	9	6.9	8587	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	65.8	81765	PASS
175	174	5	9	7.1	5817	PASS
176	174	95	101	99.6	81434	PASS
177	176	5	9	6.0	4918	PASS