


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_F\DATA\VF122818\
 Data File : VF061224.D
 Acq On : 28 Dec 2018 7:57
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F121918S.M
 Title : SW846 8260
 Last Update : Thu Dec 20 00:56:59 2018

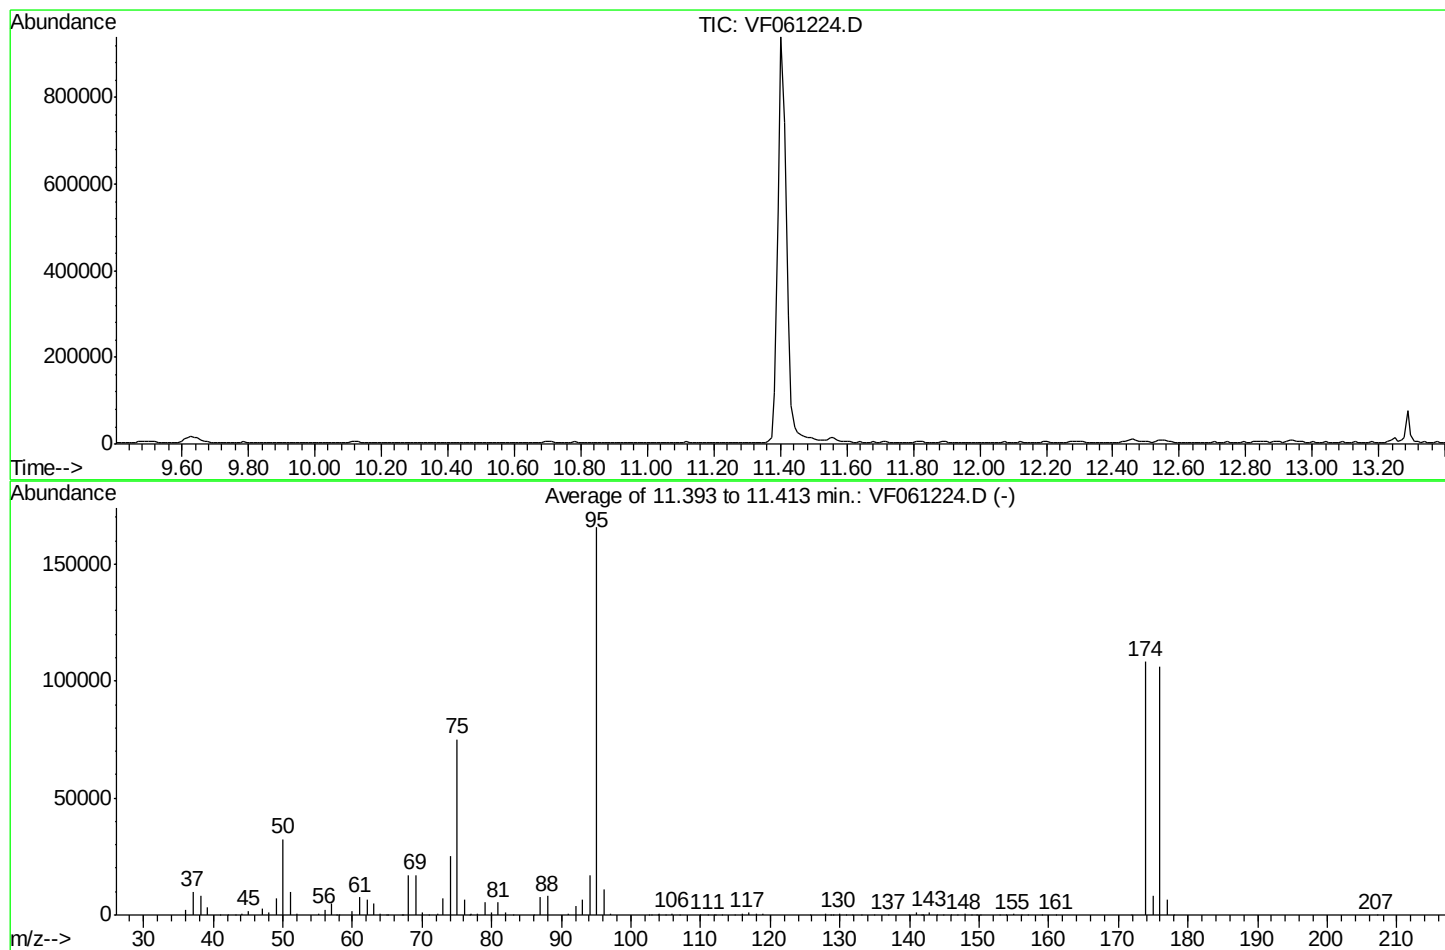

AutoFind: Scans 1091, 1092, 1093; Background Corrected with Scan 1086

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	32360	PASS
75	95	30	60	45.4	75170	PASS
95	95	100	100	100.0	165730	PASS
96	95	5	9	6.5	10843	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	65.3	108224	PASS
175	174	5	9	7.7	8304	PASS
176	174	95	101	98.2	106282	PASS
177	176	5	9	6.2	6606	PASS