


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF010919\
 Data File : VF061314.D
 Acq On : 9 Jan 2019 22:25
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F010819S.M
 Title : SW846 8260
 Last Update : Wed Jan 09 07:13:51 2019

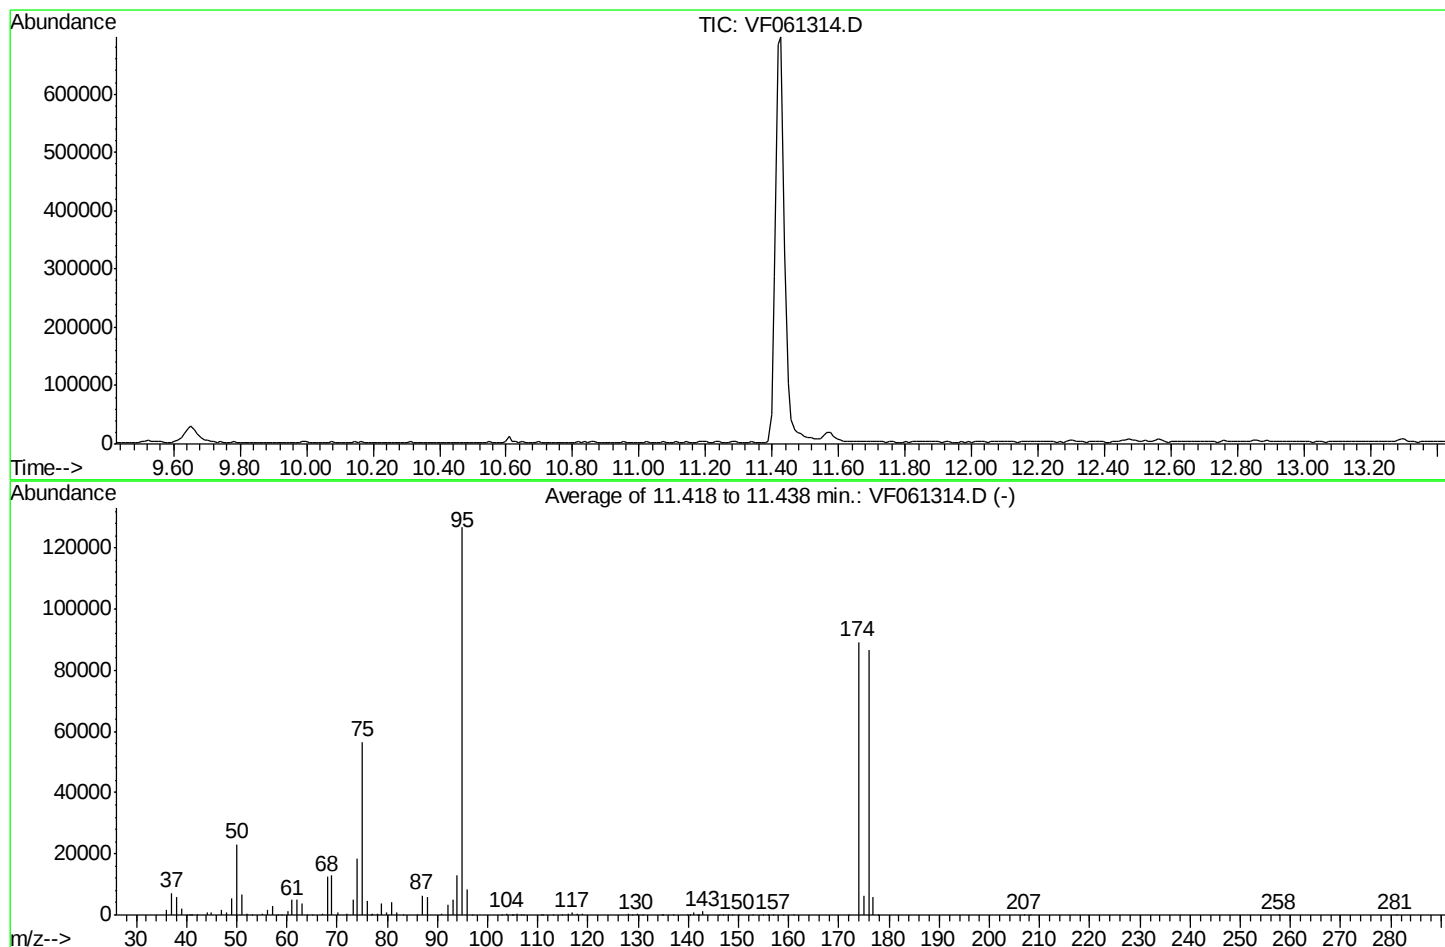

AutoFind: Scans 1094, 1095, 1096; Background Corrected with Scan 1088

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	23200	PASS
75	95	30	60	44.7	56669	PASS
95	95	100	100	100.0	126725	PASS
96	95	5	9	6.6	8410	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.3	89149	PASS
175	174	5	9	7.3	6496	PASS
176	174	95	101	97.4	86802	PASS
177	176	5	9	6.6	5735	PASS