


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF021819\
 Data File : VF061669.D
 Acq On : 18 Feb 2019 9:38
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F021319S.M
 Title : SW846 8260
 Last Update : Thu Feb 14 03:27:56 2019

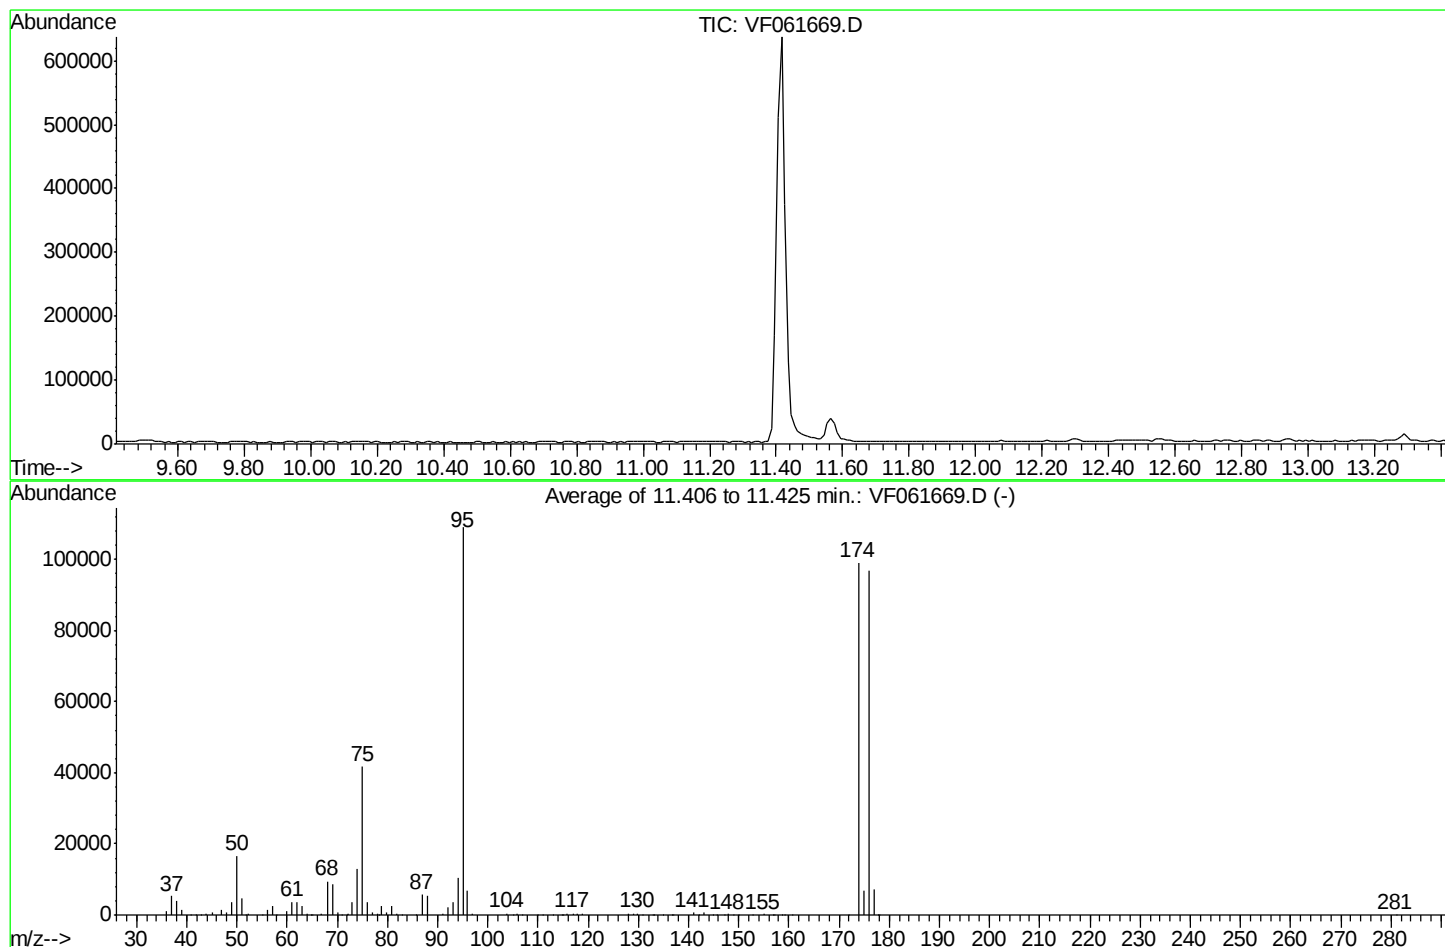

AutoFind: Scans 1093, 1094, 1095; Background Corrected with Scan 1087

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	16620	PASS
75	95	30	60	38.3	41722	PASS
95	95	100	100	100.0	109037	PASS
96	95	5	9	6.1	6690	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.9	99112	PASS
175	174	5	9	6.9	6793	PASS
176	174	95	101	97.9	97005	PASS
177	176	5	9	7.3	7053	PASS