

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_F\DATA\VF031219\
 Data File : VF061916.D
 Acq On : 12 Mar 2019 20:30
 Operator : VA/AP
 Sample : K1866-11
 Misc : 6.52g/5mL/MSVOA-F/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 MR-MH-14-COMP

Manual Integrations
 APPROVED

MMDadoda
 3/13/2019 4:41:51 PM

Quant Time: Mar 13 03:14:49 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F030419S.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 05 04:50:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.86	168	277525	50.00	ug/l	-0.02
34) 1,4-Difluorobenzene	5.58	114	457006	50.00	ug/l	-0.03
63) Chlorobenzene-d5	9.76	117	382895	50.00	ug/l	-0.02
72) 1,4-Dichlorobenzene-d4	12.54	152	221615	50.00	ug/l	-0.01
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	4.83	65	120294	59.52	ug/l	-0.02
Spiked Amount 50.000			Recovery	=	119.04%	
35) Dibromofluoromethane	4.10	113	166162	52.10	ug/l	-0.02
Spiked Amount 50.000			Recovery	=	104.20%	
50) Toluene-d8	7.54	98	424801	44.81	ug/l	-0.02
Spiked Amount 50.000			Recovery	=	89.62%	
62) 4-Bromofluorobenzene	11.40	95	196874	53.02	ug/l	-0.02
Spiked Amount 50.000			Recovery	=	106.04%	
Target Compounds						
20) Methylene Chloride	2.17	84	18934m	3.113	ug/l	Qvalue
52) Toluene	7.61	92	8748	1.310	ug/l	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_F\DATA\VF031219\
Data File : VF061916.D
Acq On : 12 Mar 2019 20:30
Operator : VA/AP
Sample : K1866-11
Misc : 6.52g/5mL/MSVOA-F/SOIL
ALS Vial : 14 Sample Multiplier: 1


Instrument :
MSVOA_F
ClientSampleId :
MR-MH-14-COMP

Manual Integrations
APPROVED

MMDadoda
3/13/2019 4:41:51 PM

Quant Time: Mar 13 03:14:49 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F030419S.M
Quant Title : SW846 8260
QLast Update : Tue Mar 05 04:50:44 2019
Response via : Initial Calibration

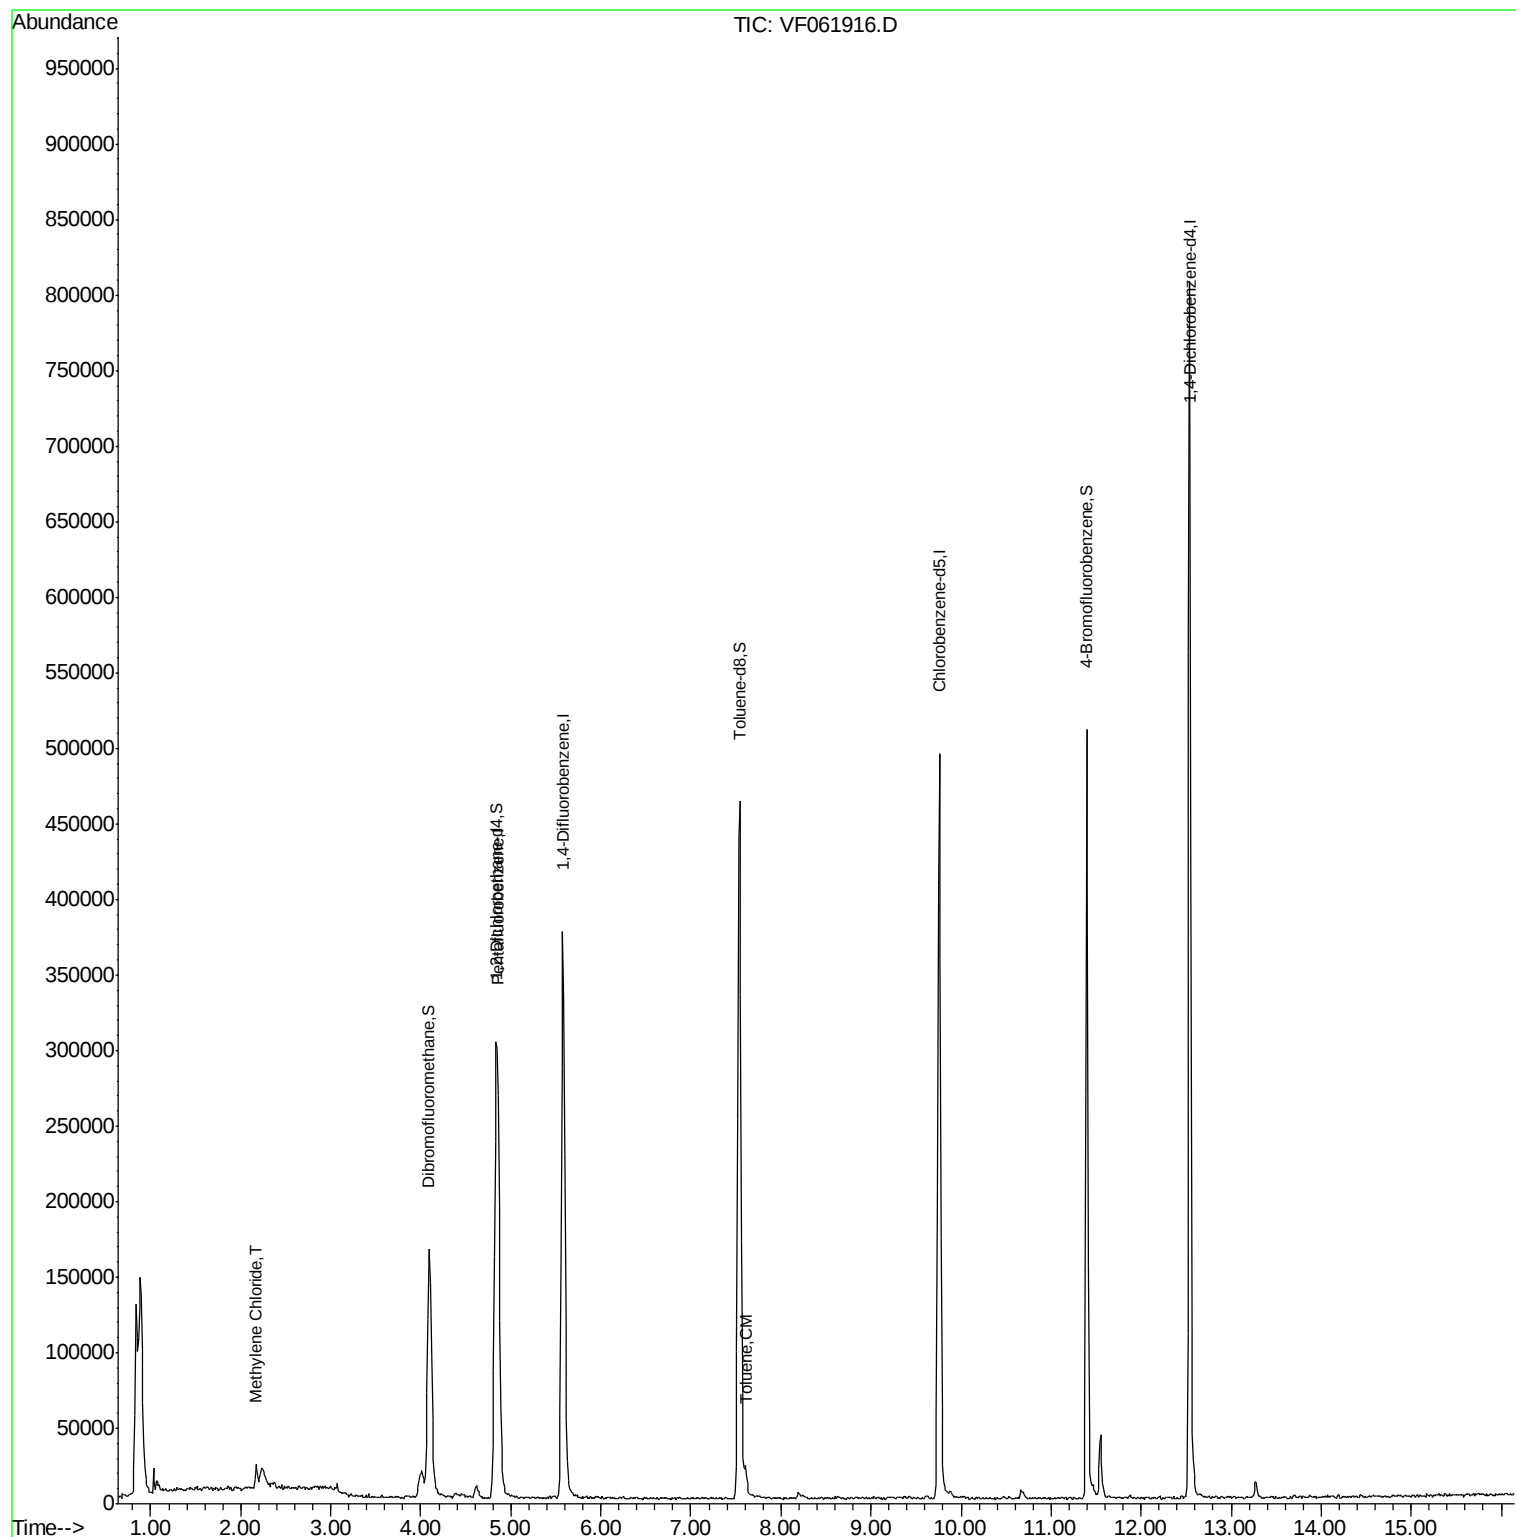

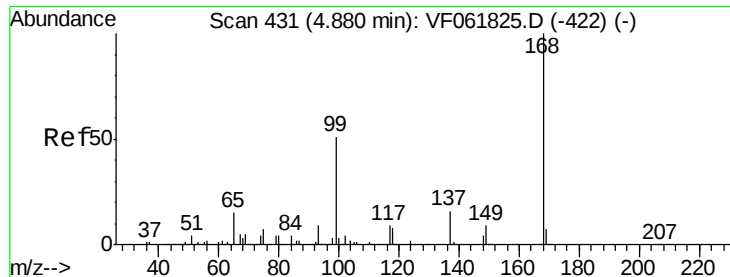

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.86 min Scan# 429

Delta R.T. -0.02 min

Lab File: VF061916.D

Acq: 12 Mar 2019 20:30

Instrument :

MSVOA_F

ClientSampleId :

MR-MH-14-COMP

Tgt Ion:168 Resp: 277525

Ion Ratio Lower Upper

168 100


99 50.1 40.8 61.2

Manual Integrations

APPROVED




MMDadoda

3/13/2019 4:41:51 PM

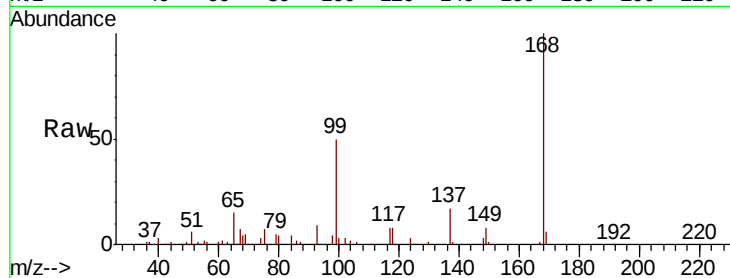

Abundance Ion 168.00 (167.70 to 168.70): V

Ion 99.00 (98.70 to 99.70): VF0

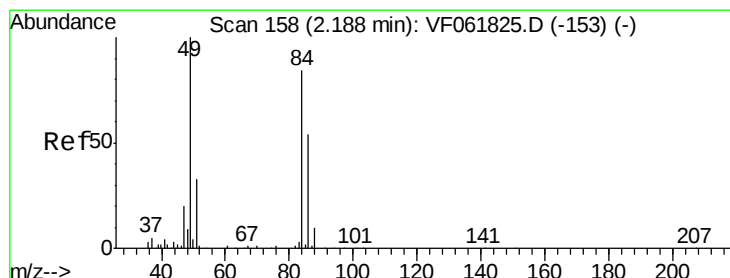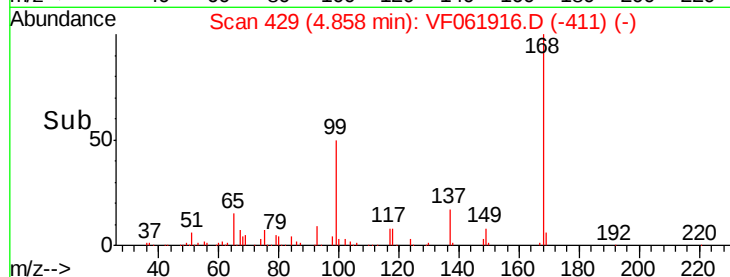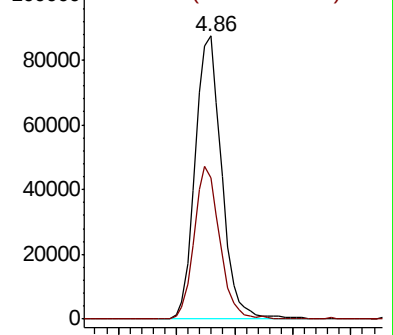

#20

Methylene Chloride

Concen: 3.113 ug/l m

RT: 2.17 min Scan# 156

Delta R.T. -0.02 min

Lab File: VF061916.D

Acq: 12 Mar 2019 20:30

Tgt Ion: 84 Resp: 18934

Ion Ratio Lower Upper

84 100

49 116.1 96.8 145.2

51 35.4 31.8 47.6




86 59.0 51.6 77.4


Abundance Ion 84.00 (83.70 to 84.70): VF0

Ion 49.00 (48.70 to 49.70): VF0

Ion 51.00 (50.70 to 51.70): VF0

Ion 86.00 (85.70 to 86.70): VF0

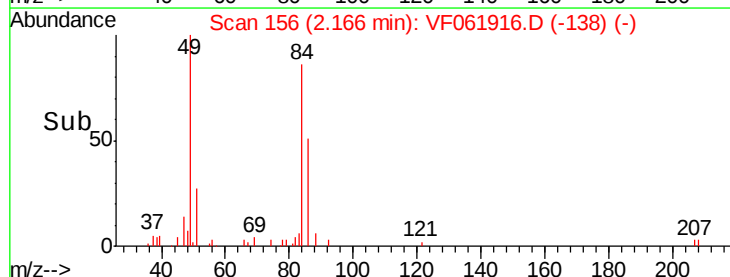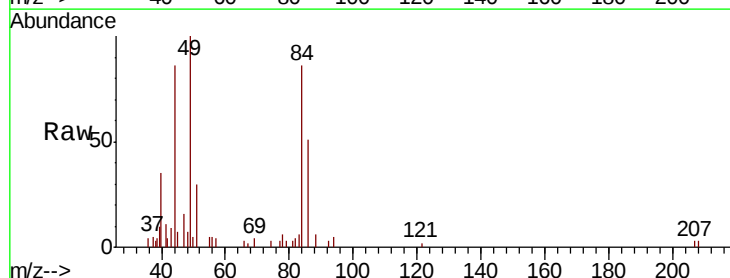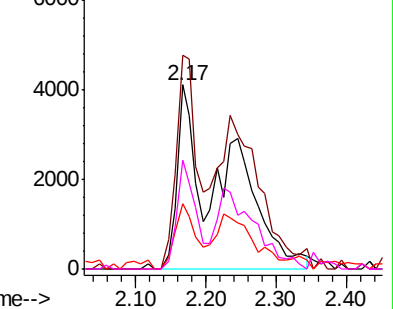

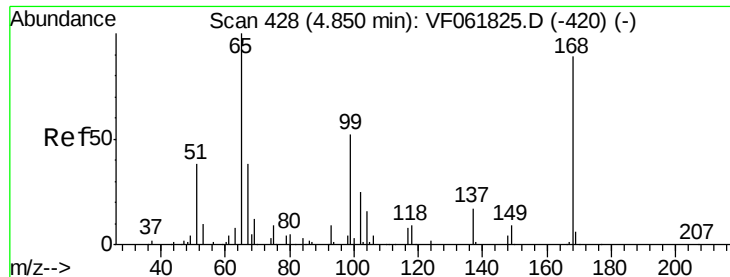





#33
 1,2-Dichloroethane-d4
 Concen: 59.520 ug/l
 RT: 4.83 min Scan# 426
 Delta R.T. -0.02 min
 Lab File: VF061916.D
 Acq: 12 Mar 2019 20:30

Instrument :
 MSVOA_F
 ClientSampleId :
 MR-MH-14-COMP

Tgt Ion	Ratio	Resp	Lower	Upper
65	100	120294		
67	54.4	0.0	108.6	




Manual Integrations
 APPROVED


MMDadoda
 3/13/2019 4:41:51 PM

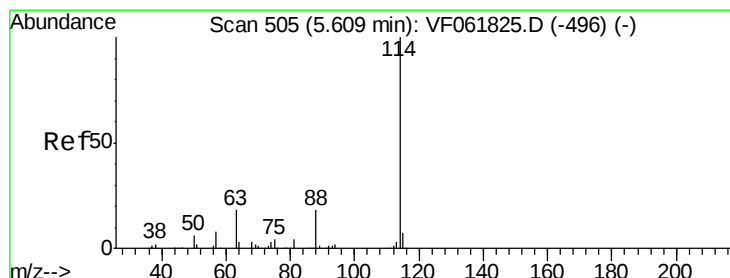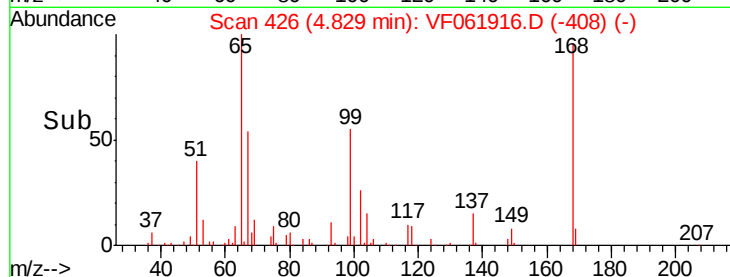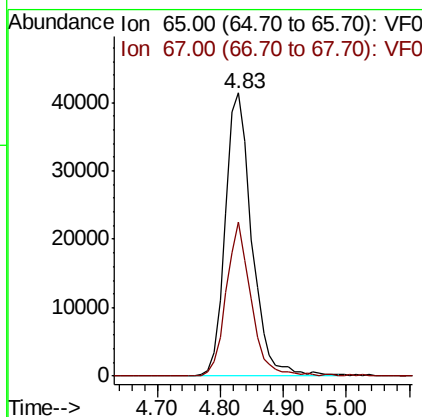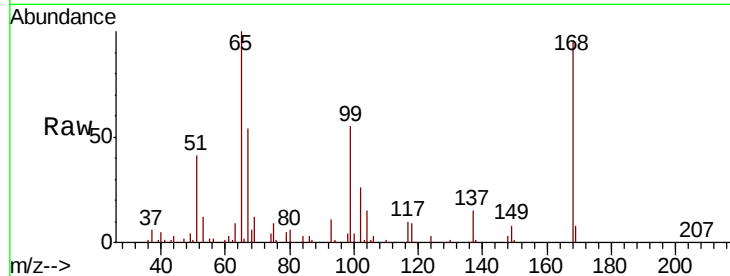

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.58 min Scan# 502
 Delta R.T. -0.03 min
 Lab File: VF061916.D
 Acq: 12 Mar 2019 20:30

Tgt Ion	Ratio	Resp	Lower	Upper
114	100	457006		
63	18.0	0.0	35.6	
88	17.5	0.0	35.6	

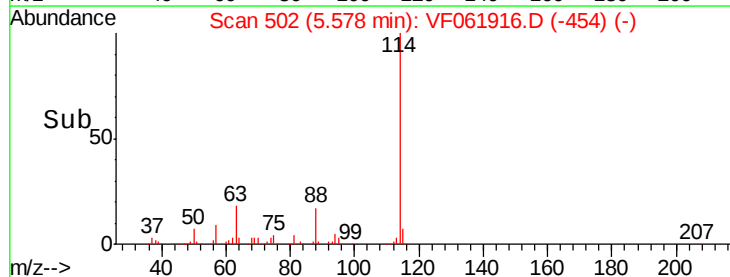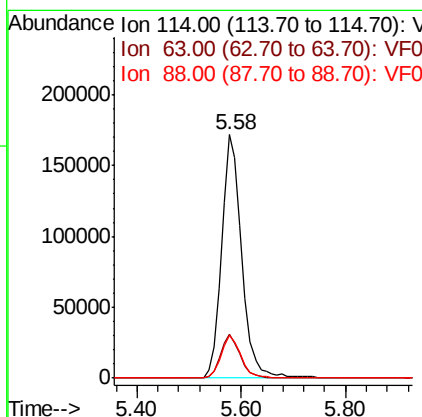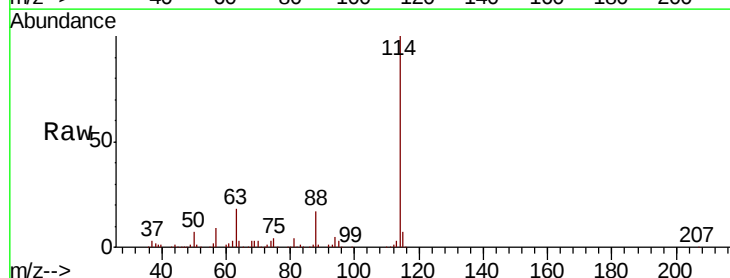

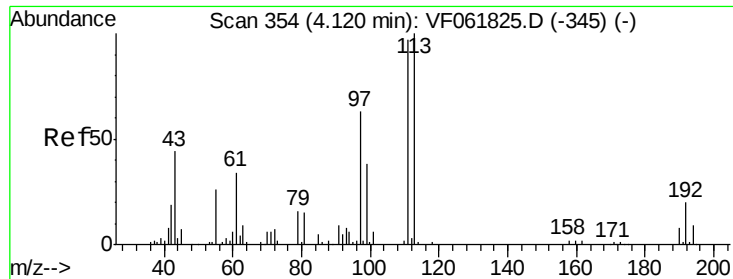





#35
Dibromofluoromethane
Concen: 52.100 ug/l
RT: 4.10 min Scan# 352
Delta R.T. -0.02 min
Lab File: VF061916.D
Acq: 12 Mar 2019 20:30

Instrument :
MSVOA_F
ClientSampleId :
MR-MH-14-COMP

Tgt Ion	Ratio	Resp	Lower	Upper
113	100	166162		
111	101.0	77.6	116.4	
192	18.3	15.9	23.9	




Manual Integrations
APPROVED


MMDadoda
3/13/2019 4:41:51 PM

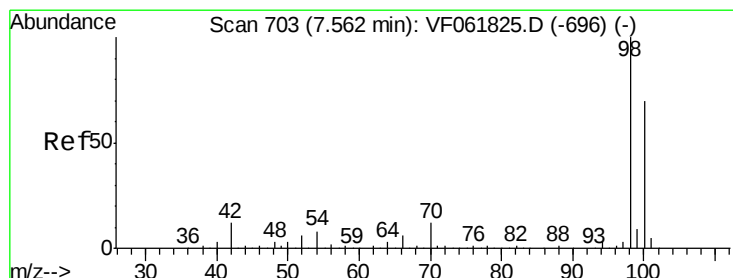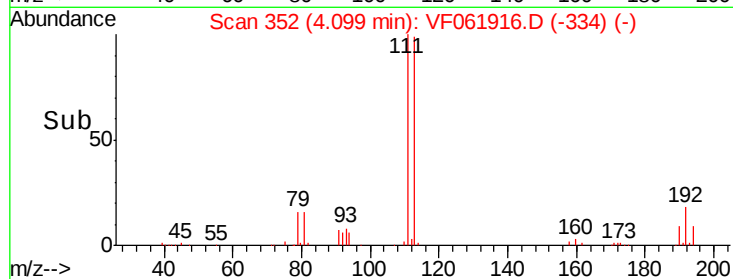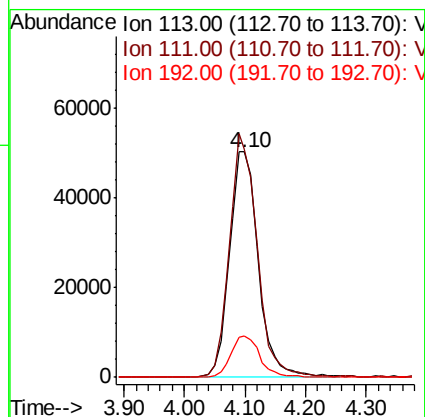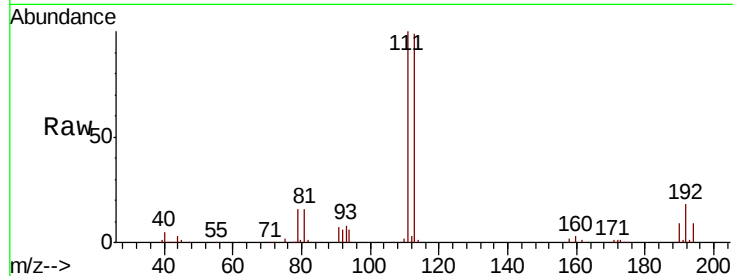

#50
Toluene-d8
Concen: 44.812 ug/l
RT: 7.54 min Scan# 701
Delta R.T. -0.02 min
Lab File: VF061916.D
Acq: 12 Mar 2019 20:30

Tgt Ion	Ratio	Resp	Lower	Upper
98	100	424801		
100	70.4	56.0	84.0	

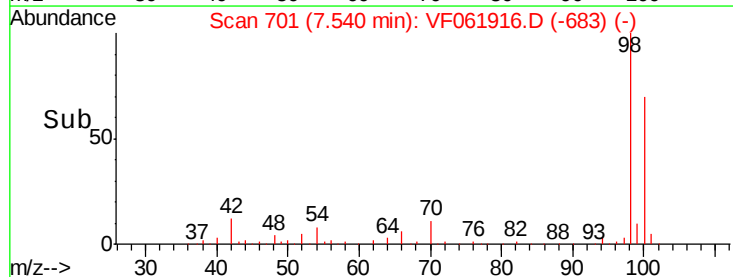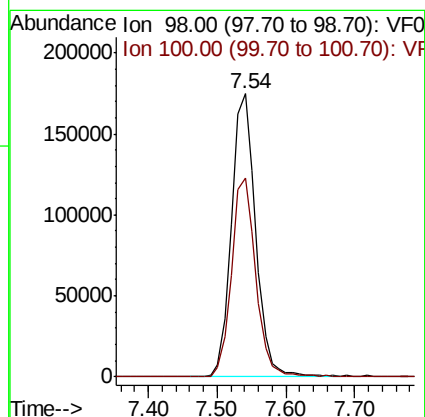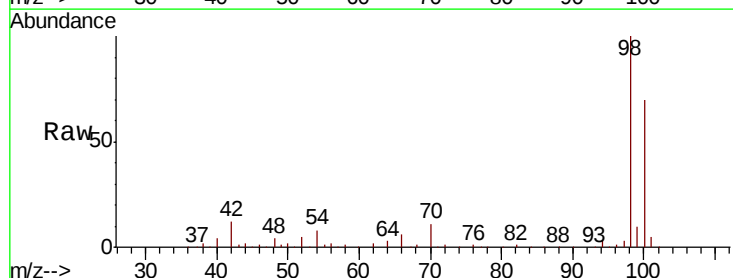

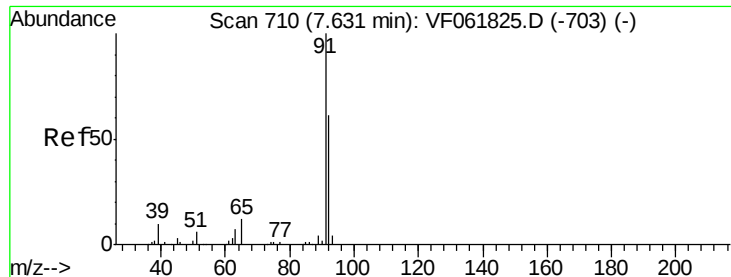

#52

Toluene

Concen: 1.310 ug/l

RT: 7.61 min Scan# 708

Delta R.T. -0.02 min

Lab File: VF061916.D

Acq: 12 Mar 2019 20:30

Instrument :

MSVOA_F

ClientSampleId :

MR-MH-14-COMP

Tgt Ion: 92 Resp: 8748

Ion Ratio Lower Upper

92 100





91 183.8 132.0 198.0

Manual Integrations

APPROVED

MMDadoda

3/13/2019 4:41:51 PM

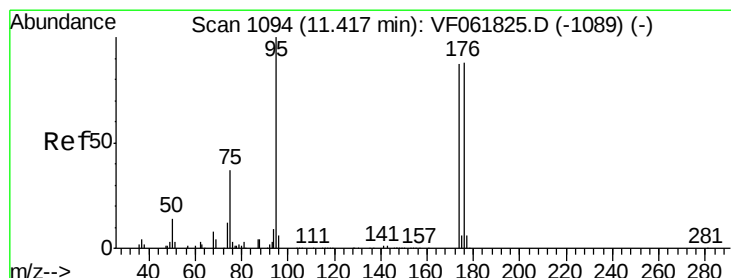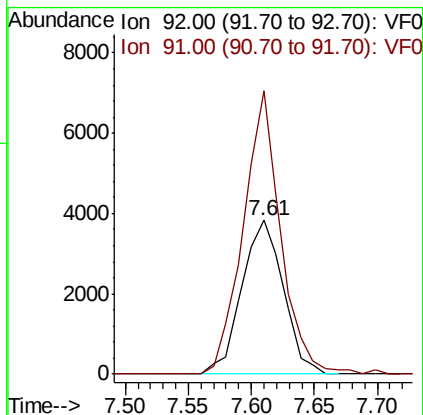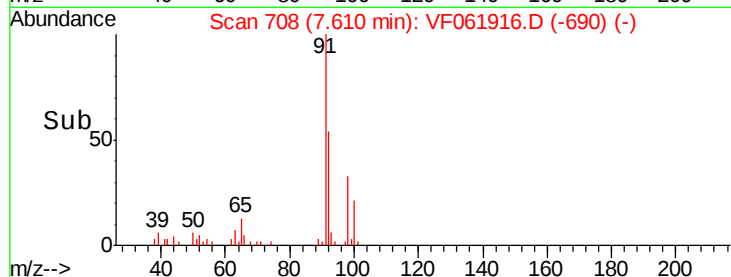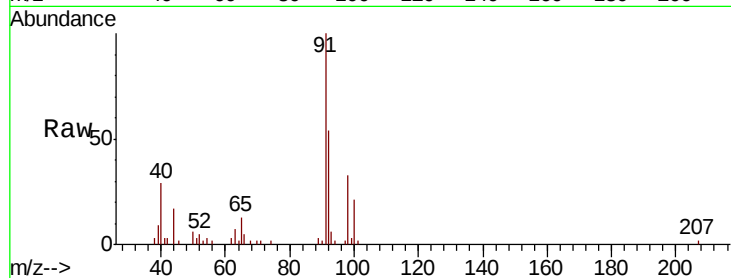

#62

4-Bromofluorobenzene

Concen: 53.017 ug/l

RT: 11.40 min Scan# 1092

Delta R.T. -0.02 min

Lab File: VF061916.D

Acq: 12 Mar 2019 20:30




Tgt Ion: 95 Resp: 196874


Ion Ratio Lower Upper

95 100

174 80.1 0.0 174.0

176 77.7 0.0 175.2

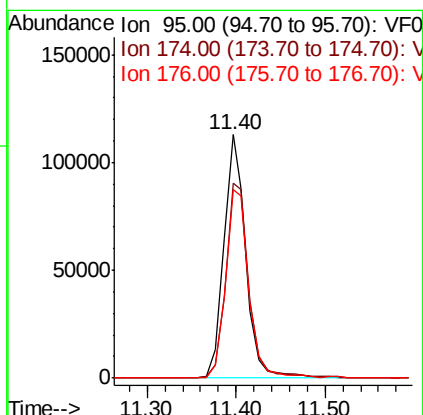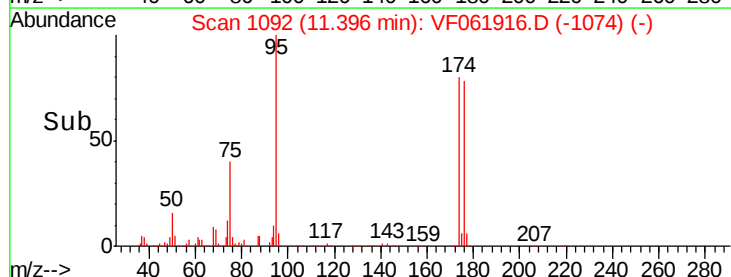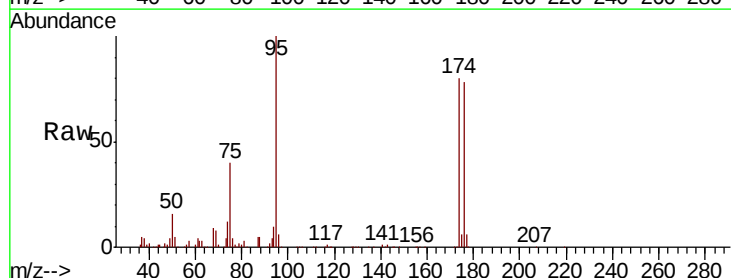

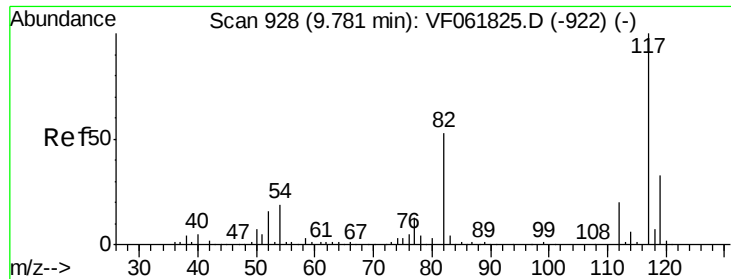


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.76 min Scan# 926
Delta R.T. -0.02 min
Lab File: VF061916.D
Acq: 12 Mar 2019 20:30

Instrument :
MSVOA_F
ClientSampleId :
MR-MH-14-COMP

Tgt Ion	Ratio	Resp	Lower	Upper
117	100	382895		
82	49.6	42.6	63.8	
119	31.5	26.0	39.0	

Manual Integrations
APPROVED

MMDadoda
3/13/2019 4:41:51 PM



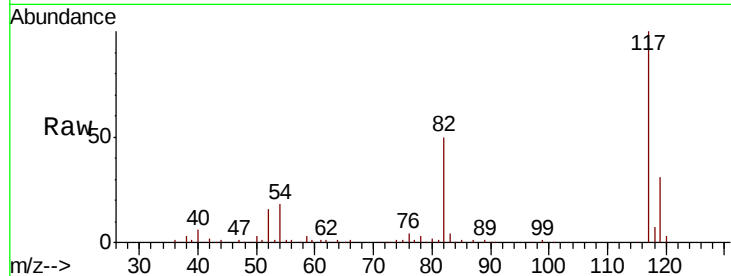


Abundance

Ion 117.00 (116.70 to 117.70): V


Ion 82.00 (81.70 to 82.70): VF0

Ion 119.00 (118.70 to 119.70): V

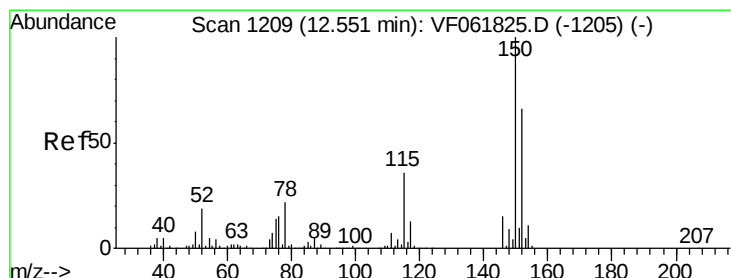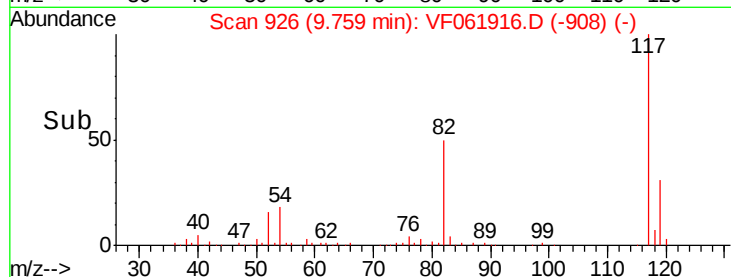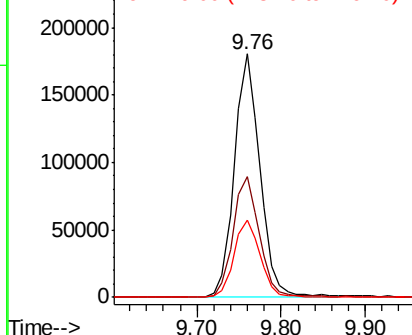

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.54 min Scan# 1208
Delta R.T. -0.01 min
Lab File: VF061916.D
Acq: 12 Mar 2019 20:30

Tgt Ion	Ratio	Resp	Lower	Upper
152	100	221615		
115	52.7	27.7	83.1	
150	155.9	0.0	304.2	

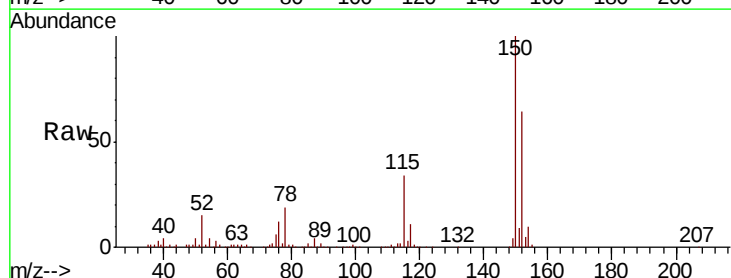

Abundance

Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

