


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF062118\
 Data File : VF059262.D
 Acq On : 21 Jun 2018 14:35
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F062118S.M
 Title : SW846 8260
 Last Update : Fri Jun 22 05:22:31 2018

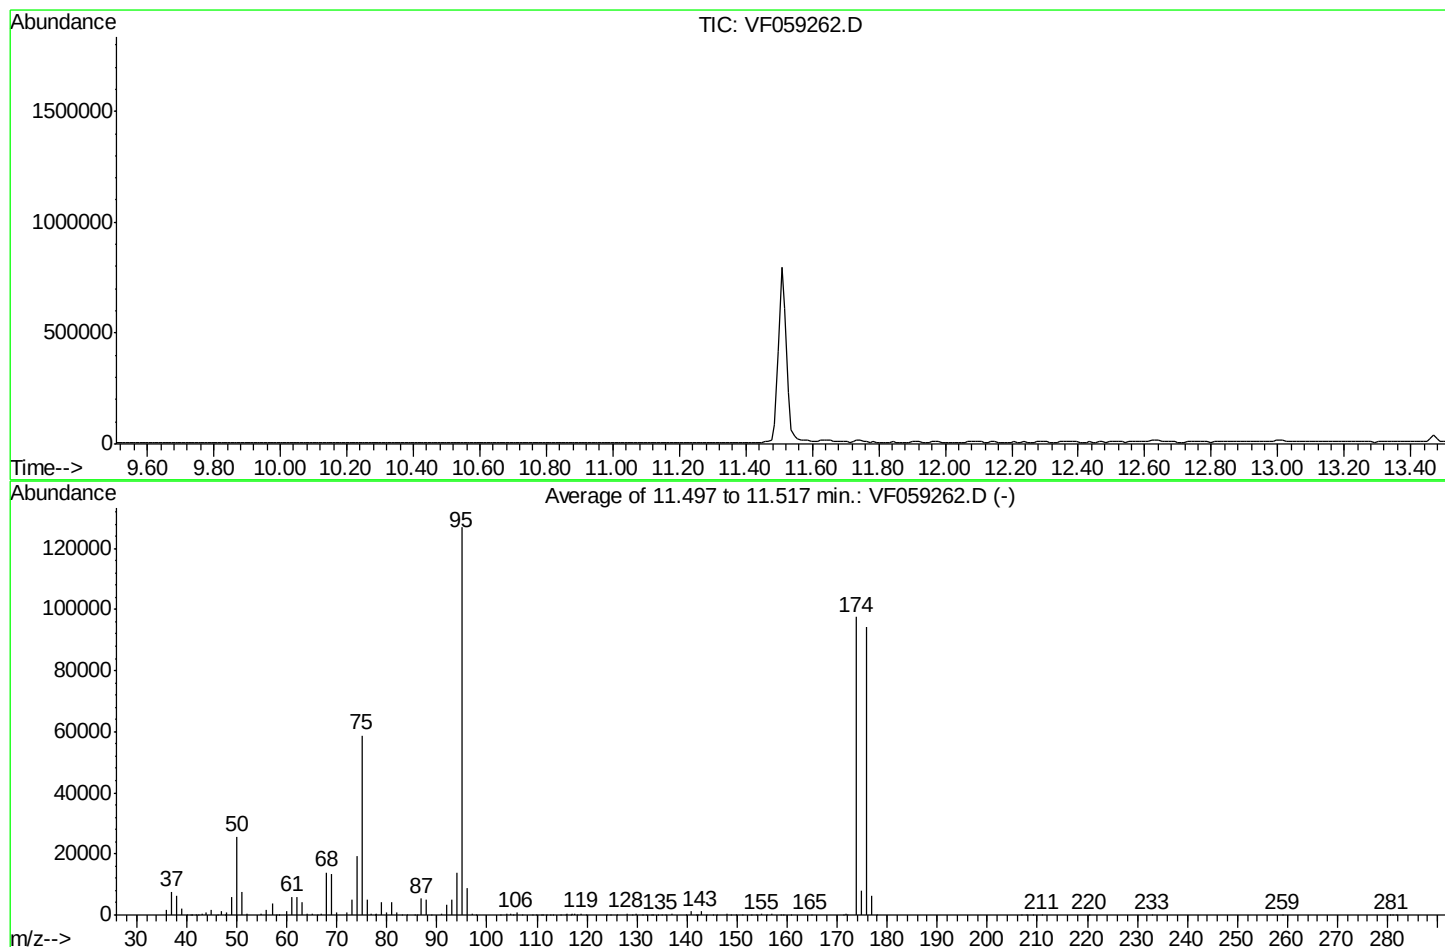

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1106

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	25618	PASS
75	95	30	60	46.3	58733	PASS
95	95	100	100	100.0	126901	PASS
96	95	5	9	7.0	8855	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.9	97549	PASS
175	174	5	9	8.0	7824	PASS
176	174	95	101	96.6	94234	PASS
177	176	5	9	6.6	6230	PASS