




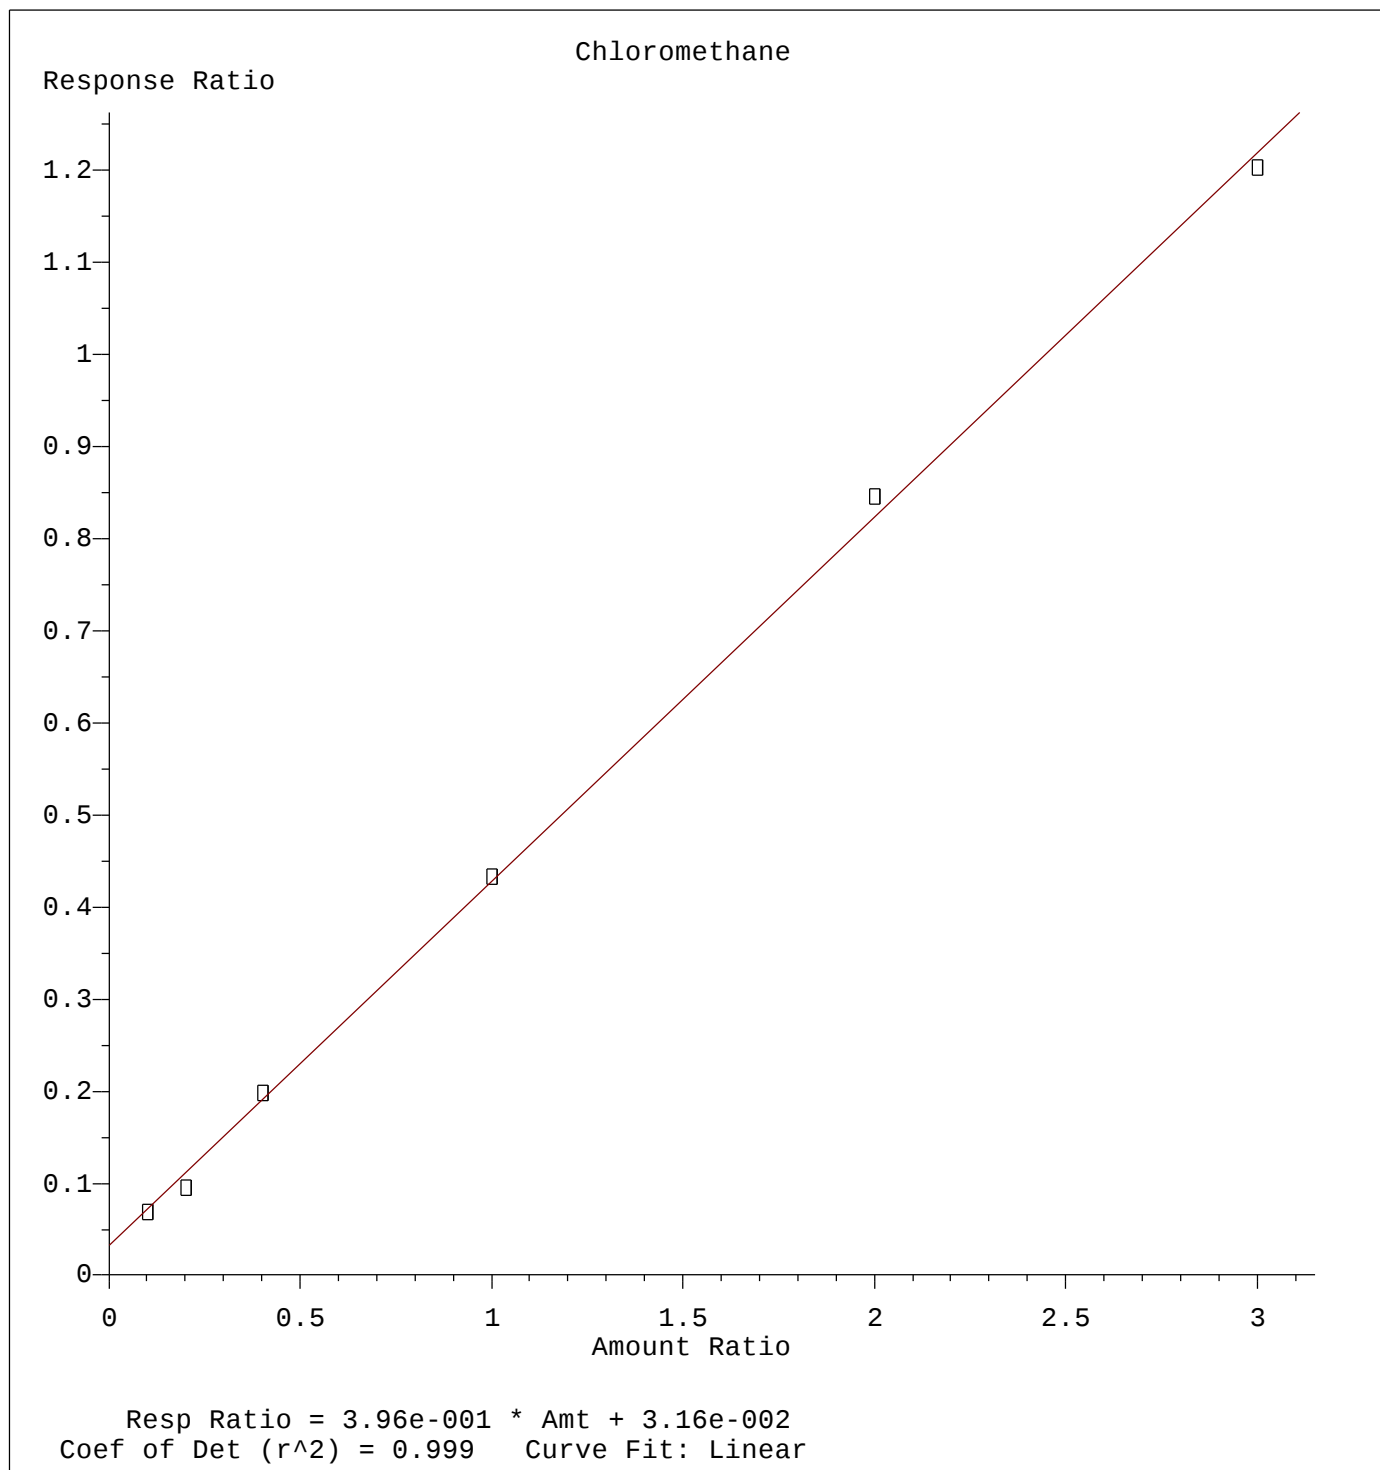


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F082118S.M
Calibration Table Last Updated: Wed Aug 22 04:43:43 2018

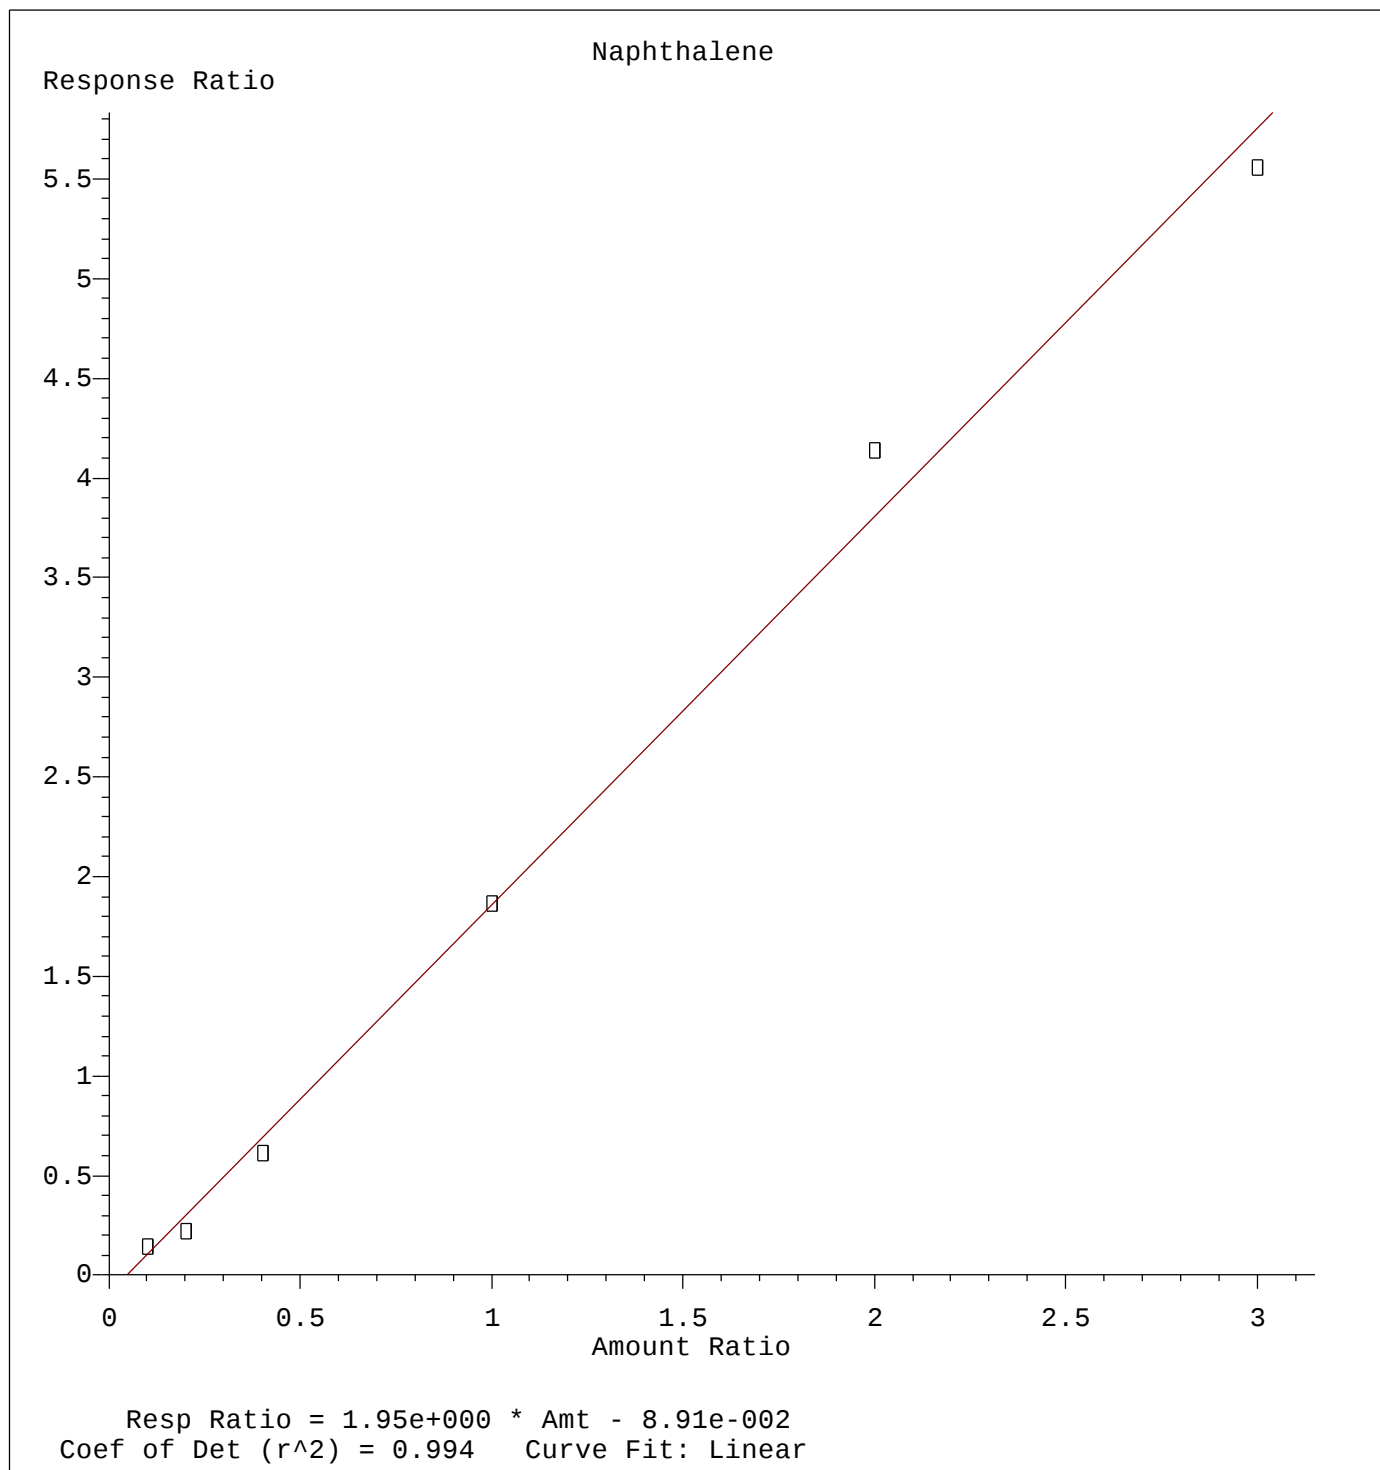

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F082118S.M
Calibration Table Last Updated: Wed Aug 22 04:43:43 2018

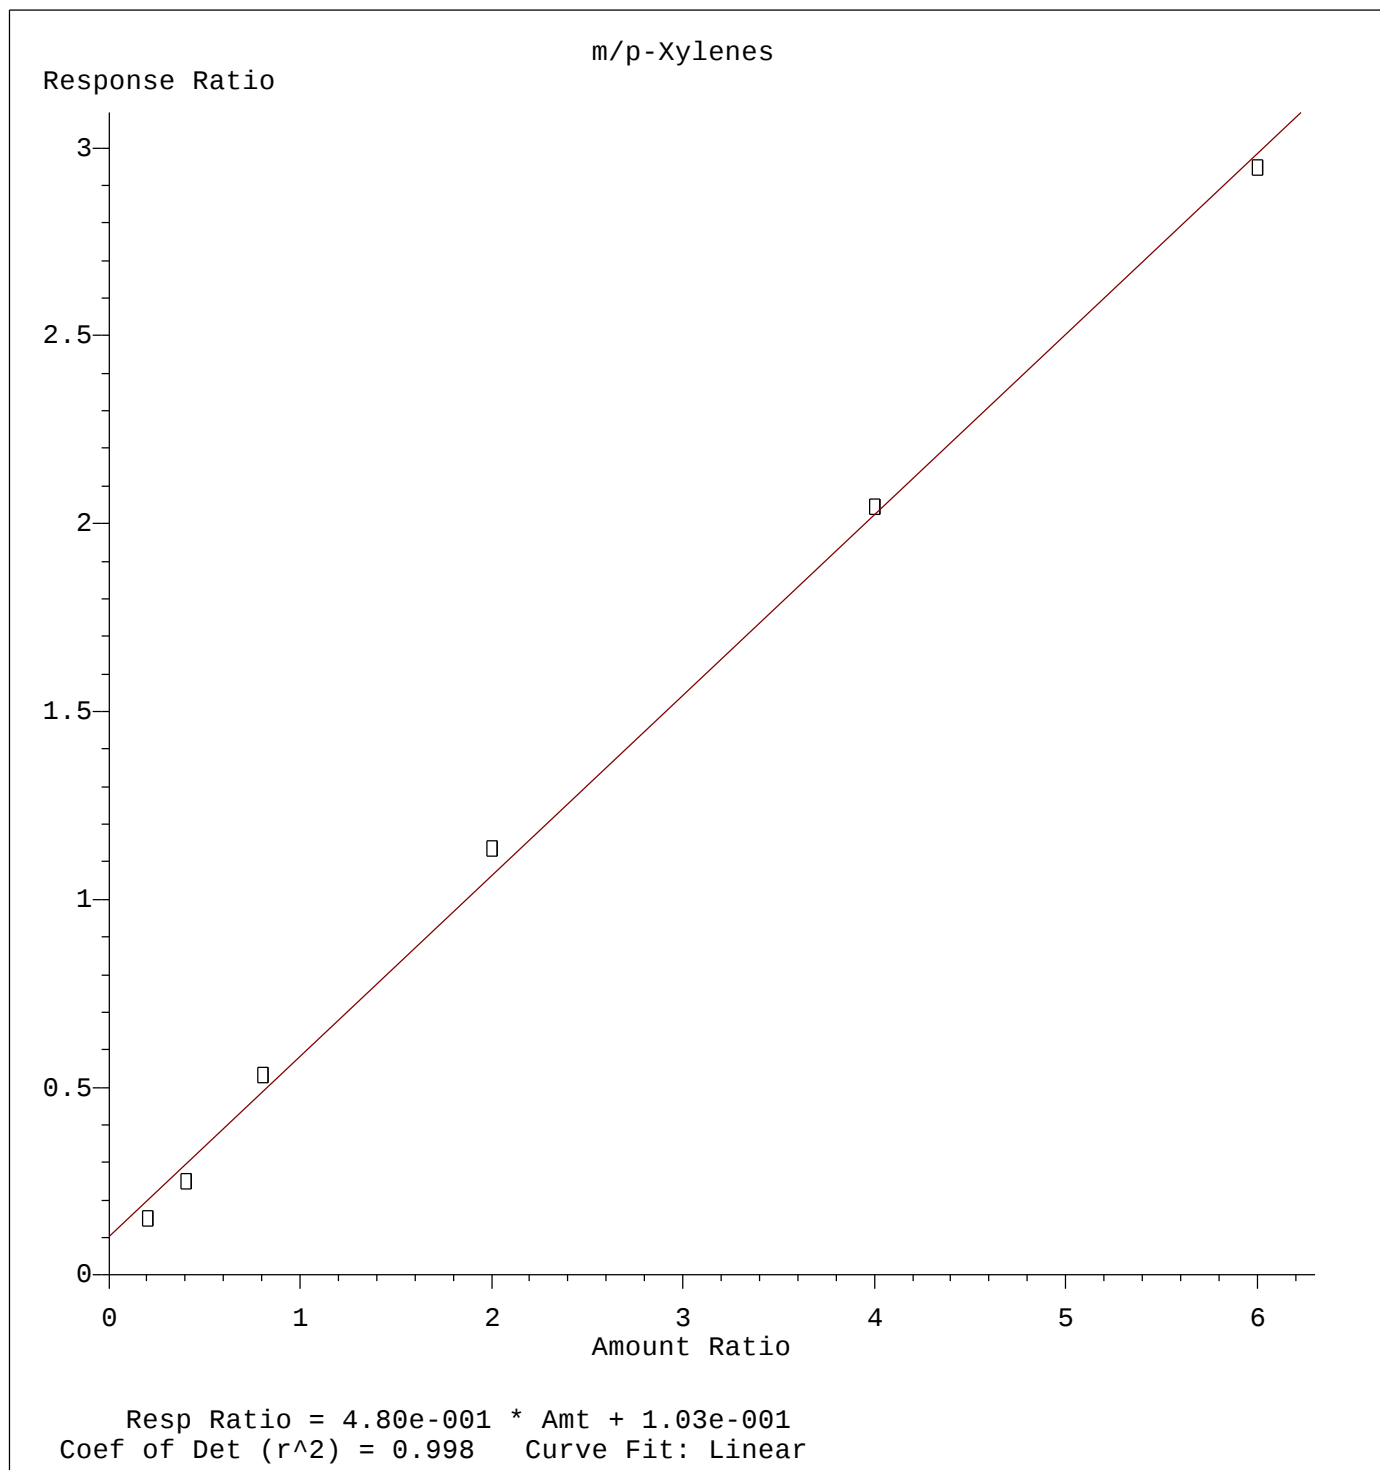


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F082118S.M
Calibration Table Last Updated: Wed Aug 22 04:43:43 2018

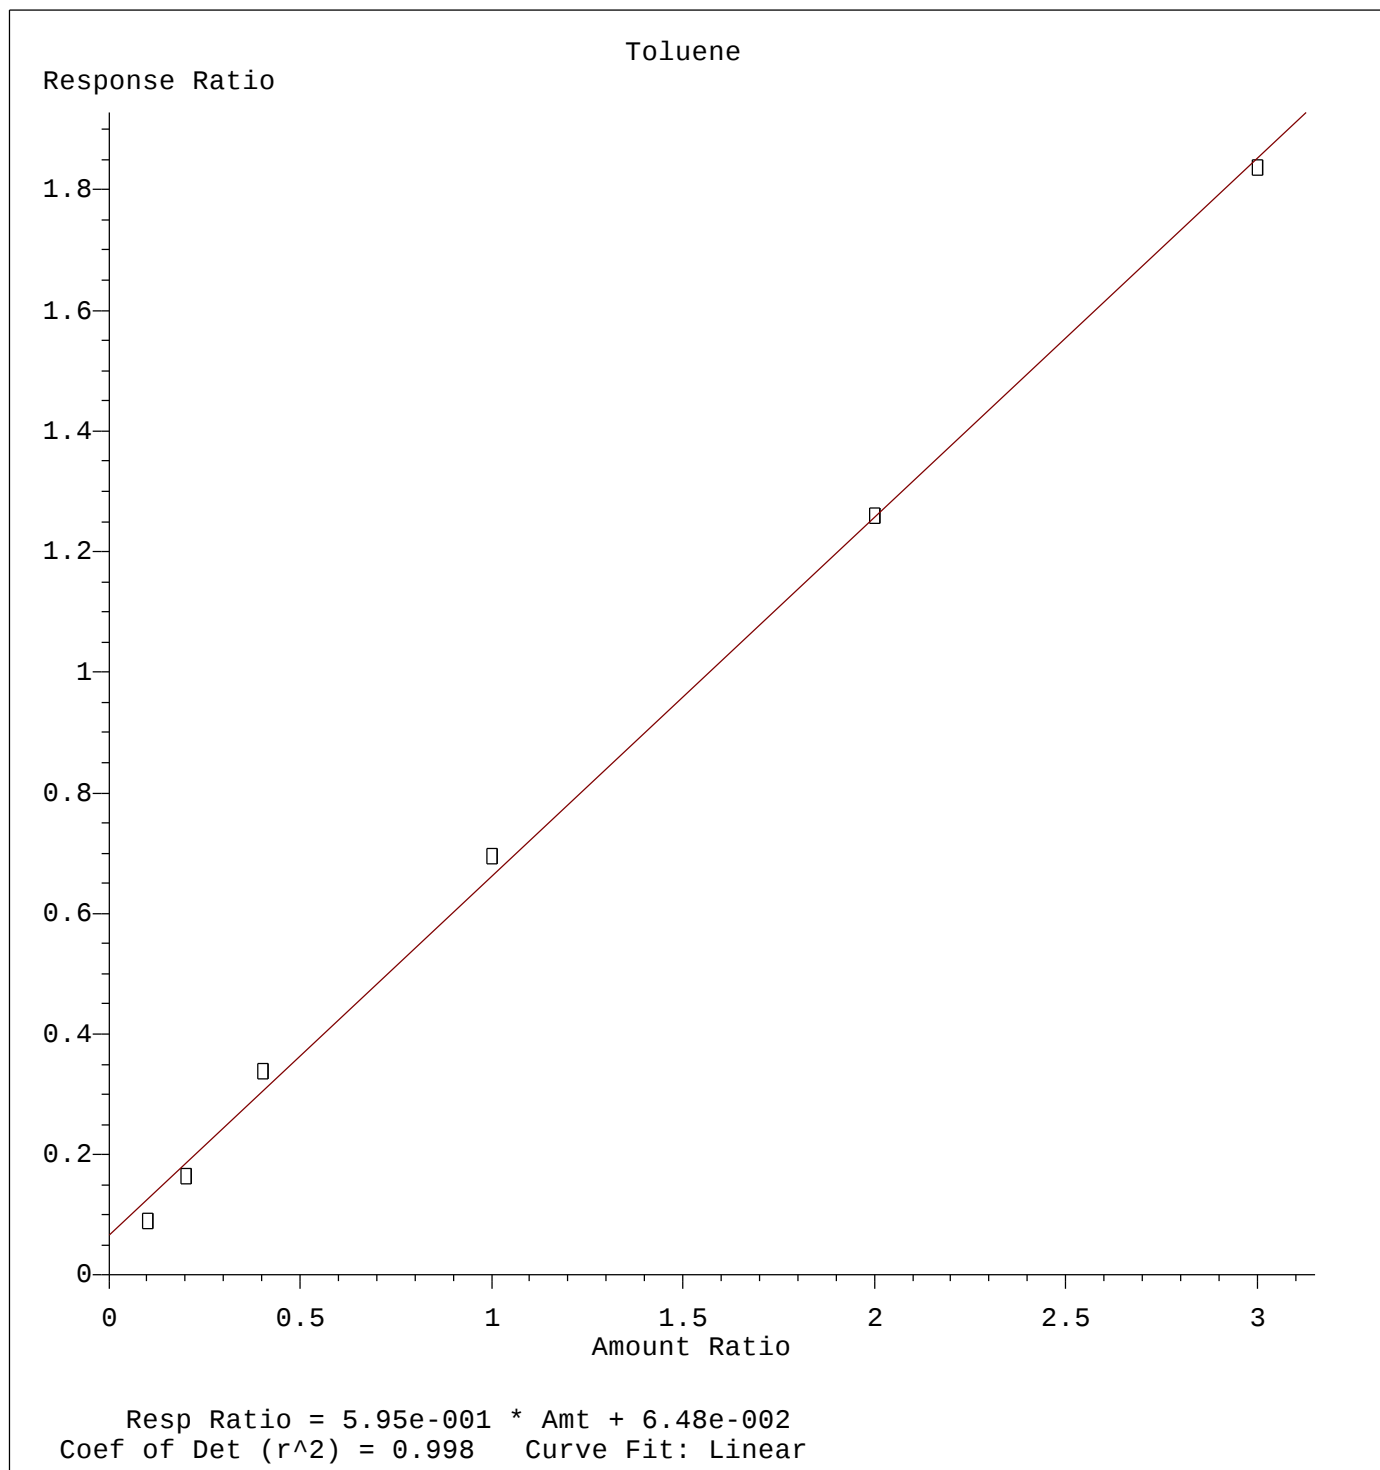

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F082118S.M
Calibration Table Last Updated: Wed Aug 22 04:43:43 2018


Methylene Chloride

Response Ratio

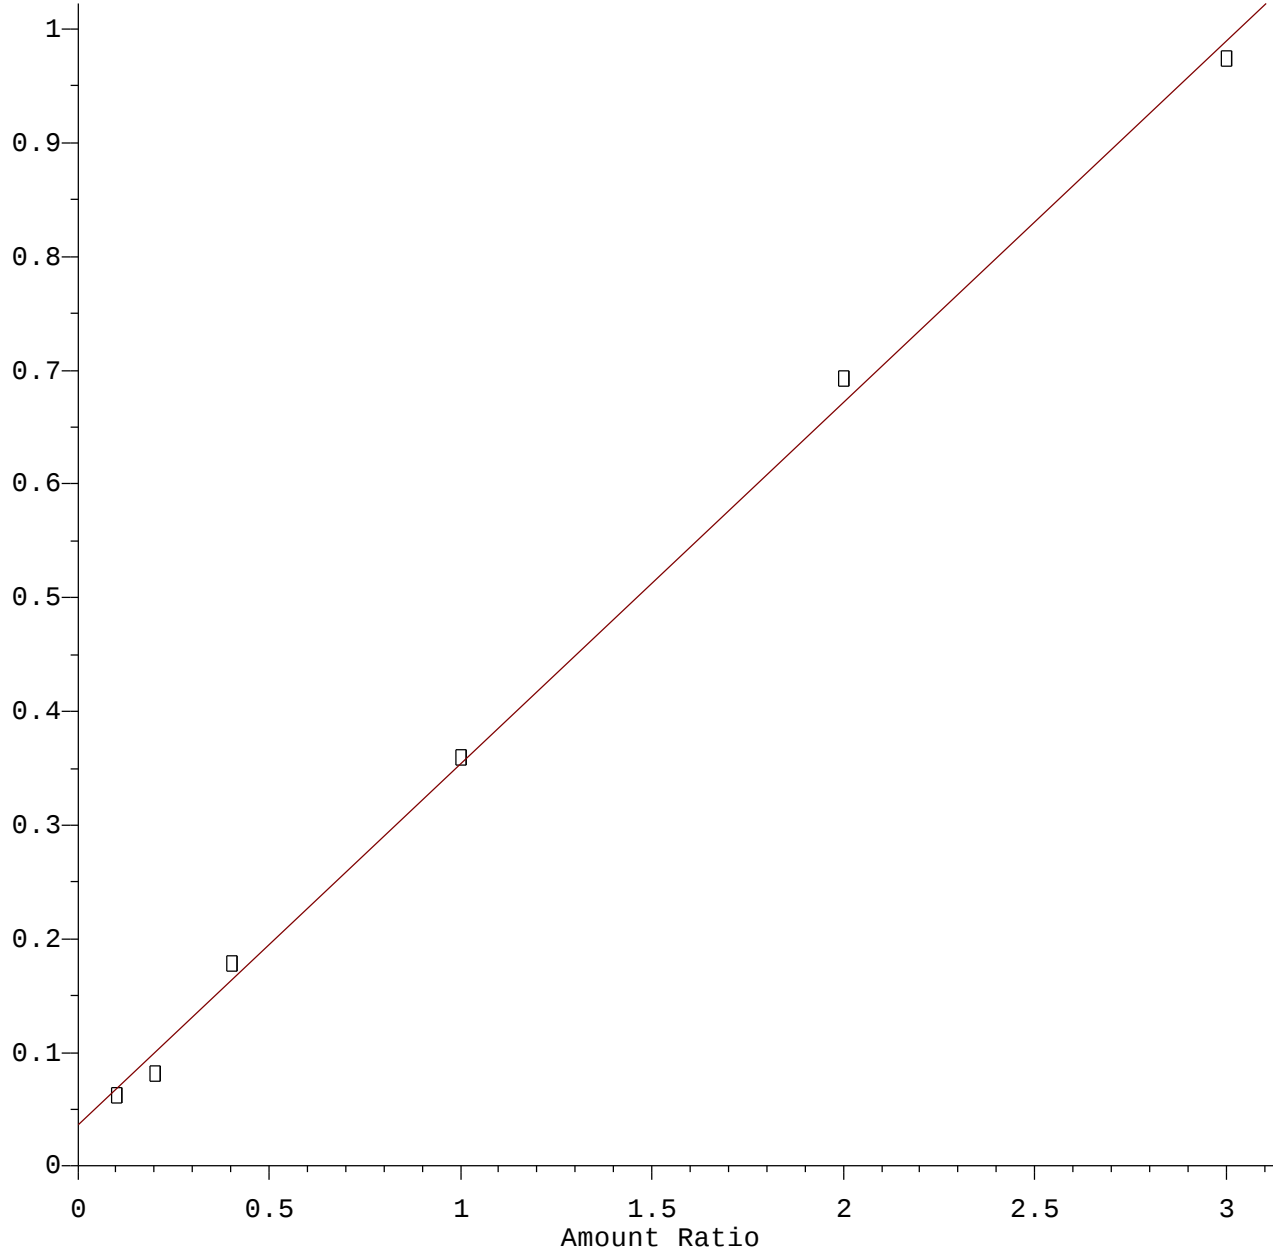


Resp Ratio = $3.18 \times 10^{-1} \times \text{Amt} + 3.63 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F082118S.M
Calibration Table Last Updated: Wed Aug 22 04:43:43 2018

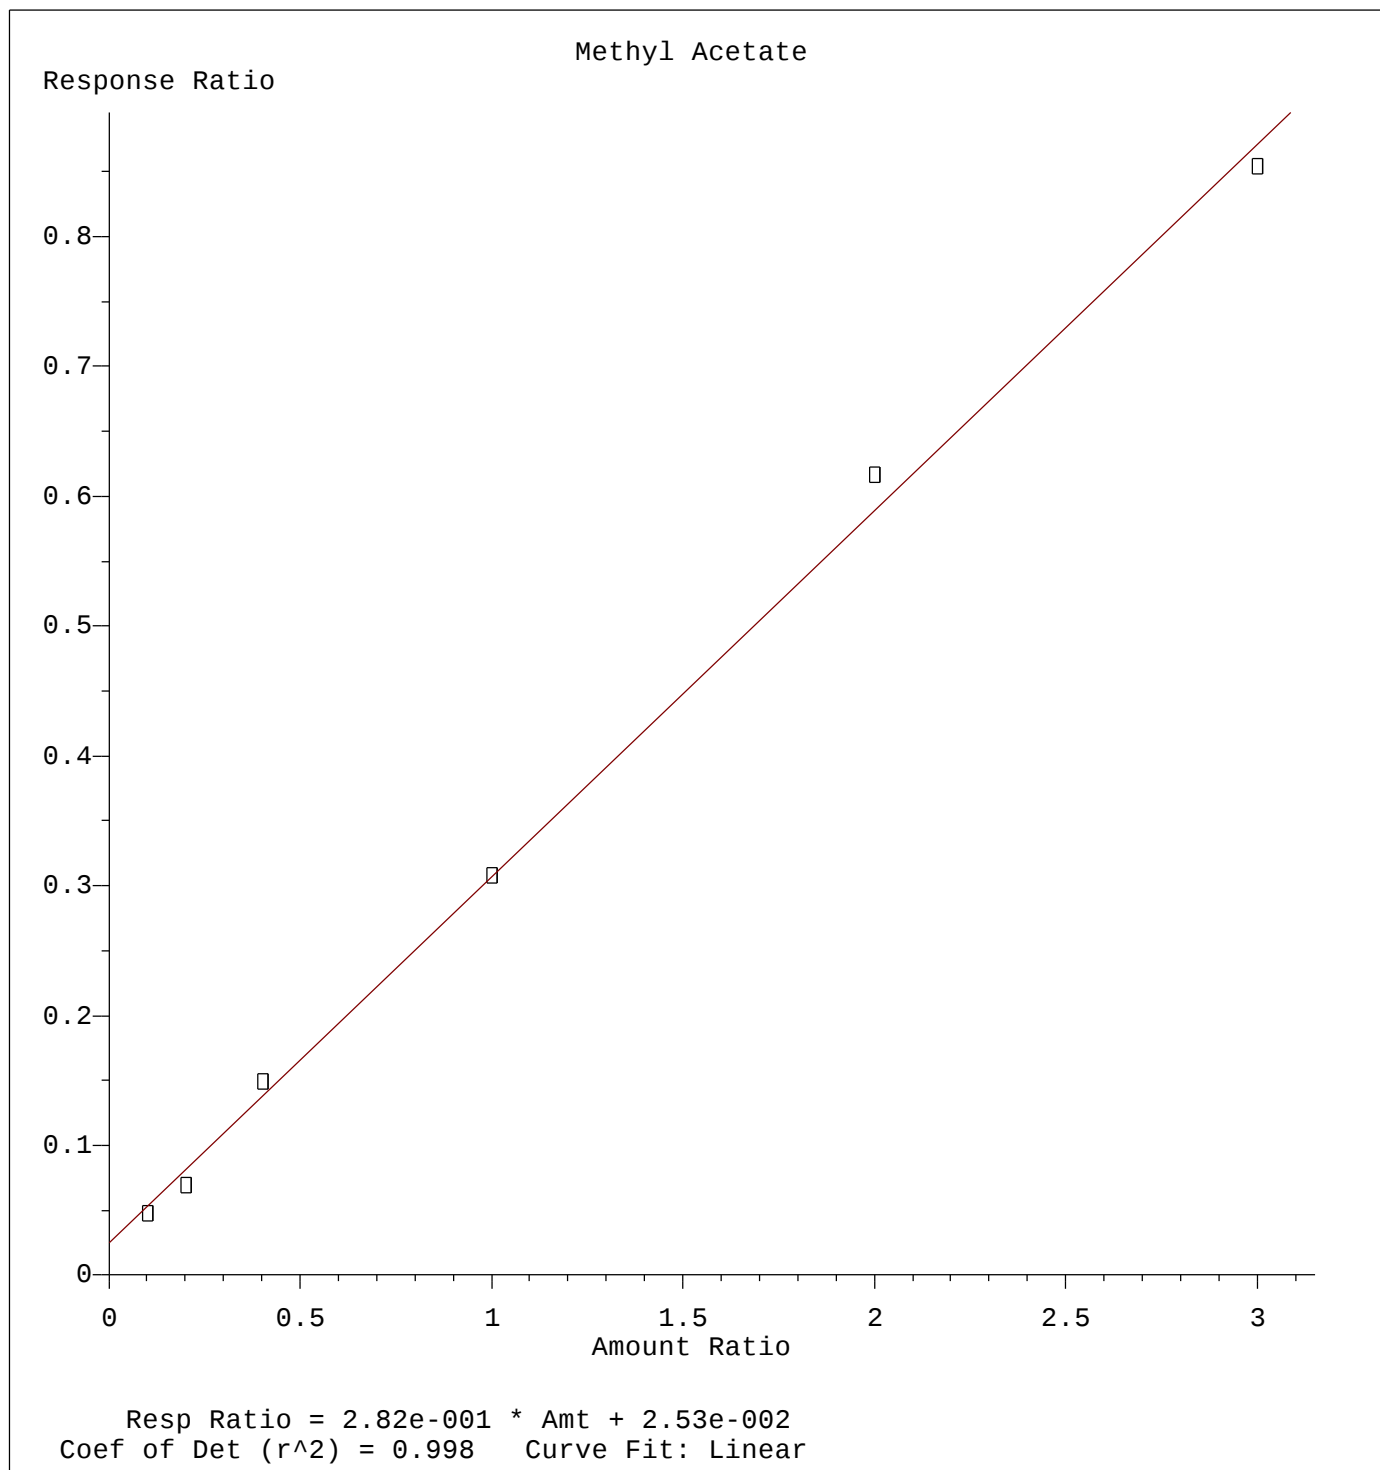

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F082118S.M
Calibration Table Last Updated: Wed Aug 22 04:43:43 2018

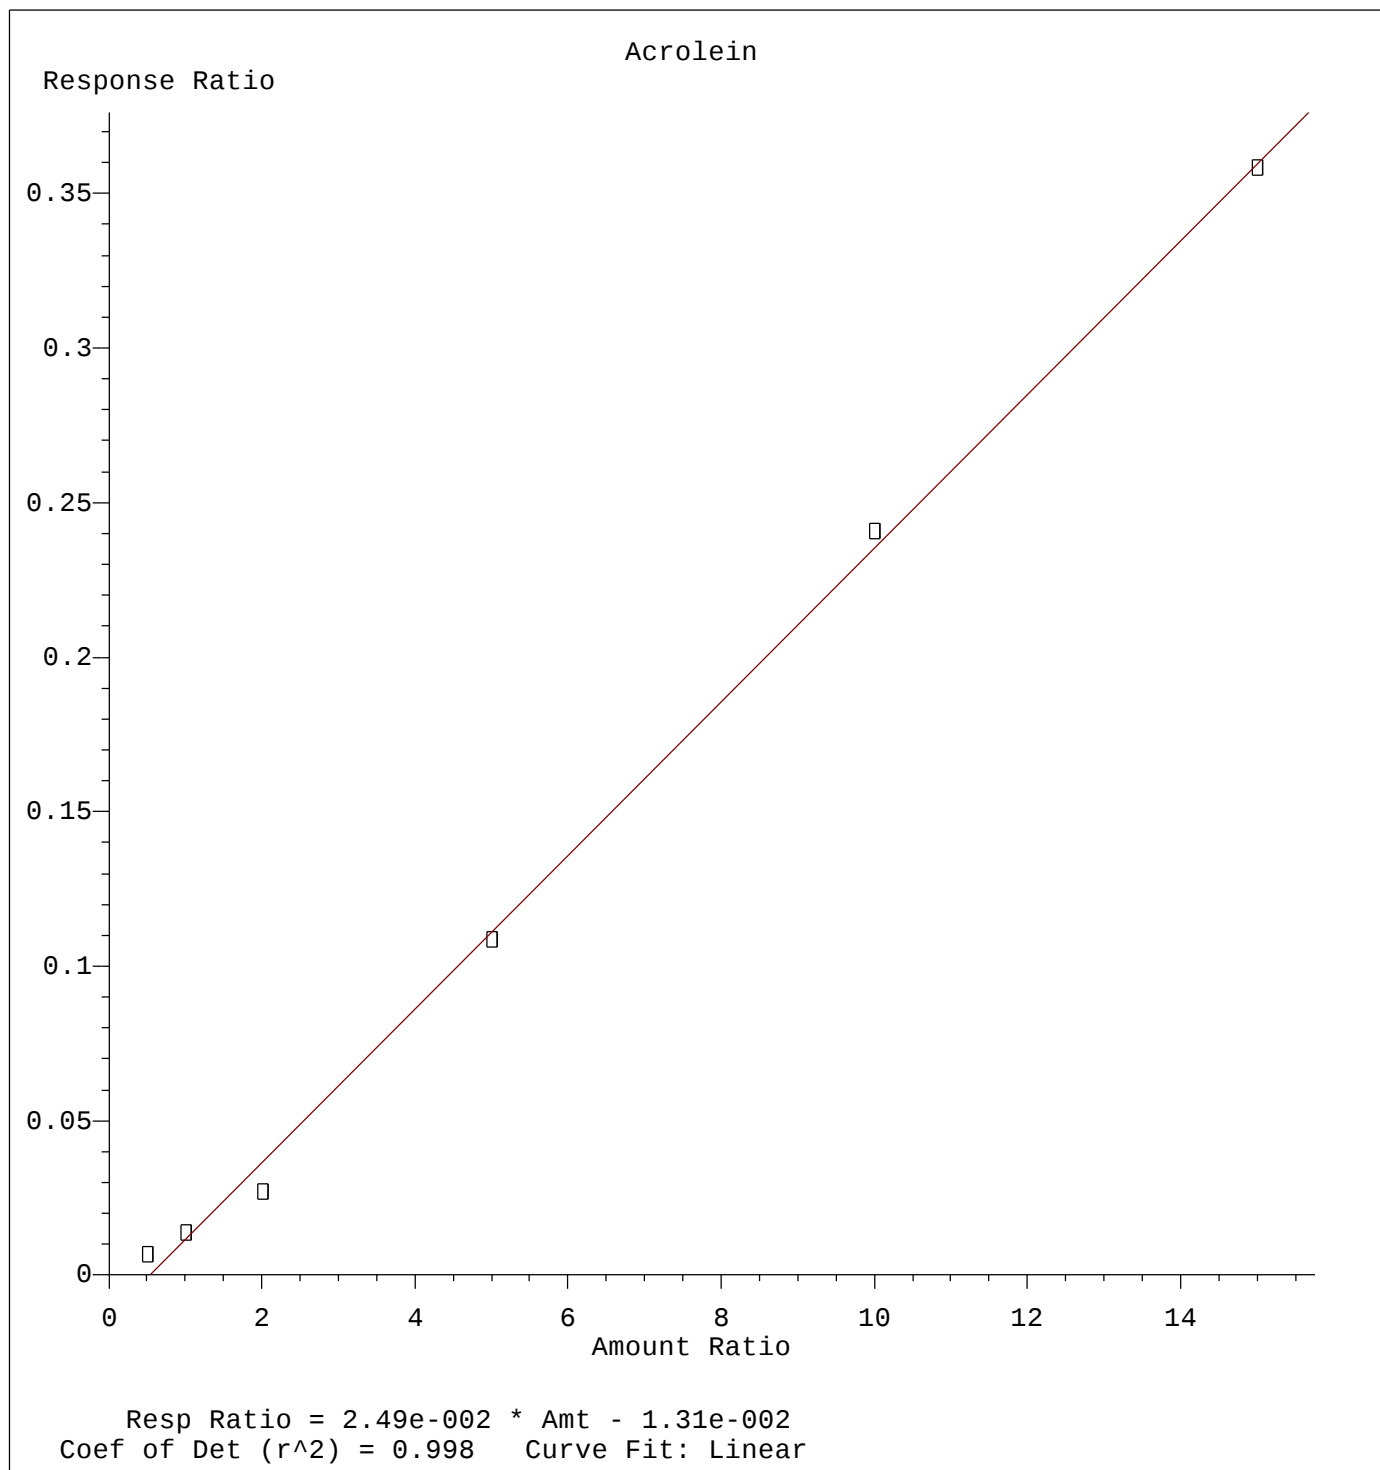

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F082118S.M
Calibration Table Last Updated: Wed Aug 22 04:43:43 2018