


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF082118\
Data File : VF060022.D
Acq On : 21 Aug 2018 15:56
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F082118S.M
Title : SW846 8260
Last Update : Wed Aug 22 04:43:43 2018

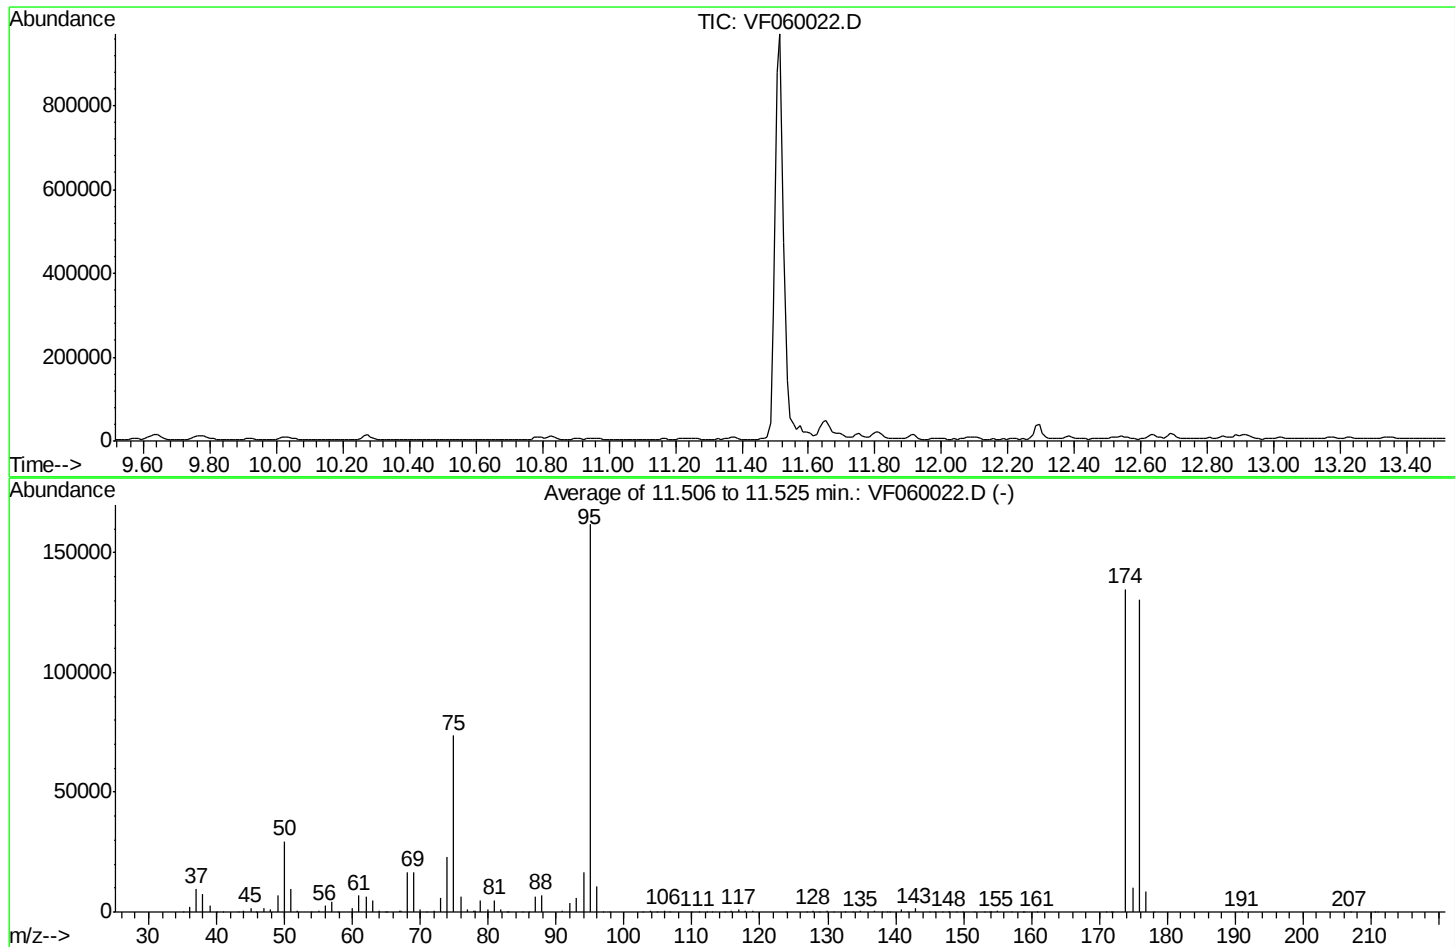

AutoFind: Scans 1113, 1114, 1115; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	29667	PASS
75	95	30	60	45.5	73613	PASS
95	95	100	100	100.0	161890	PASS
96	95	5	9	6.6	10723	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.3	134933	PASS
175	174	5	9	7.4	9930	PASS
176	174	95	101	96.8	130621	PASS
177	176	5	9	6.7	8793	PASS