


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF092118\
 Data File : VF060310.D
 Acq On : 21 Sep 2018 9:57
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00/5mL/MSVOA F/SOIL
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F091918S.M
 Title : SW846 8260
 Last Update : Thu Sep 20 02:58:42 2018

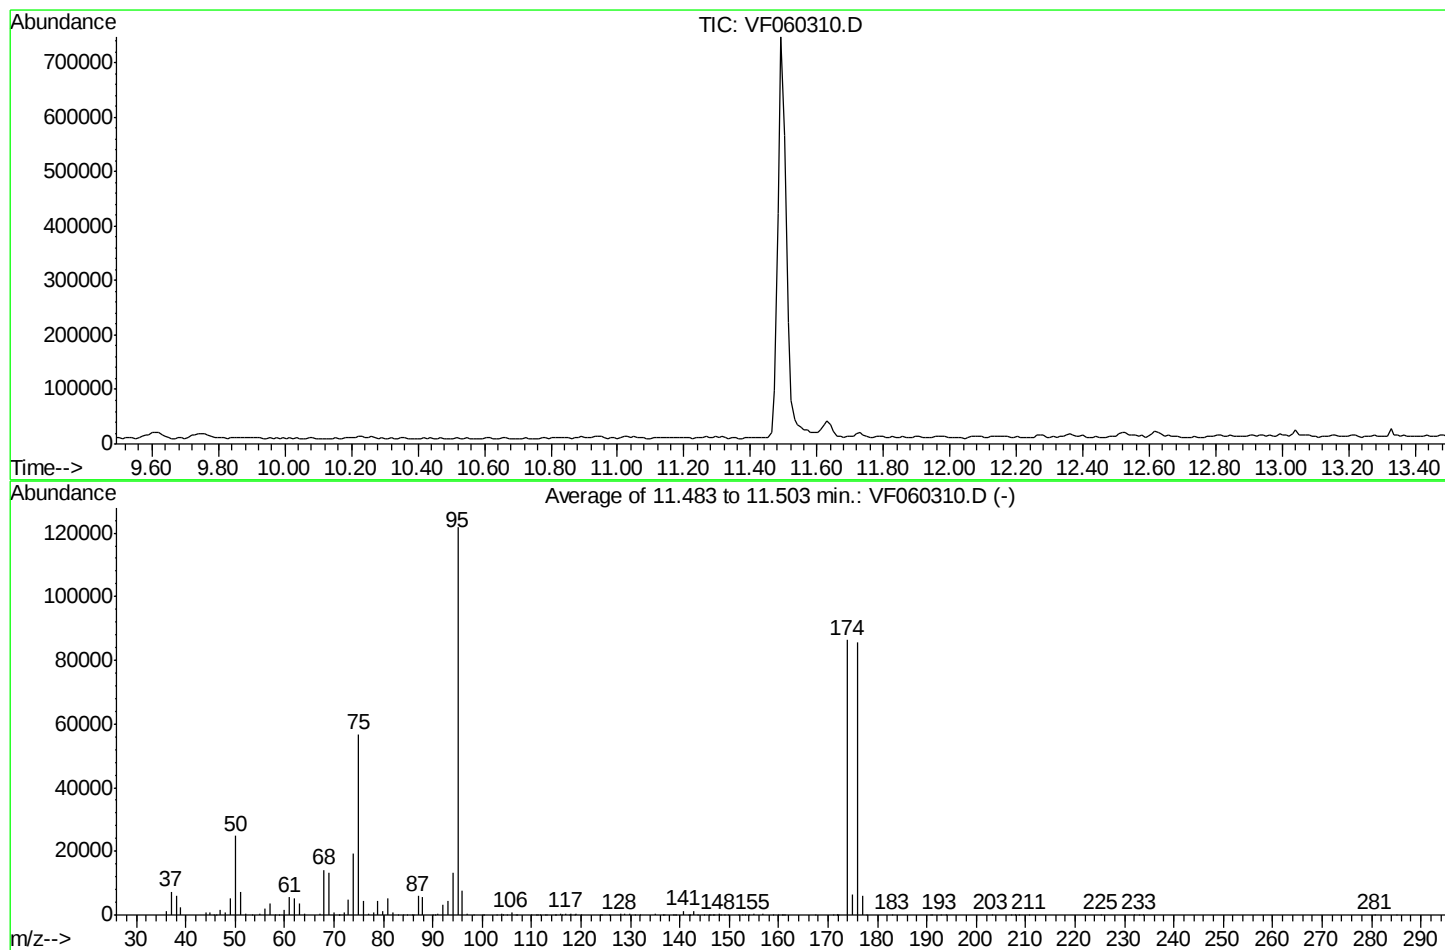

AutoFind: Scans 1101, 1102, 1103; Background Corrected with Scan 1094

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	24917	PASS
75	95	30	60	46.5	56656	PASS
95	95	100	100	100.0	121776	PASS
96	95	5	9	6.4	7809	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.0	86434	PASS
175	174	5	9	7.3	6347	PASS
176	174	95	101	99.1	85664	PASS
177	176	5	9	7.1	6094	PASS