


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF092618\  
Data File : VF060346.D  
Acq On : 26 Sep 2018 10:25  
Operator : VA/AP  
Sample : BFB  
Misc : 5.00/5mL/MSVOA F/SOIL  
ALS Vial : 29 Sample Multiplier: 1

Instrument :  
MSVOA\_F  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F091918S.M  
Title : SW846 8260  
Last Update : Thu Sep 20 02:58:42 2018

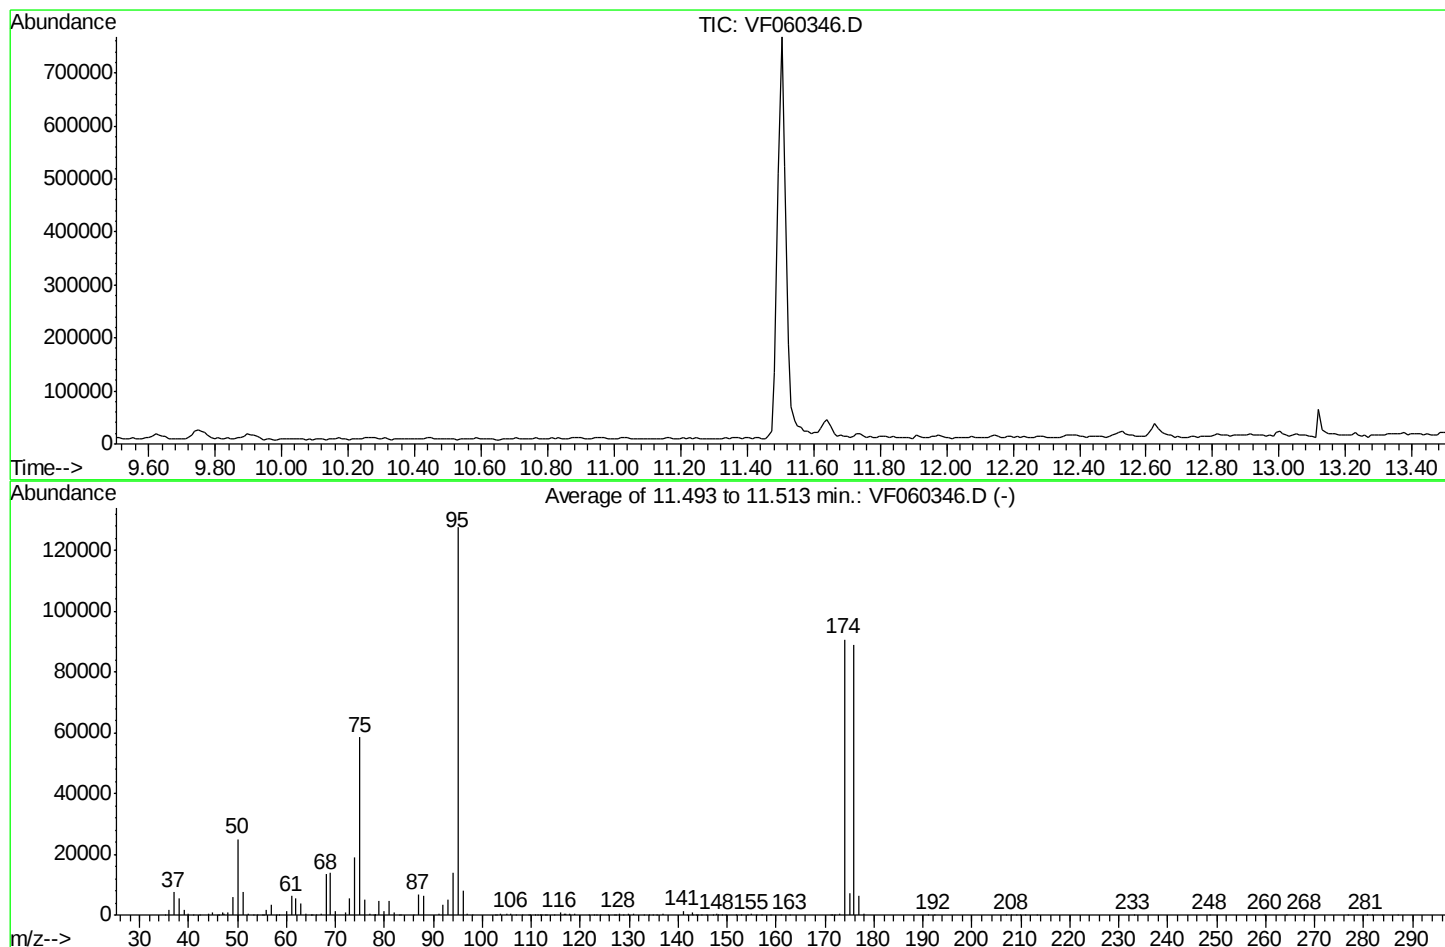

AutoFind: Scans 1102, 1103, 1104; Background Corrected with Scan 1097

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.5      | 24901   | PASS             |
| 75          | 95           | 30           | 60           | 45.9      | 58480   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 127512  | PASS             |
| 96          | 95           | 5            | 9            | 6.4       | 8158    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.5       | 464     | PASS             |
| 174         | 95           | 50           | 100          | 71.0      | 90536   | PASS             |
| 175         | 174          | 5            | 9            | 8.1       | 7378    | PASS             |
| 176         | 174          | 95           | 101          | 98.2      | 88925   | PASS             |
| 177         | 176          | 5            | 9            | 7.2       | 6412    | PASS             |