



Dichlorodifluoromethane

Response Ratio

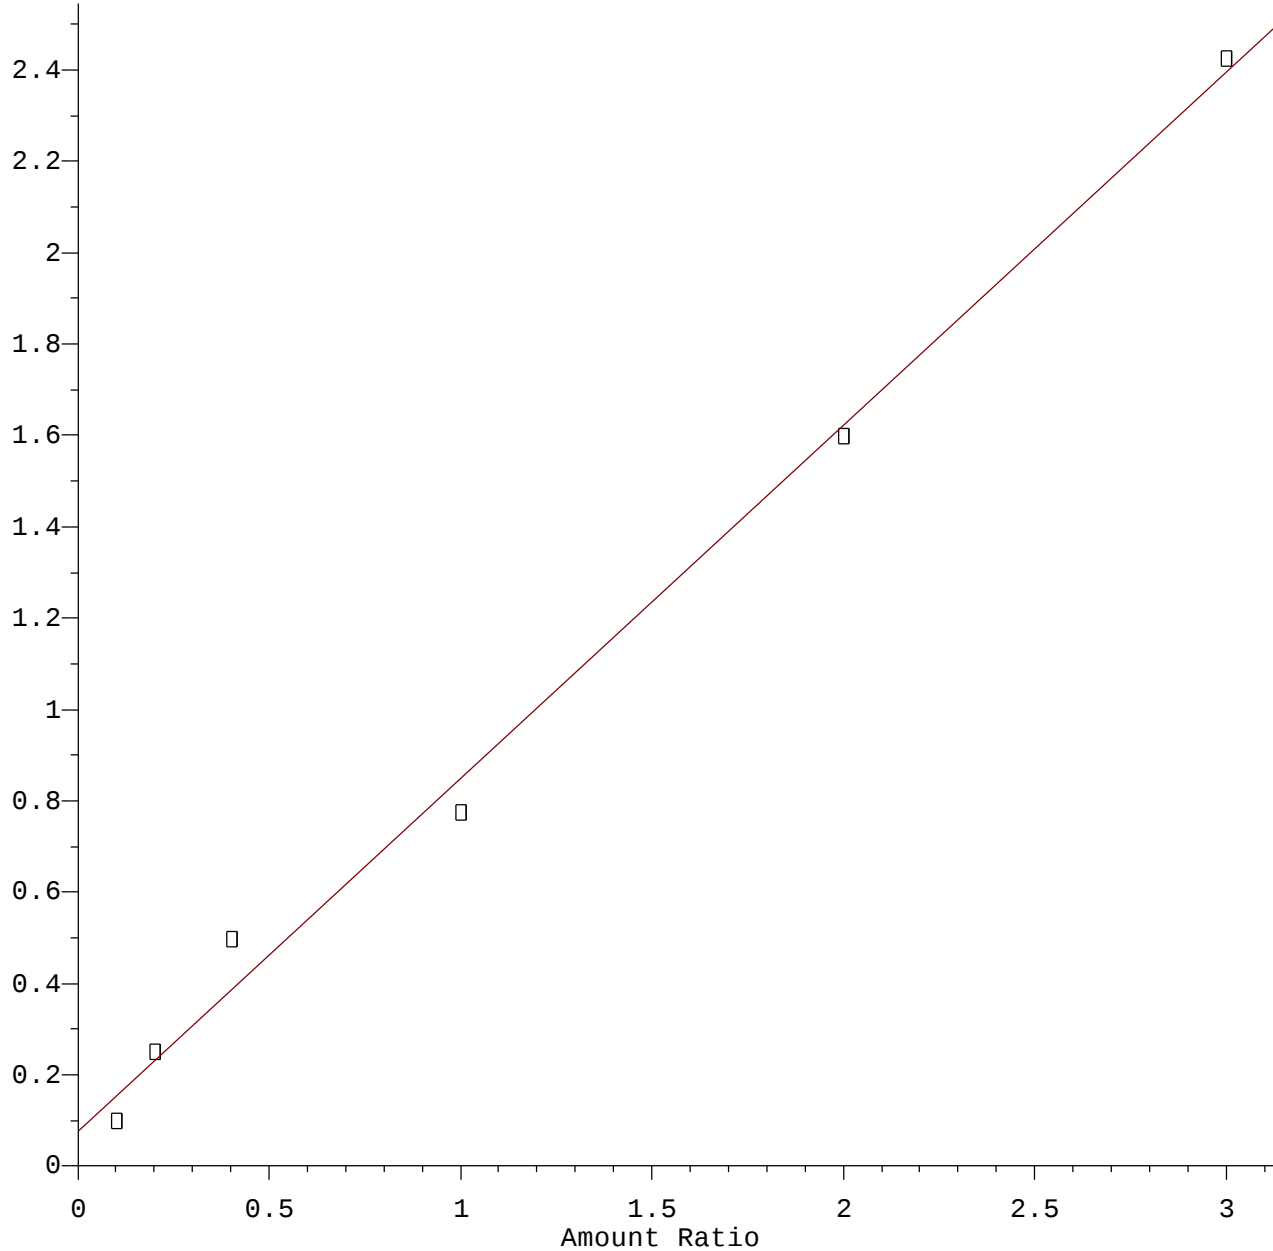

Resp Ratio = $7.73 \times 10^{-1} \times \text{Amt} + 7.67 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102918S.M
Calibration Table Last Updated: Thu Nov 01 15:08:55 2018

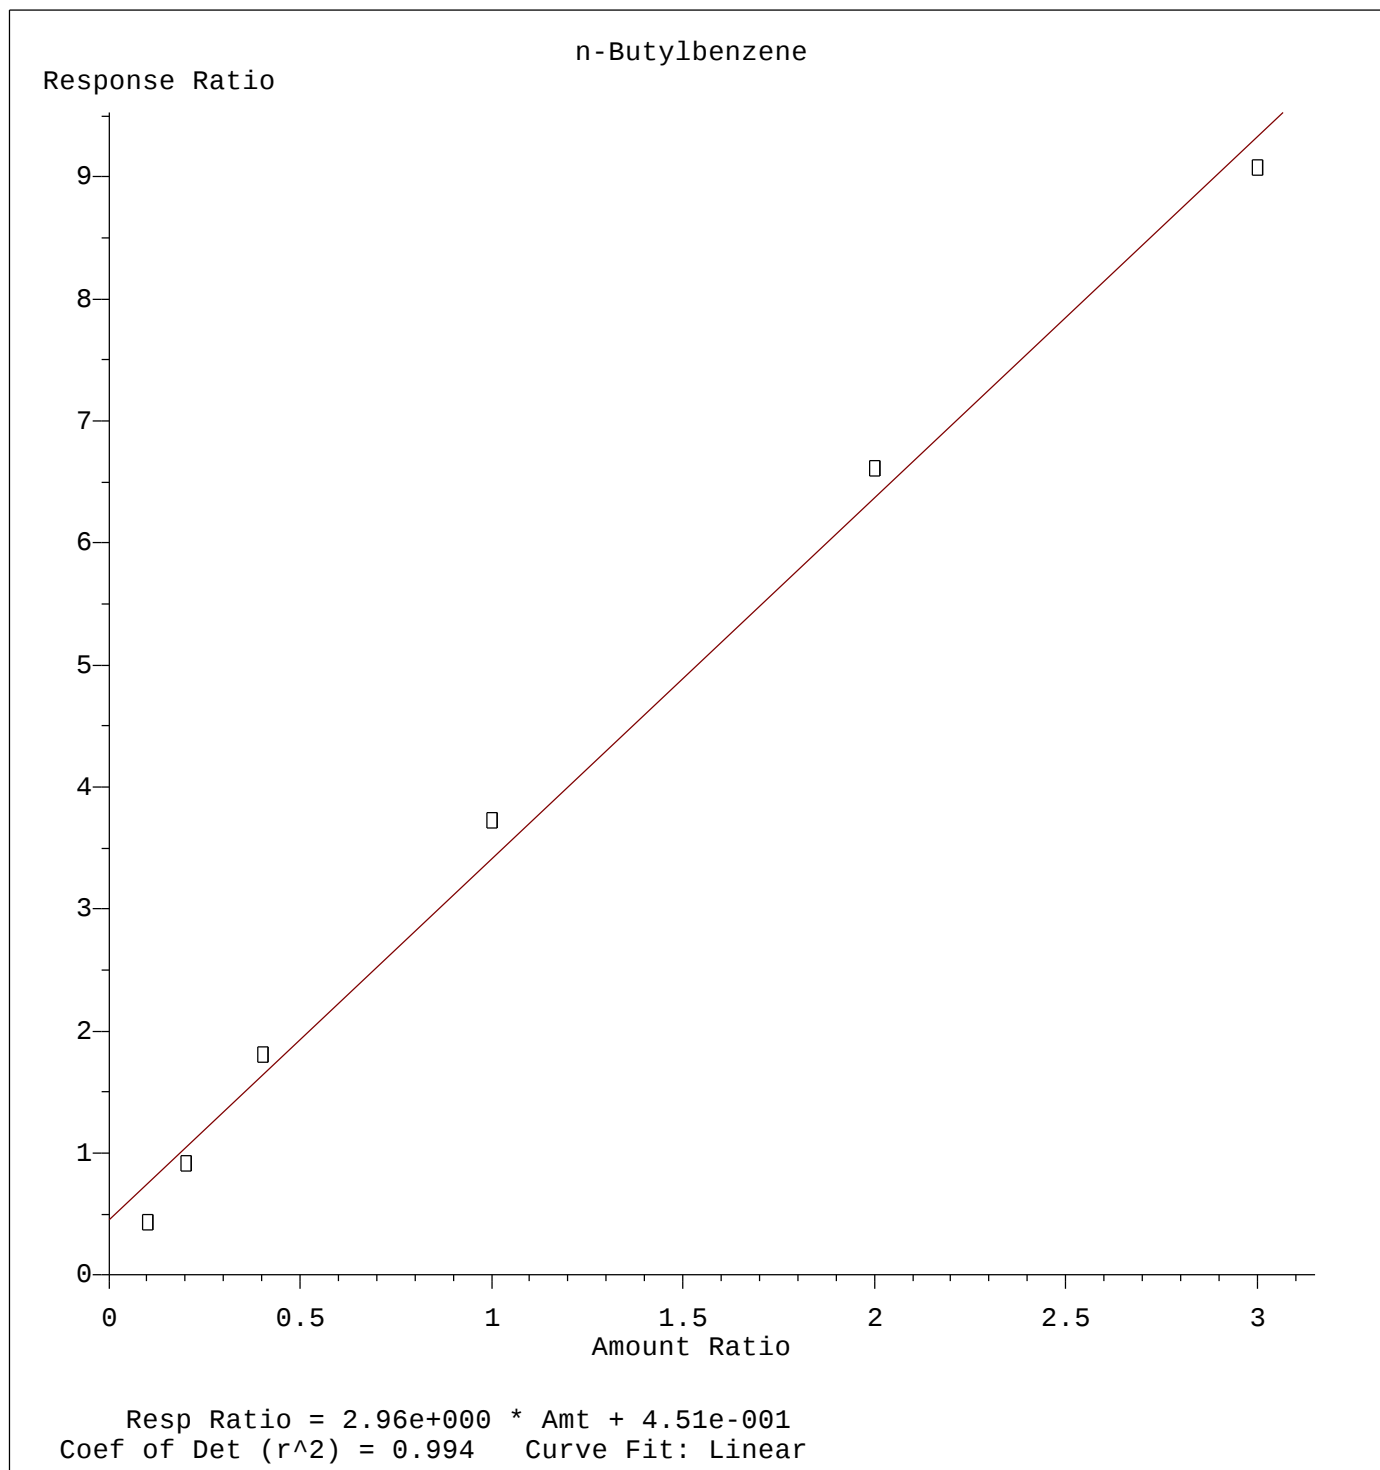

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102918S.M
Calibration Table Last Updated: Thu Nov 01 15:08:55 2018


2-Hexanone

Response Ratio

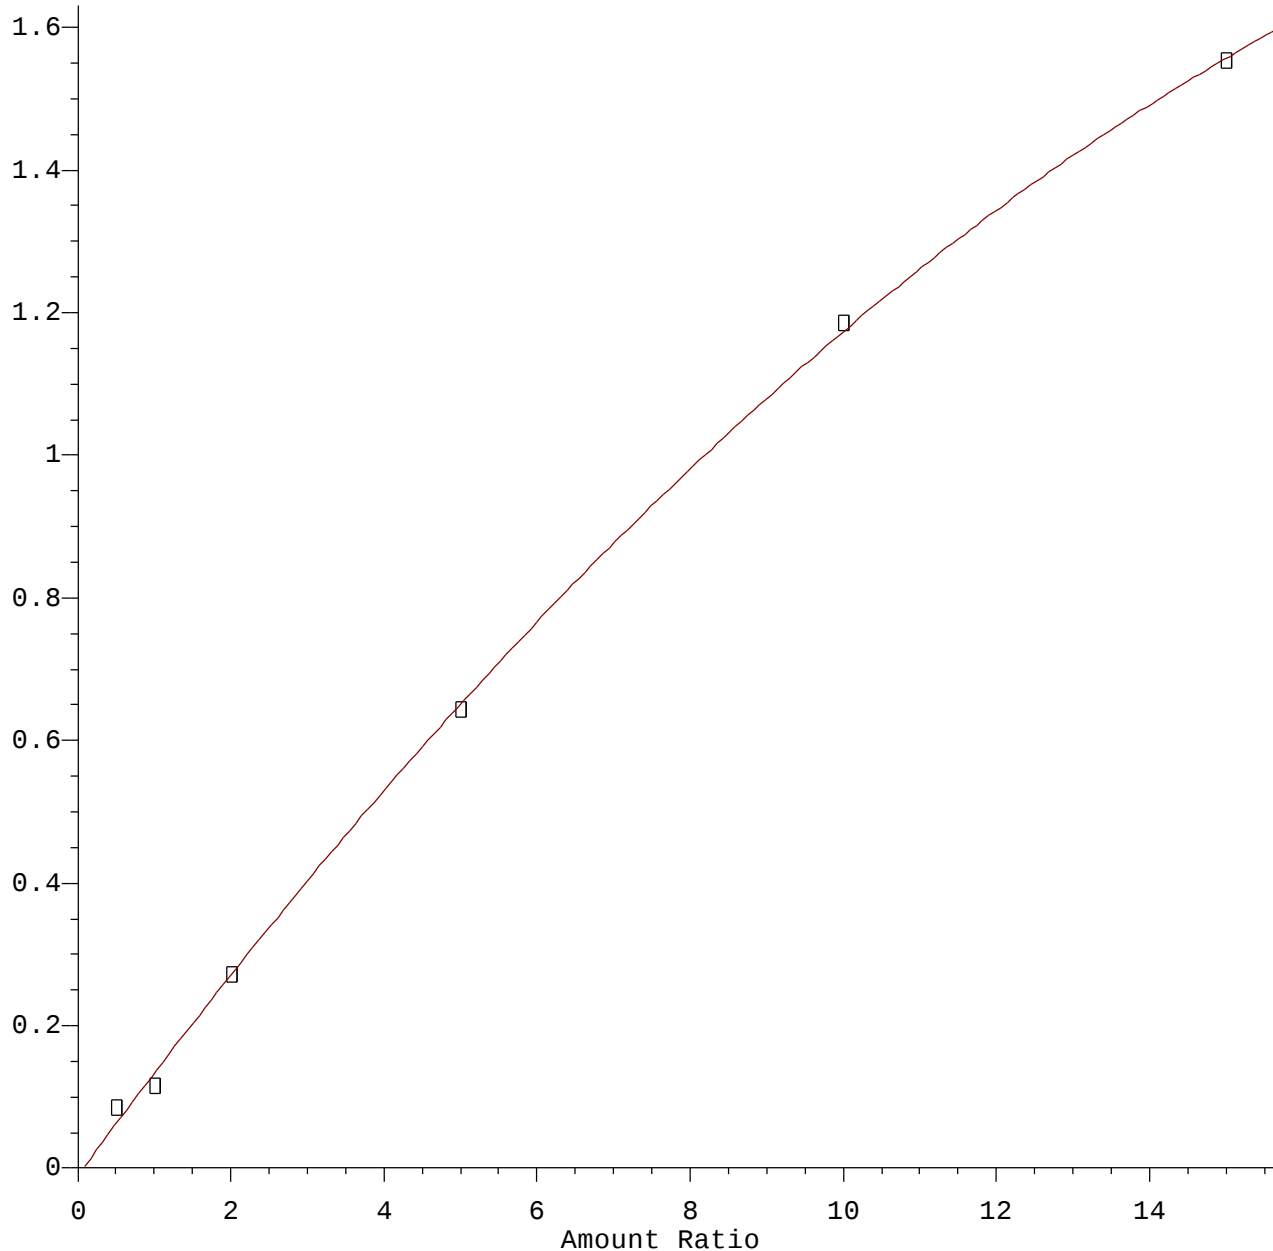

$R = -2.77e-003 A^2 + 1.46e-001 A - 9.68e-003$
Coef of Det (r^2) = 0.999 Curve Fit: Quadratic


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102918S.M
Calibration Table Last Updated: Thu Nov 01 15:08:55 2018

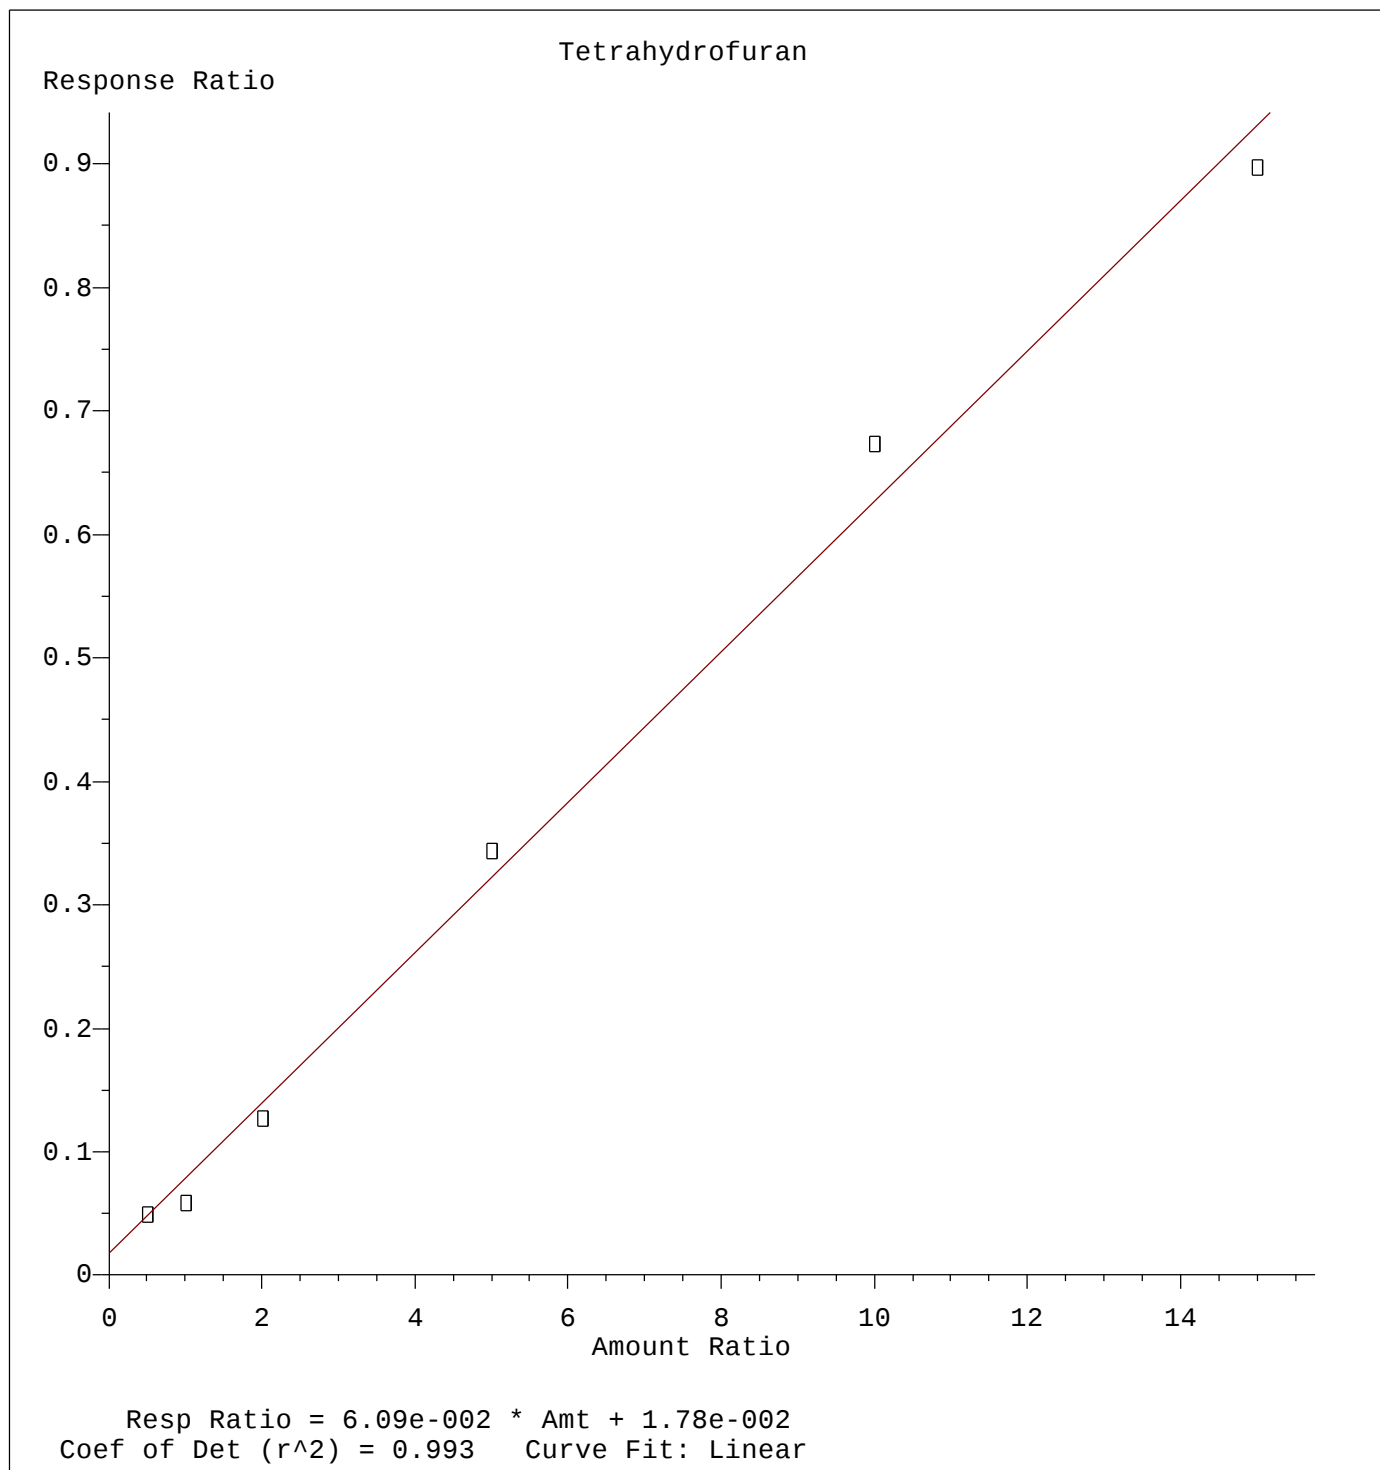

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102918S.M
Calibration Table Last Updated: Thu Nov 01 15:08:55 2018

2-Butanone

Response Ratio

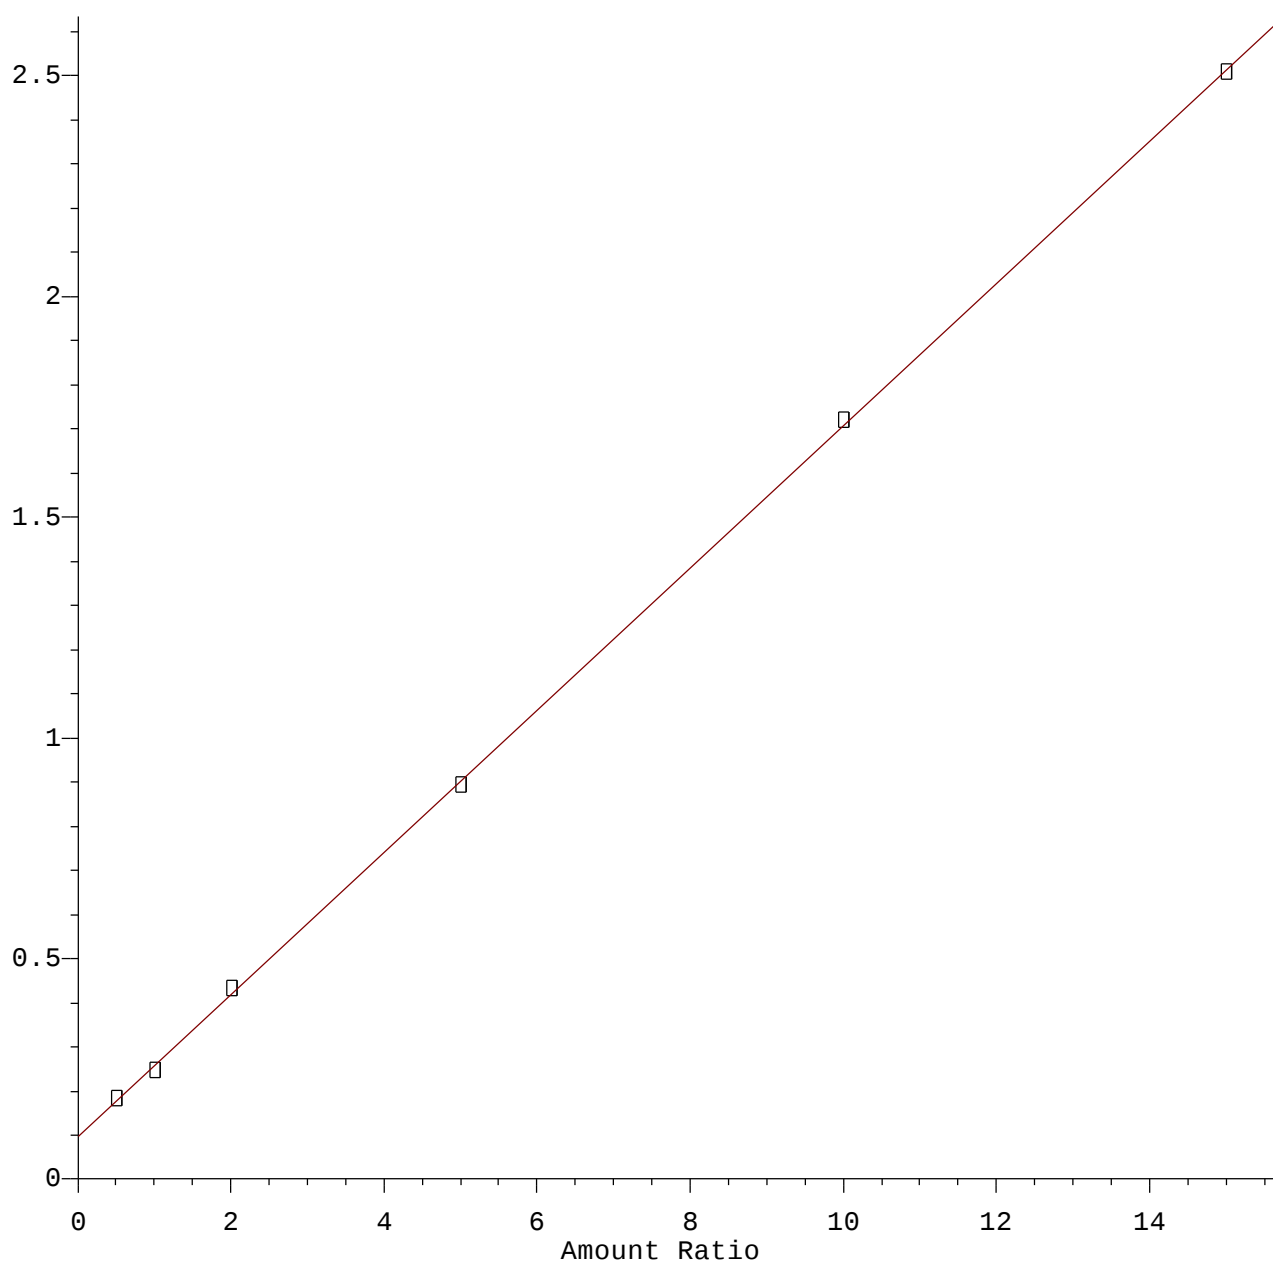


Resp Ratio = $1.61 \times 10^{-1} \times \text{Amt} + 9.73 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102918S.M
Calibration Table Last Updated: Thu Nov 01 15:08:55 2018


Methylene Chloride

Response Ratio

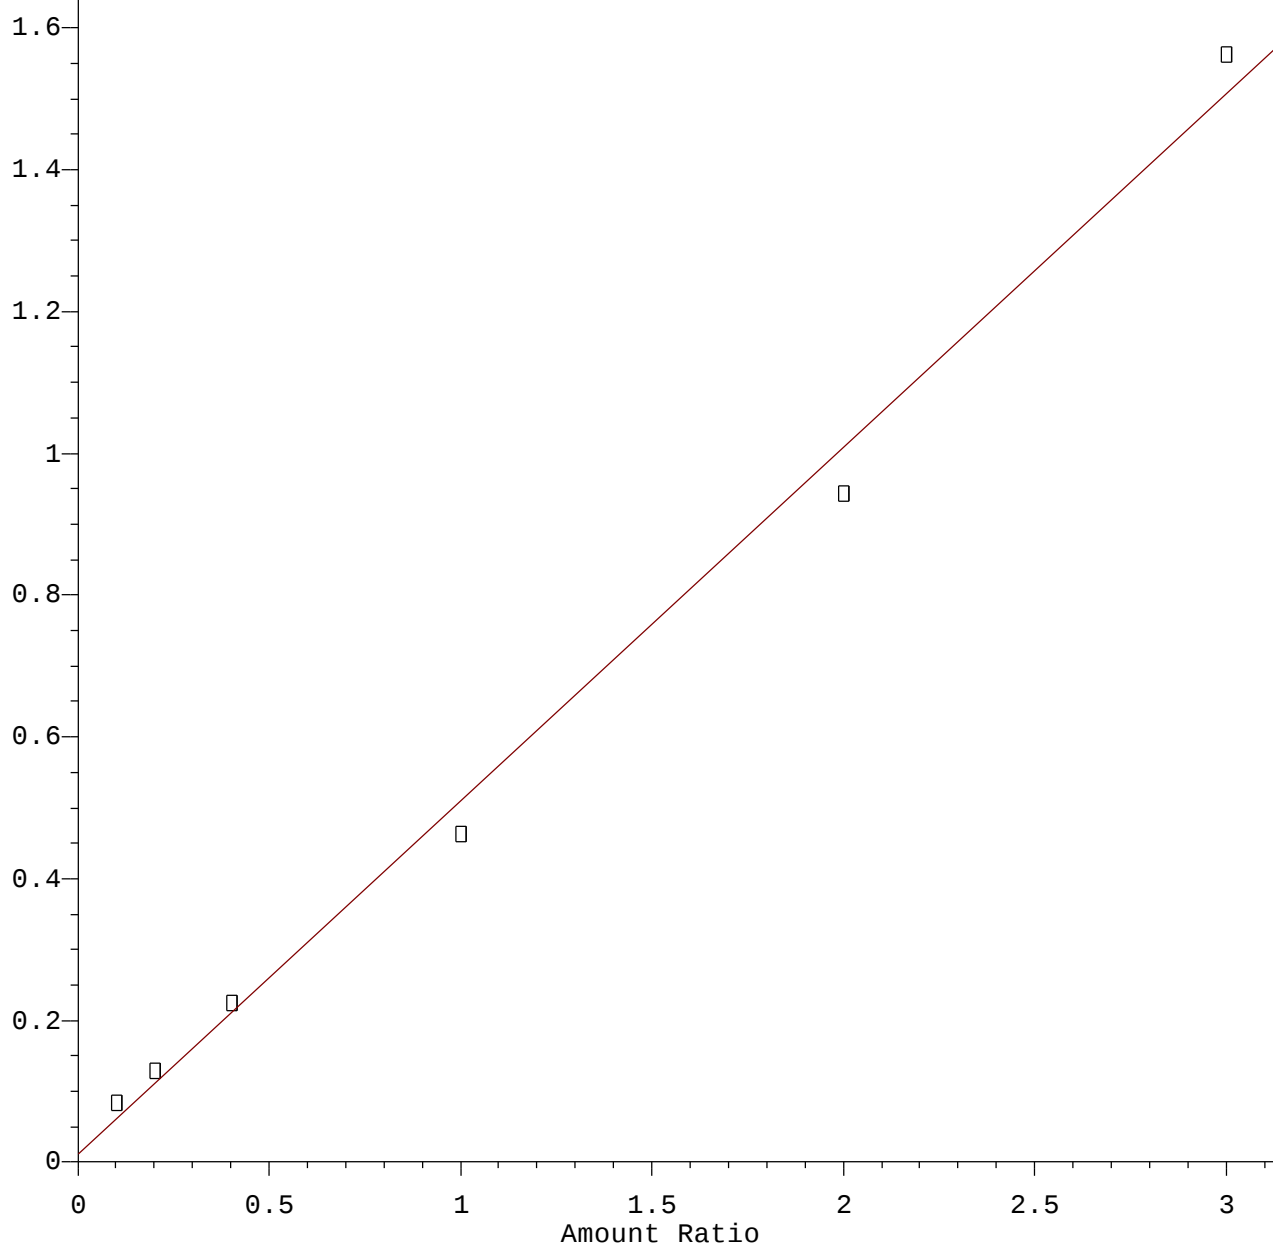


Resp Ratio = $4.99 \times 10^{-1} \times \text{Amt} + 1.00 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102918S.M
Calibration Table Last Updated: Thu Nov 01 15:08:55 2018

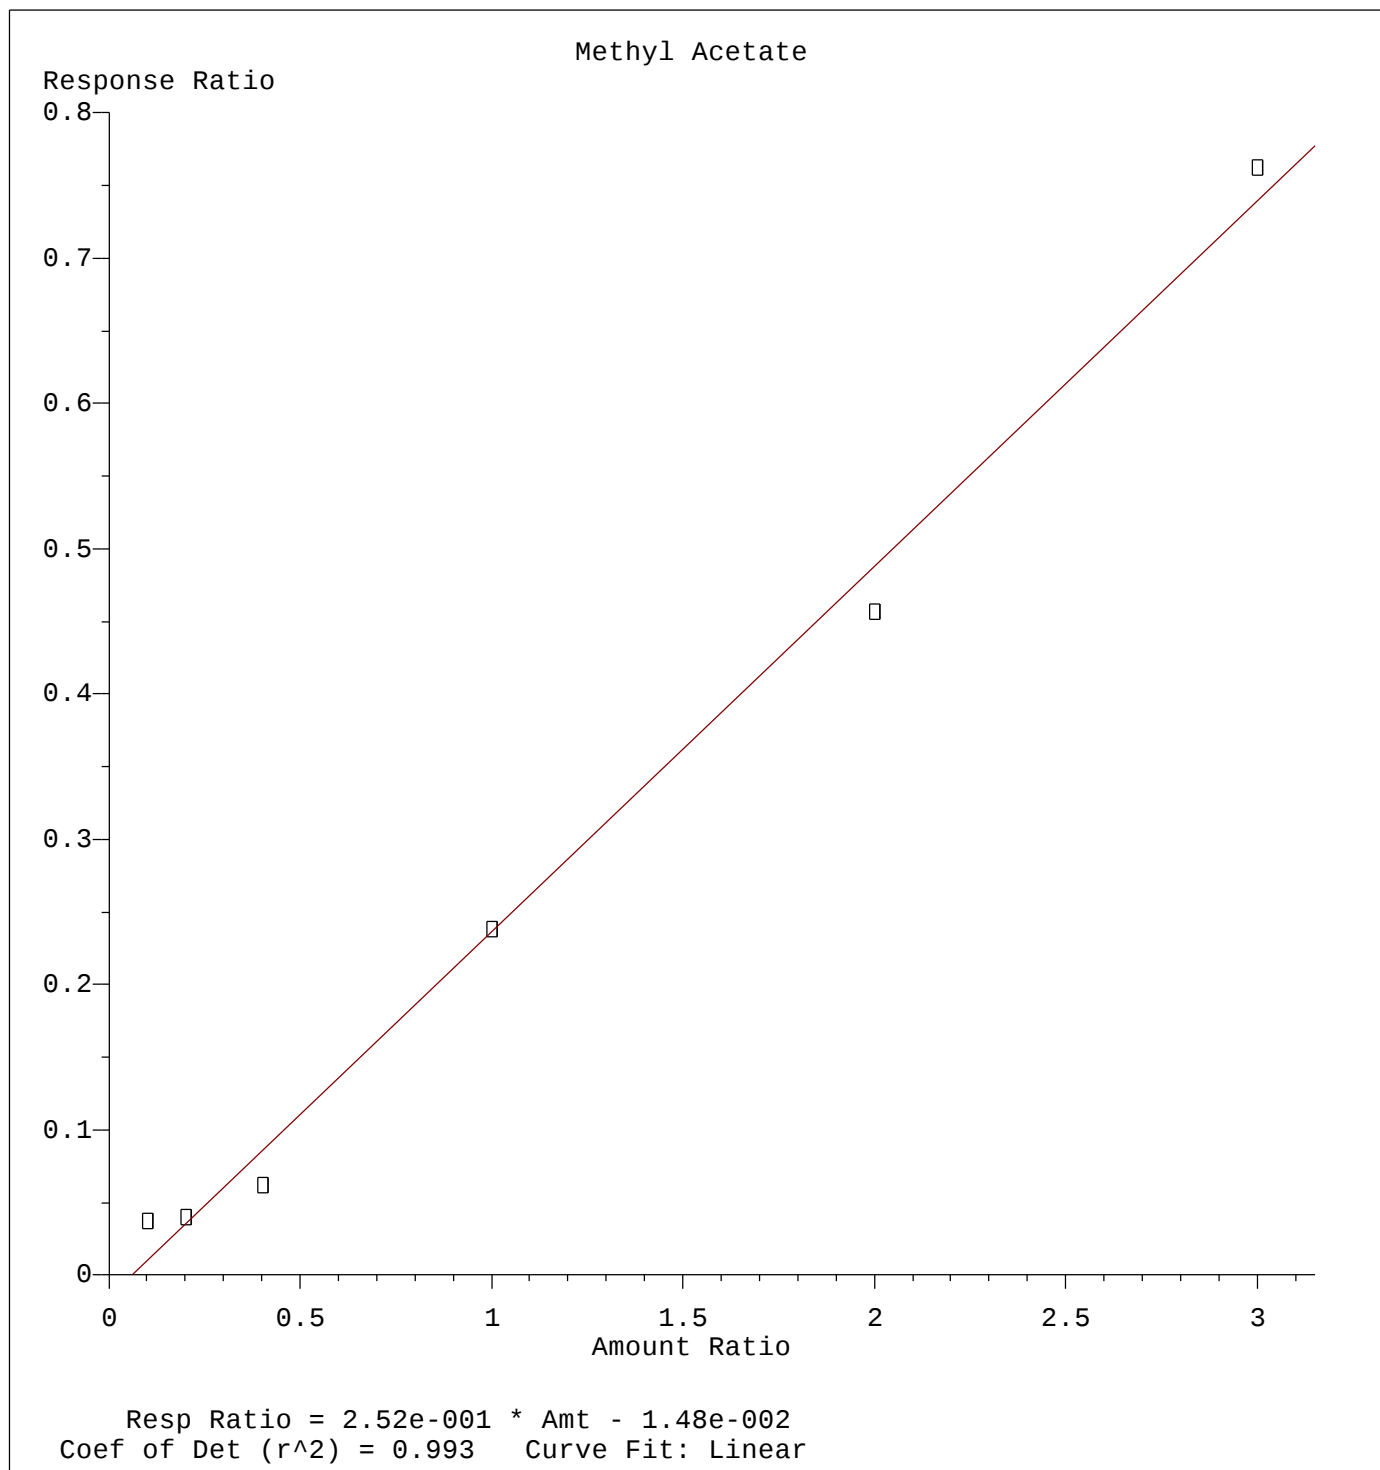


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102918S.M
Calibration Table Last Updated: Thu Nov 01 15:08:55 2018

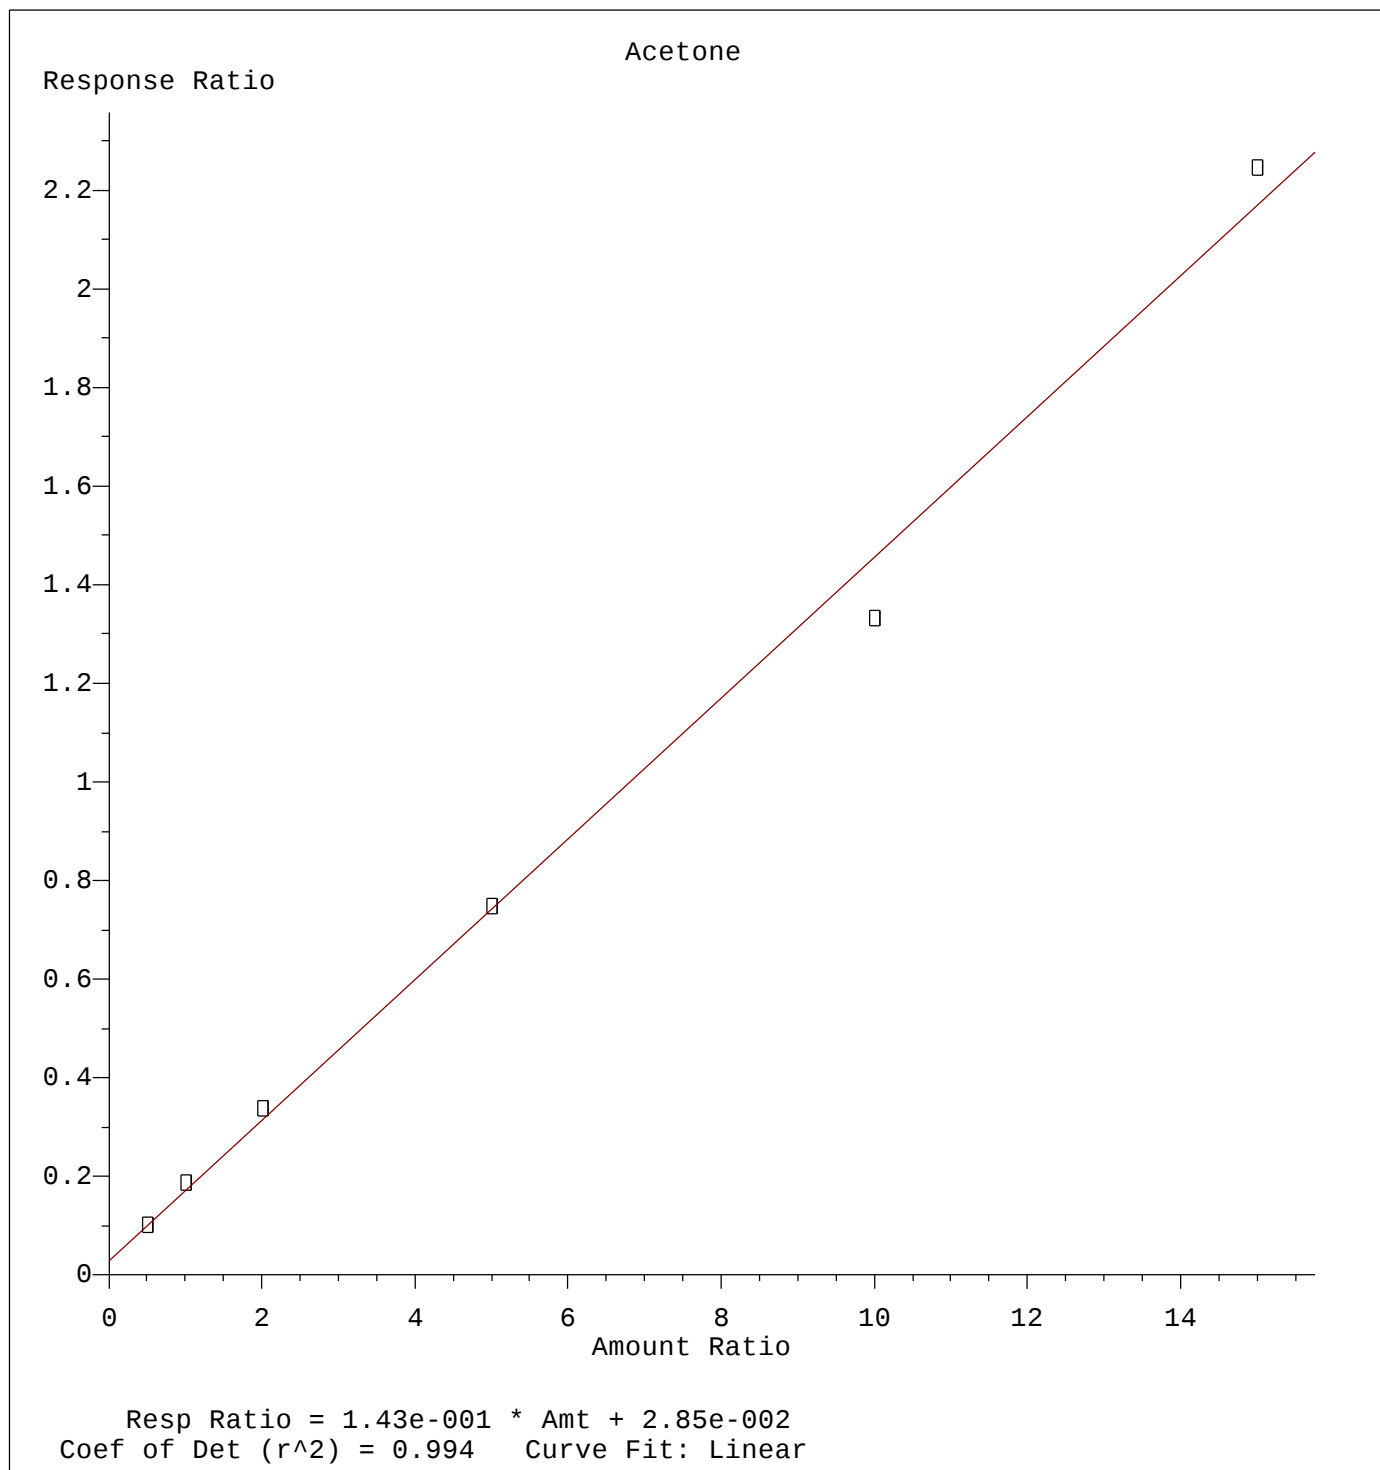

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102918S.M
Calibration Table Last Updated: Thu Nov 01 15:08:55 2018

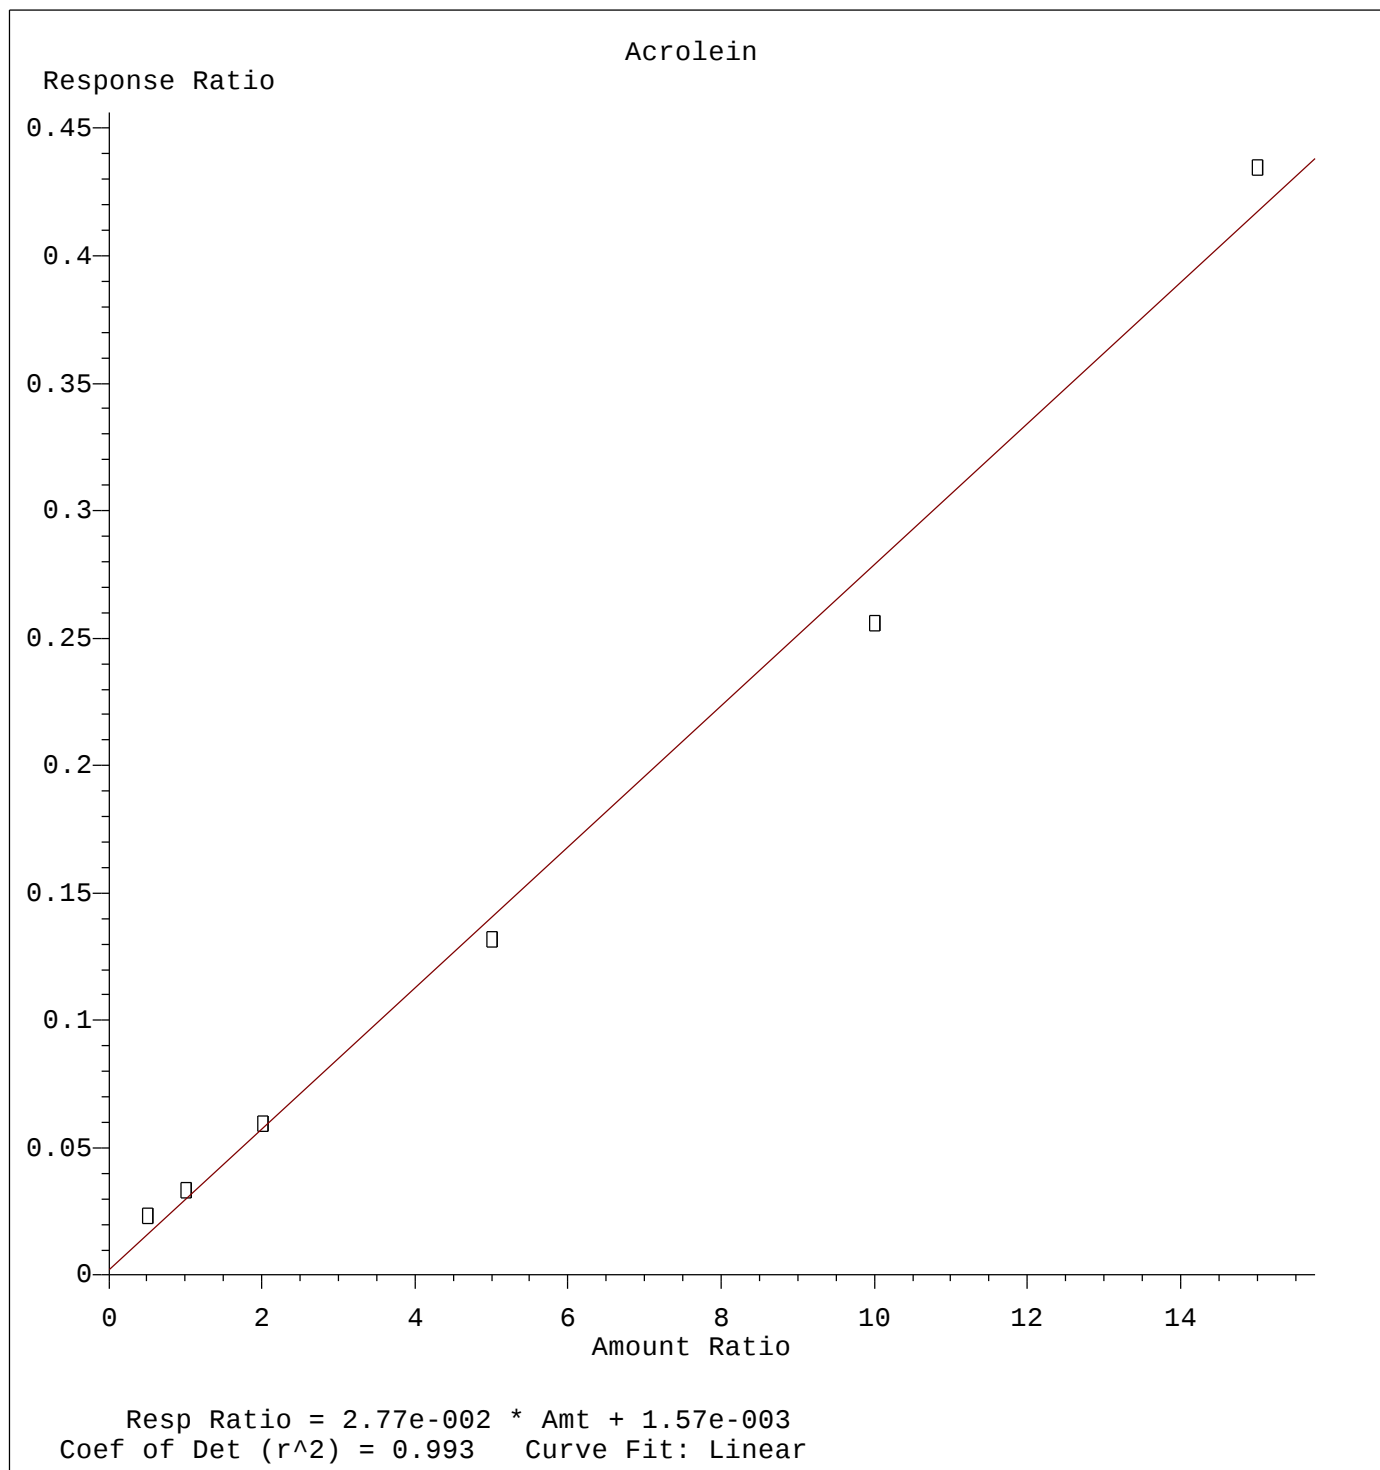


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102918S.M
Calibration Table Last Updated: Thu Nov 01 15:08:55 2018

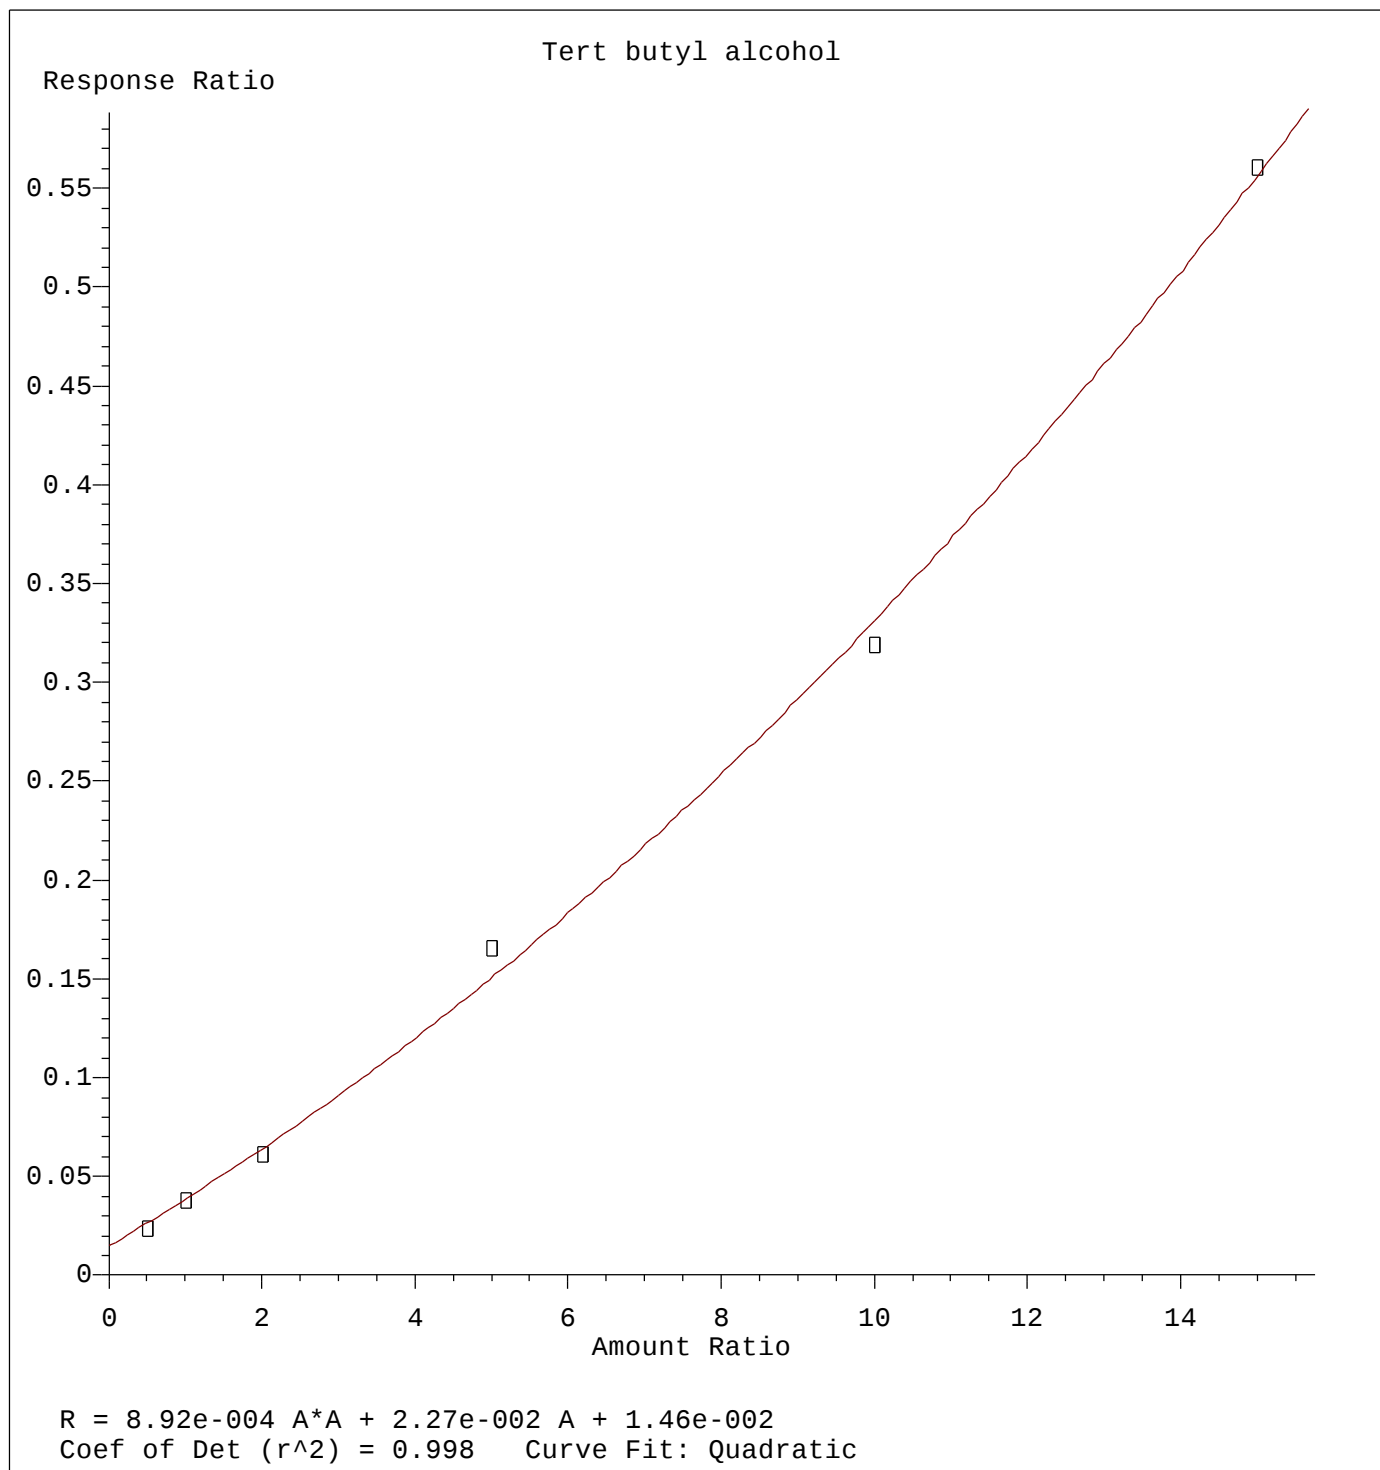

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102918S.M
Calibration Table Last Updated: Thu Nov 01 15:08:55 2018

1,1,2-Trichlorotrifluoroethane

Response Ratio

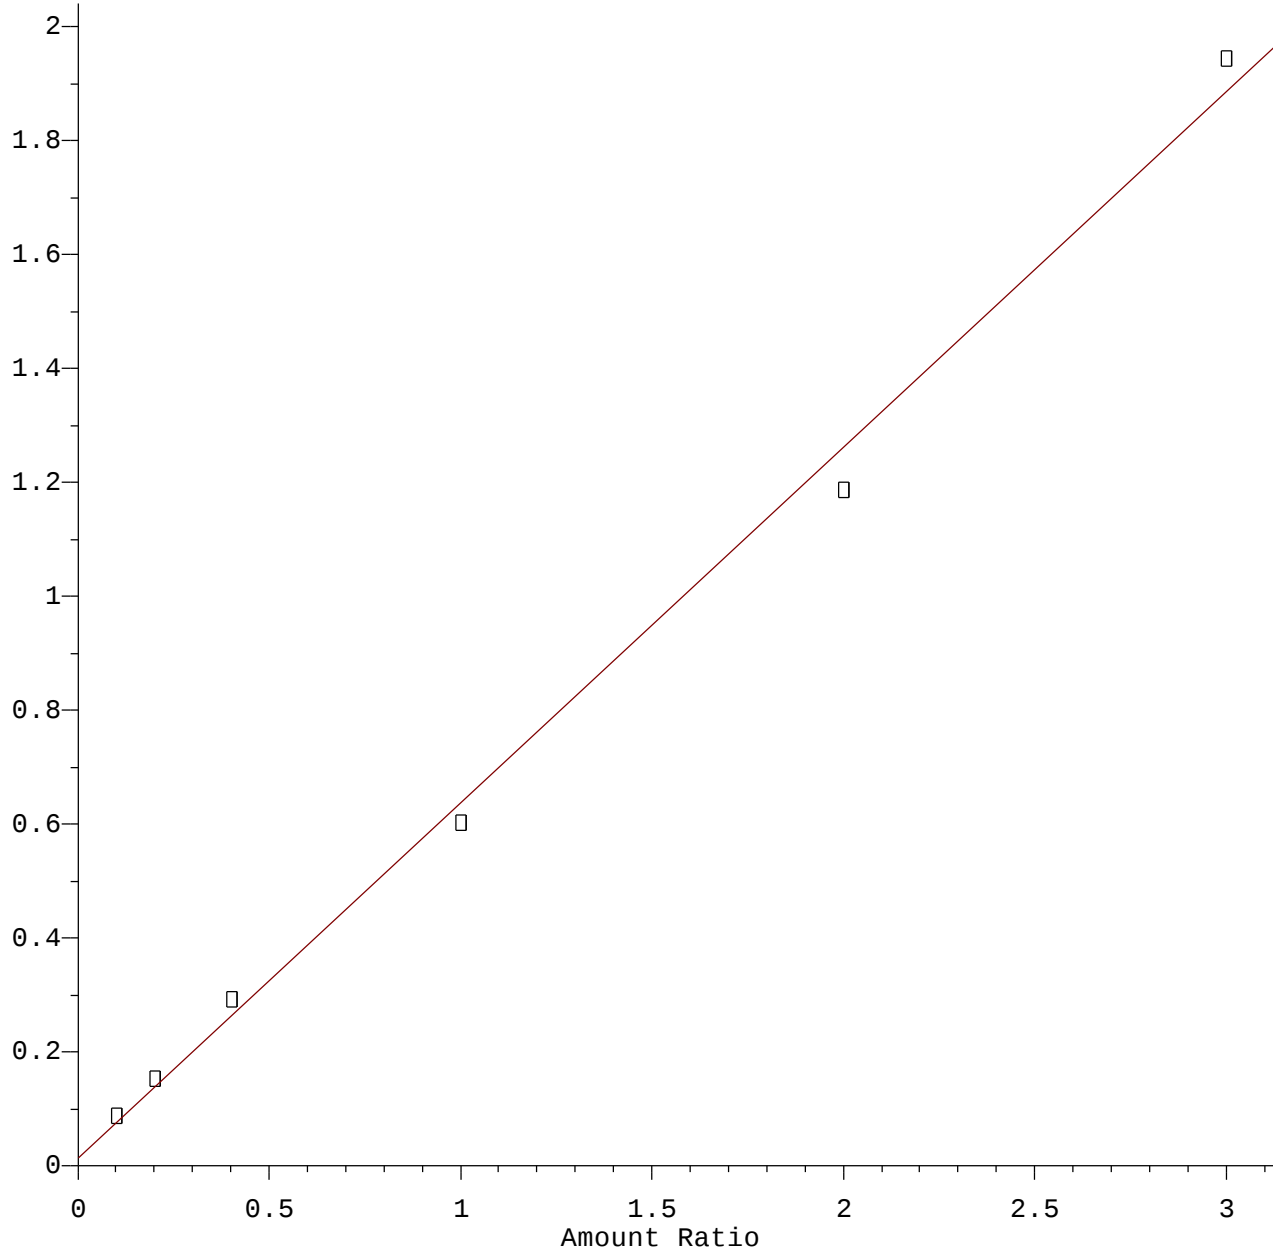


Resp Ratio = $6.24 \times 10^{-1} \times \text{Amt} + 1.40 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102918S.M
Calibration Table Last Updated: Thu Nov 01 15:08:55 2018

Chloromethane

Response Ratio

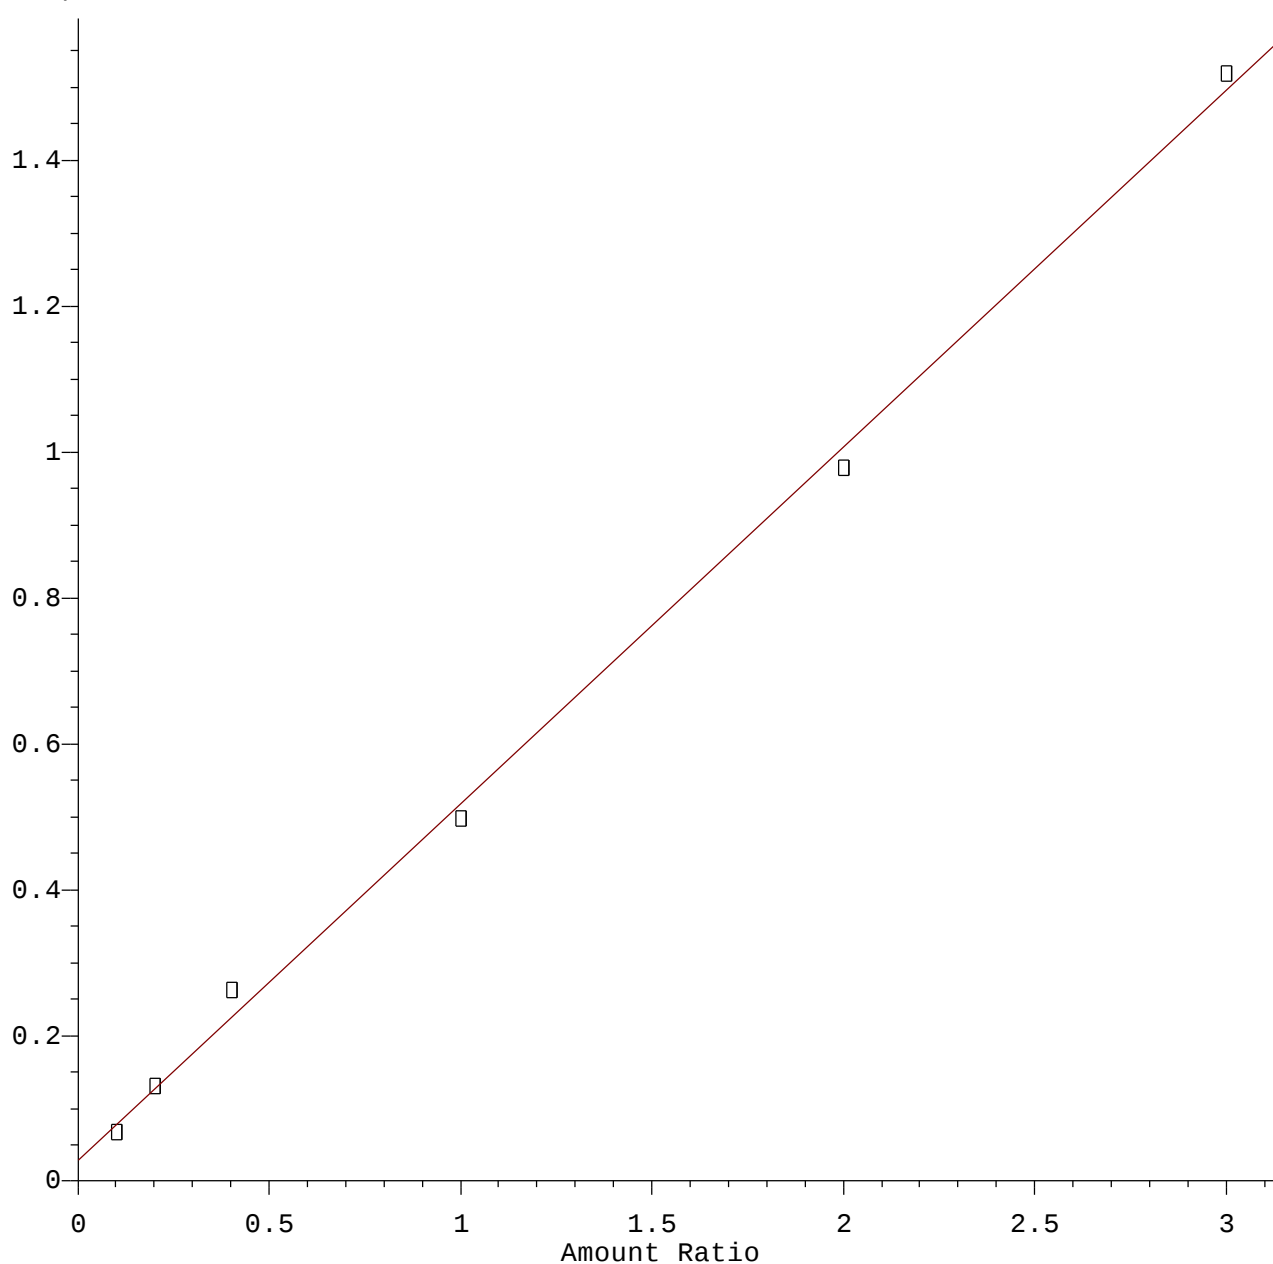

Resp Ratio = $4.89 \times 10^{-1} \times \text{Amt} + 2.89 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102918S.M
Calibration Table Last Updated: Thu Nov 01 15:08:55 2018