


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF102918\
Data File : VF060530.D
Acq On : 29 Oct 2018 15:15
Operator : VA/AP
Sample : BFB
Misc : 5.00/5mL/MSVOA F/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F102918S.M
Title : SW846 8260
Last Update : Tue Oct 30 05:31:58 2018

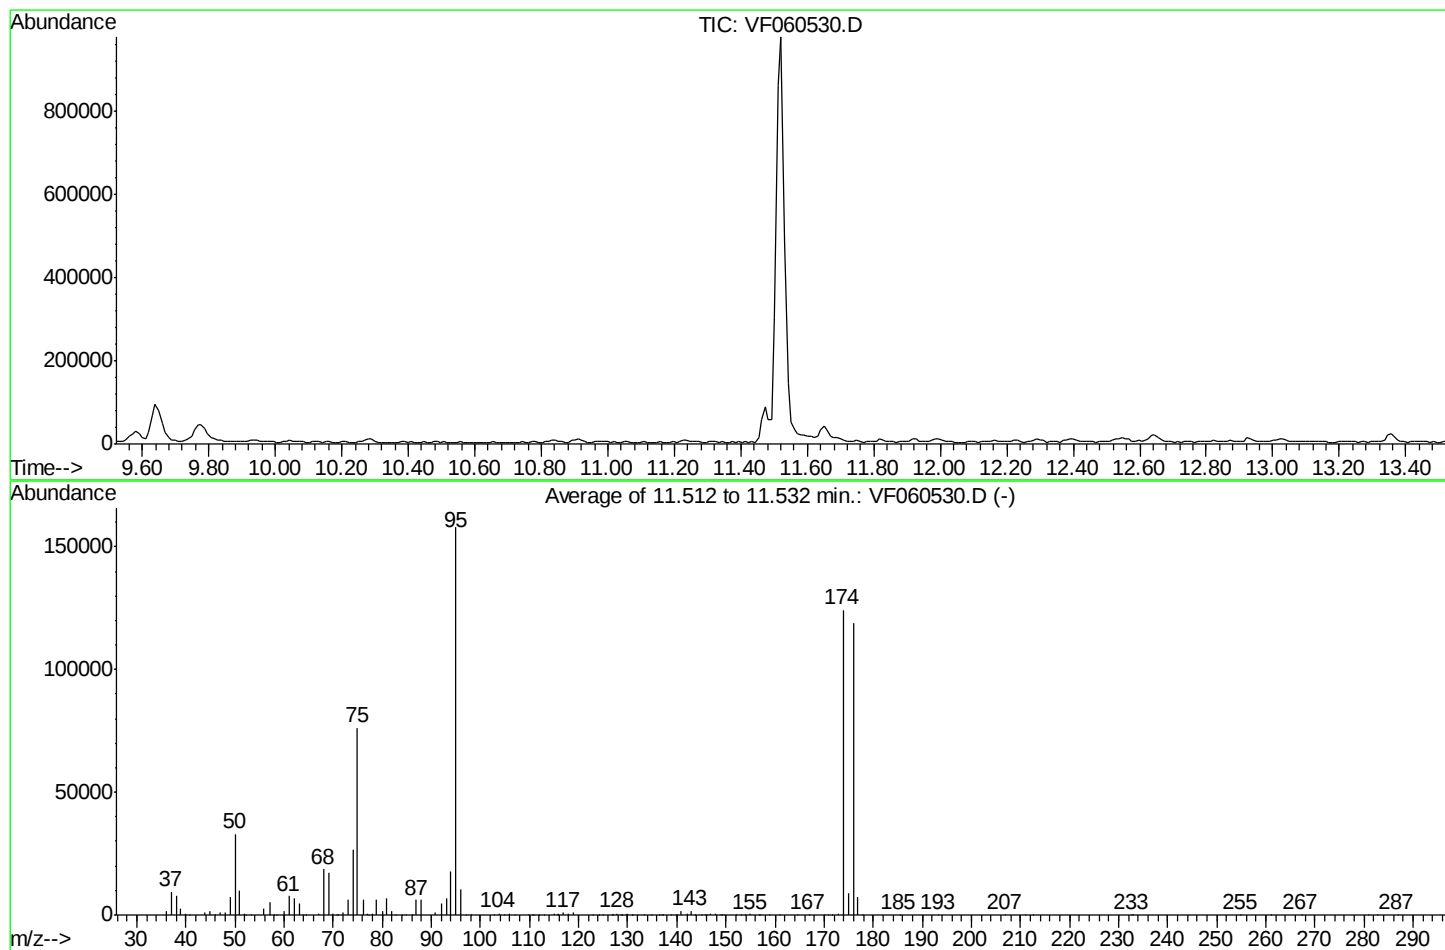

AutoFind: Scans 1104, 1105, 1106; Background Corrected with Scan 1098

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	33037	PASS
75	95	30	60	48.3	76330	PASS
95	95	100	100	100.0	157914	PASS
96	95	5	9	6.5	10213	PASS
173	174	0.00	2	0.3	330	PASS
174	95	50	100	78.7	124317	PASS
175	174	5	9	7.0	8672	PASS
176	174	95	101	95.8	119122	PASS
177	176	5	9	6.3	7521	PASS