


Instrument :
MSVOA_F
ClientSampleId :

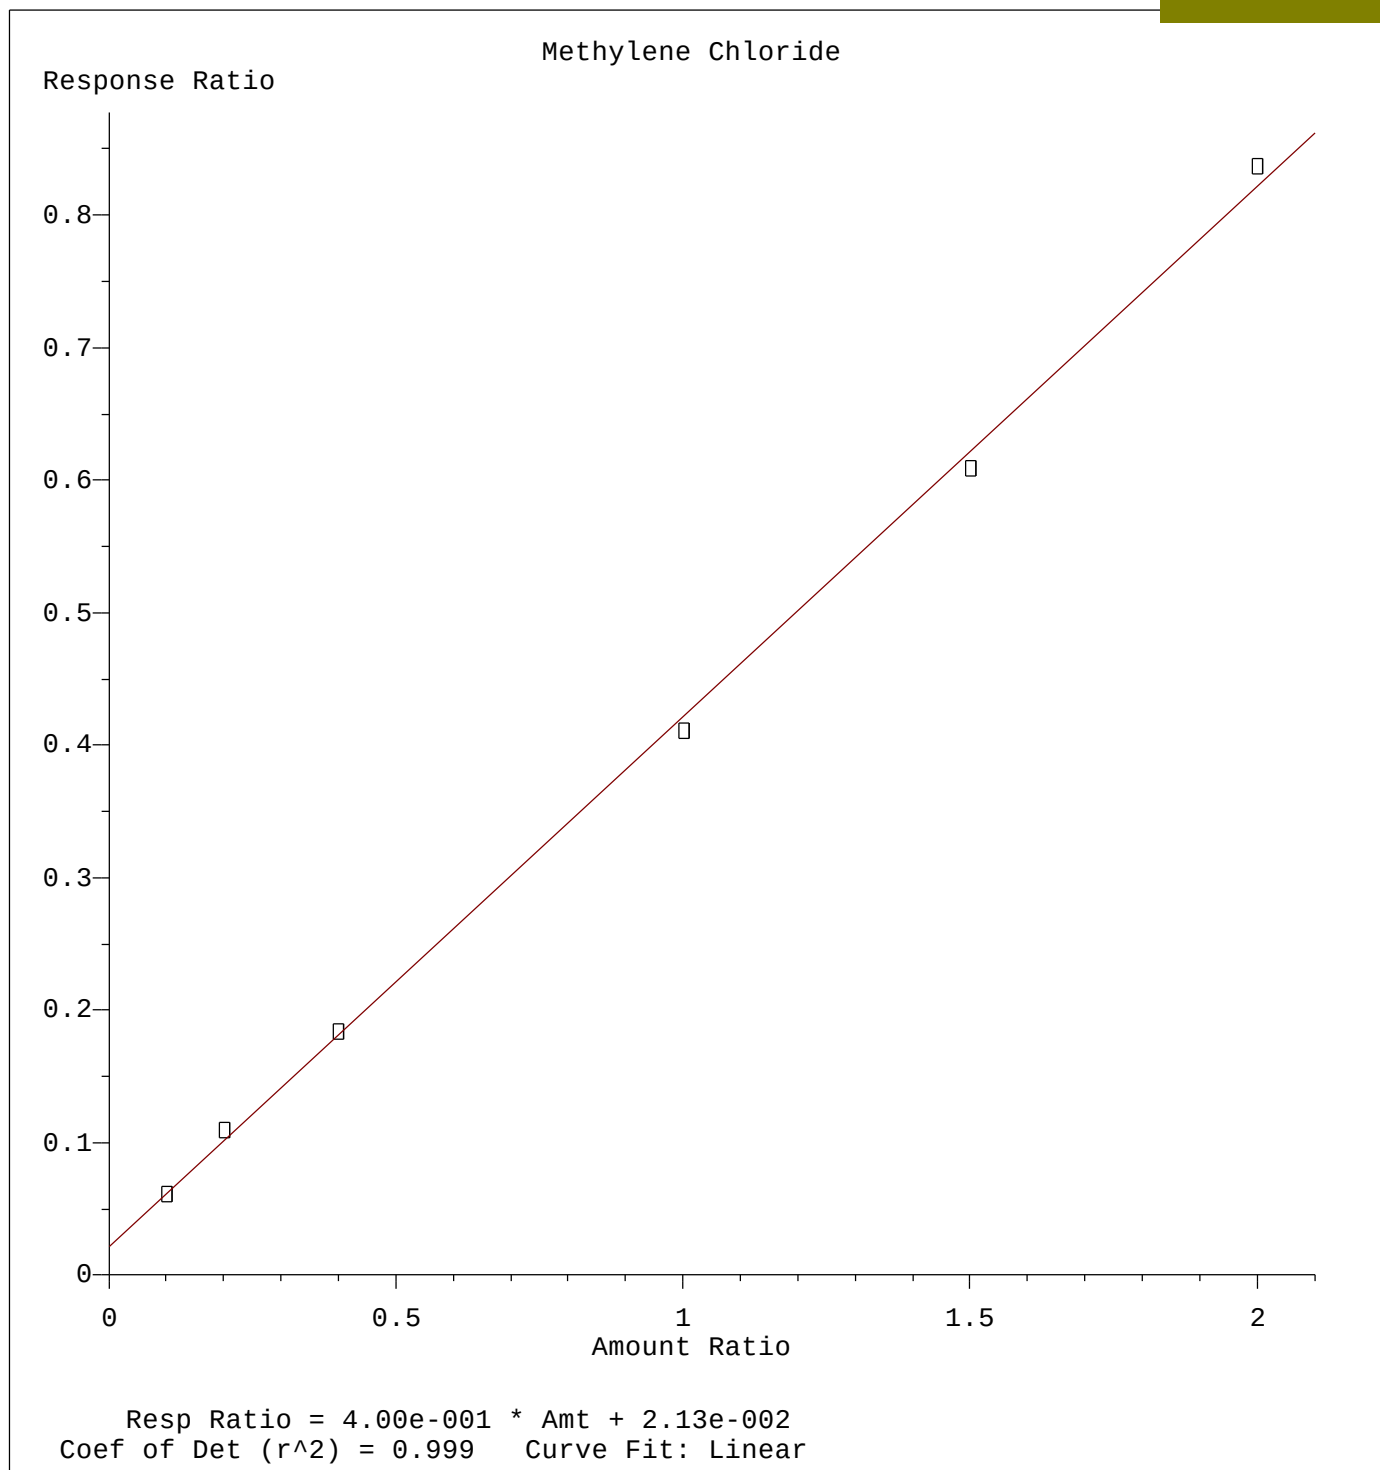

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F021319S.M
Calibration Table Last Updated: Thu Feb 14 03:27:56 2019