


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF021519\
Data File : VF061648.D
Acq On : 15 Feb 2019 9:39
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F021319S.M
Title : SW846 8260
Last Update : Thu Feb 14 03:27:56 2019

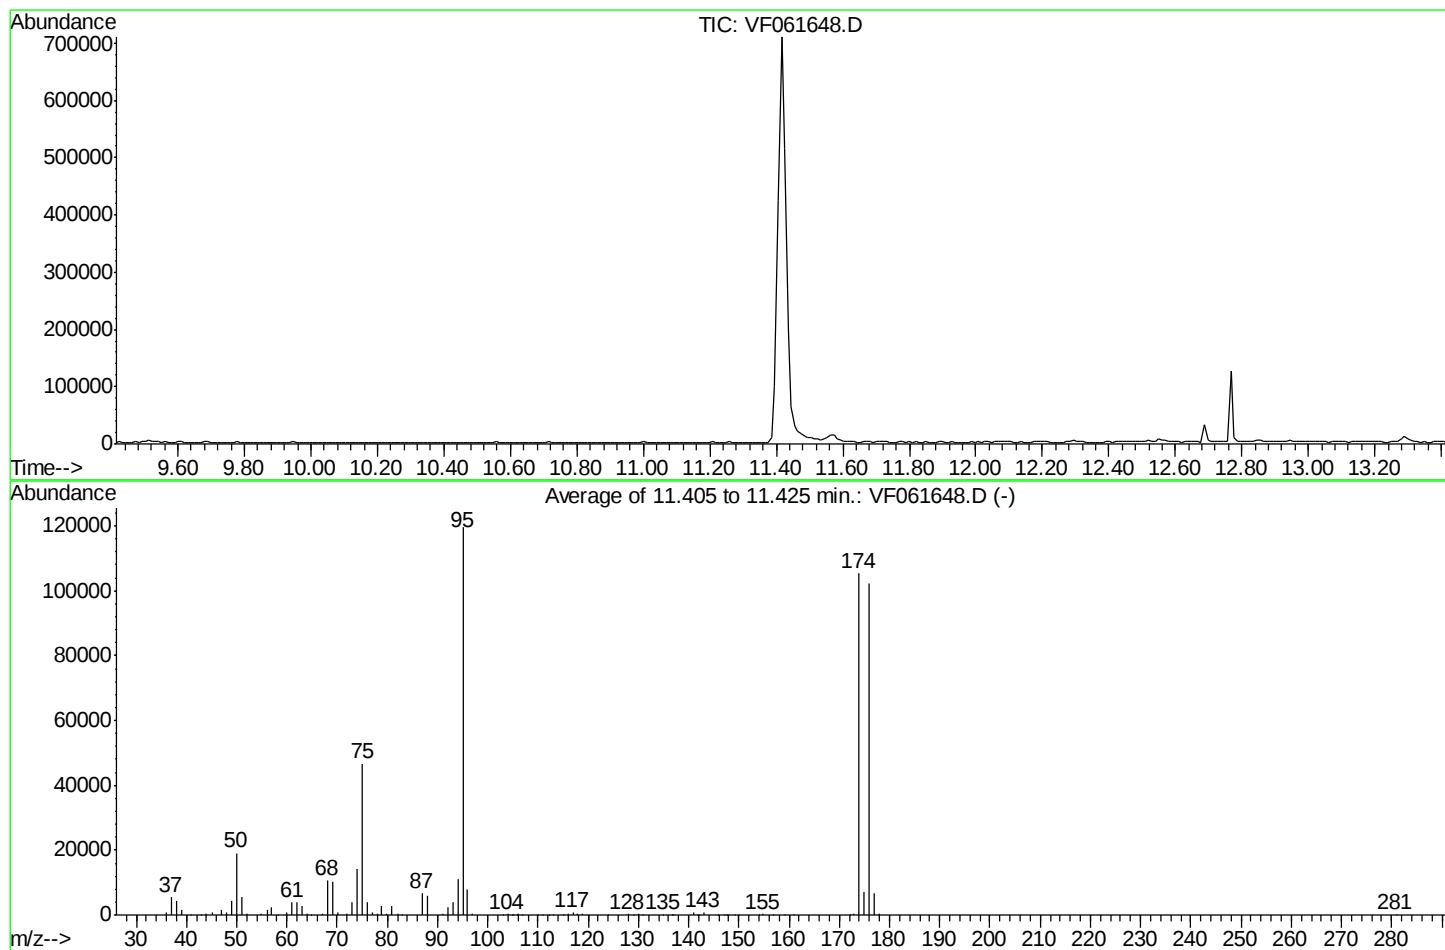

AutoFind: Scans 1093, 1094, 1095; Background Corrected with Scan 1085

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	18977	PASS
75	95	30	60	39.1	46741	PASS
95	95	100	100	100.0	119568	PASS
96	95	5	9	6.6	7888	PASS
173	174	0.00	2	0.4	417	PASS
174	95	50	100	88.1	105280	PASS
175	174	5	9	6.8	7199	PASS
176	174	95	101	97.1	102277	PASS
177	176	5	9	6.7	6825	PASS