


Data Path : W:\HPCHEM1\MSVOA_F\Data\VF022318\
Data File : VF056649.D
Acq On : 23 Feb 2018 9:14
Operator : JC/SY
Sample : BFB
Misc : 5.00g/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_F\METHODS\82F022018S.M
Title : SW846 8260
Last Update : Mon Feb 26 07:51:29 2018

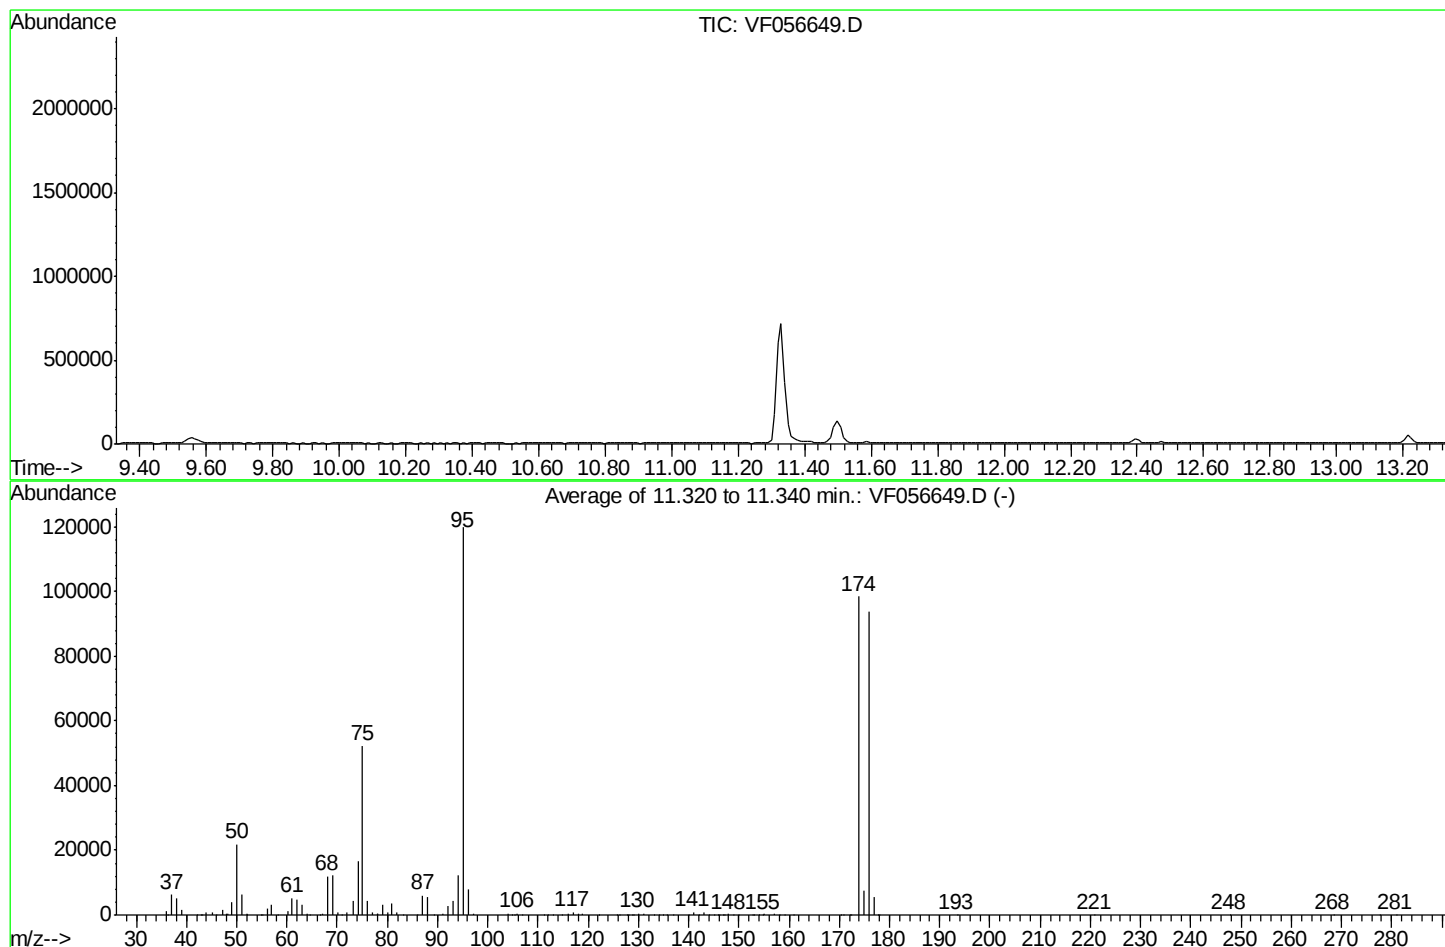

AutoFind: Scans 1094, 1095, 1096; Background Corrected with Scan 1089

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	21952	PASS
75	95	30	60	43.7	52344	PASS
95	95	100	100	100.0	119794	PASS
96	95	5	9	6.5	7742	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.1	98370	PASS
175	174	5	9	7.9	7725	PASS
176	174	95	101	95.3	93704	PASS
177	176	5	9	6.0	5590	PASS