


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF061918\
 Data File : VF059190.D
 Acq On : 19 Jun 2018 15:25
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F060618S.M
 Title : SW846 8260
 Last Update : Thu Jun 07 10:52:00 2018

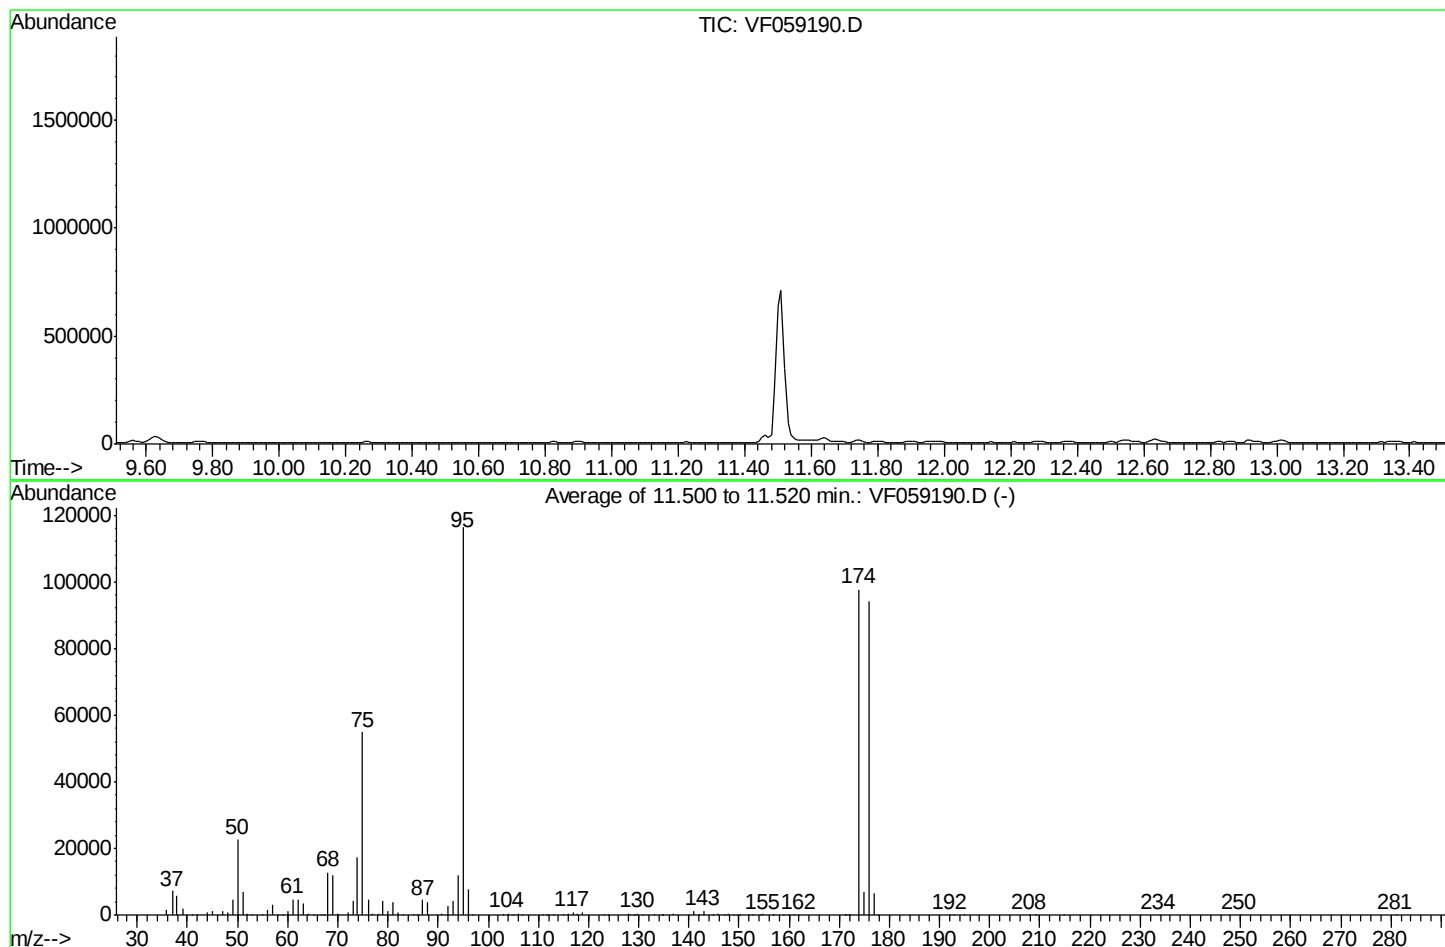

AutoFind: Scans 1113, 1114, 1115; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	22534	PASS
75	95	30	60	47.1	54792	PASS
95	95	100	100	100.0	116290	PASS
96	95	5	9	6.5	7505	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.9	97605	PASS
175	174	5	9	7.2	7046	PASS
176	174	95	101	96.2	93936	PASS
177	176	5	9	6.8	6415	PASS