


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF062018\
Data File : VF059228.D
Acq On : 20 Jun 2018 14:19
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F060618S.M
Title : SW846 8260
Last Update : Thu Jun 07 10:52:00 2018

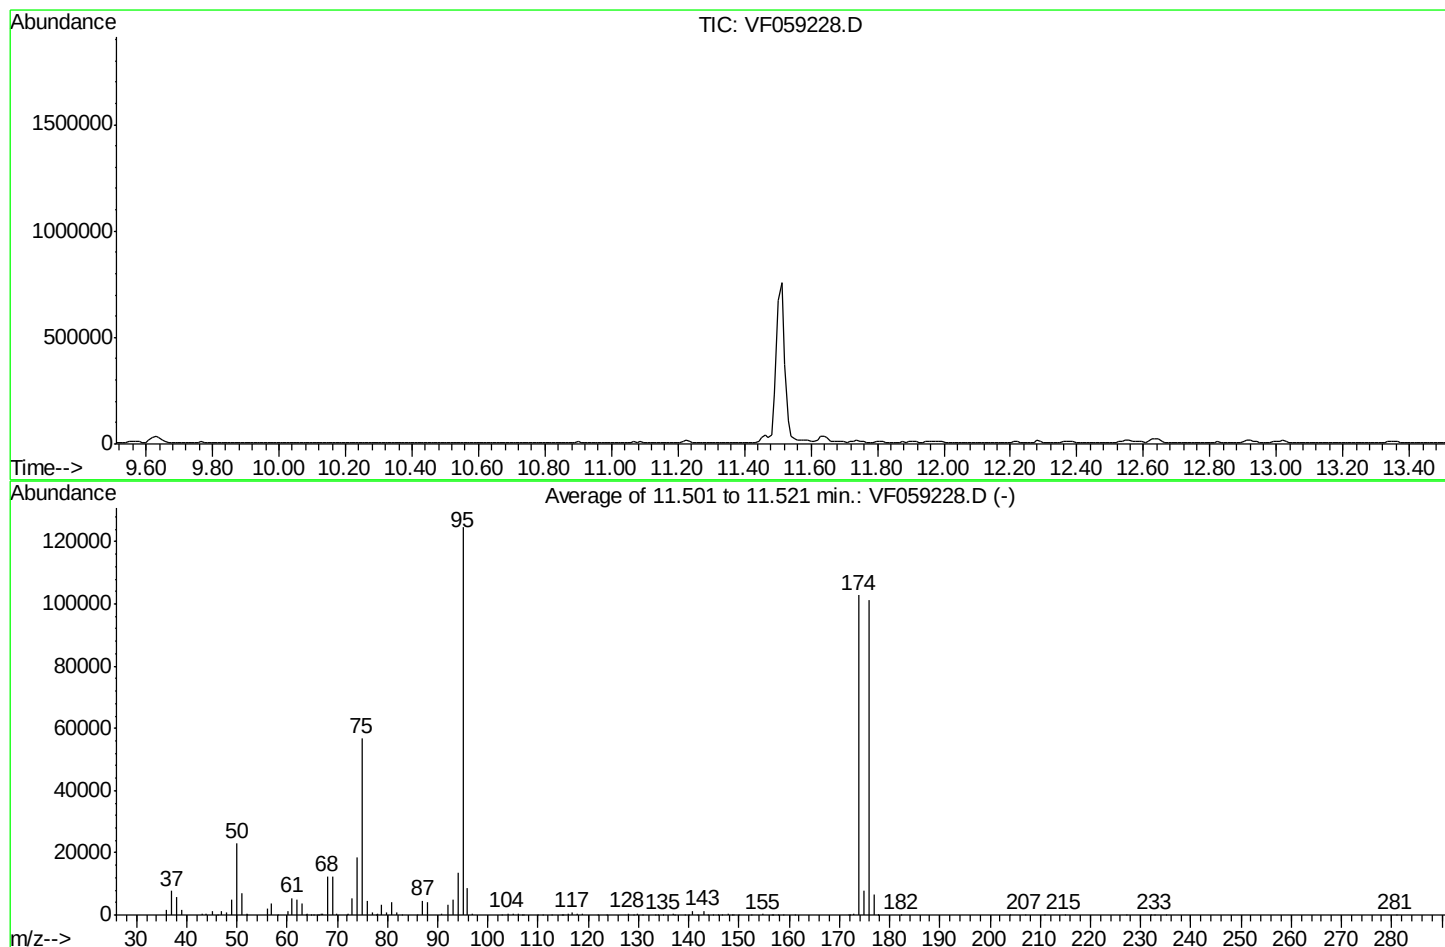

AutoFind: Scans 1113, 1114, 1115; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	22923	PASS
75	95	30	60	45.6	56776	PASS
95	95	100	100	100.0	124626	PASS
96	95	5	9	6.9	8559	PASS
173	174	0.00	2	0.3	295	PASS
174	95	50	100	82.4	102698	PASS
175	174	5	9	7.6	7796	PASS
176	174	95	101	98.6	101256	PASS
177	176	5	9	6.4	6510	PASS