


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF062018\
 Data File : VF059246.D
 Acq On : 21 Jun 2018 1:37
 Operator : VA/AP
 Sample : BFB
 Misc : 5.20µ/5mL/MSVOA-F/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F060618S.M
 Title : SW846 8260
 Last Update : Thu Jun 07 10:52:00 2018

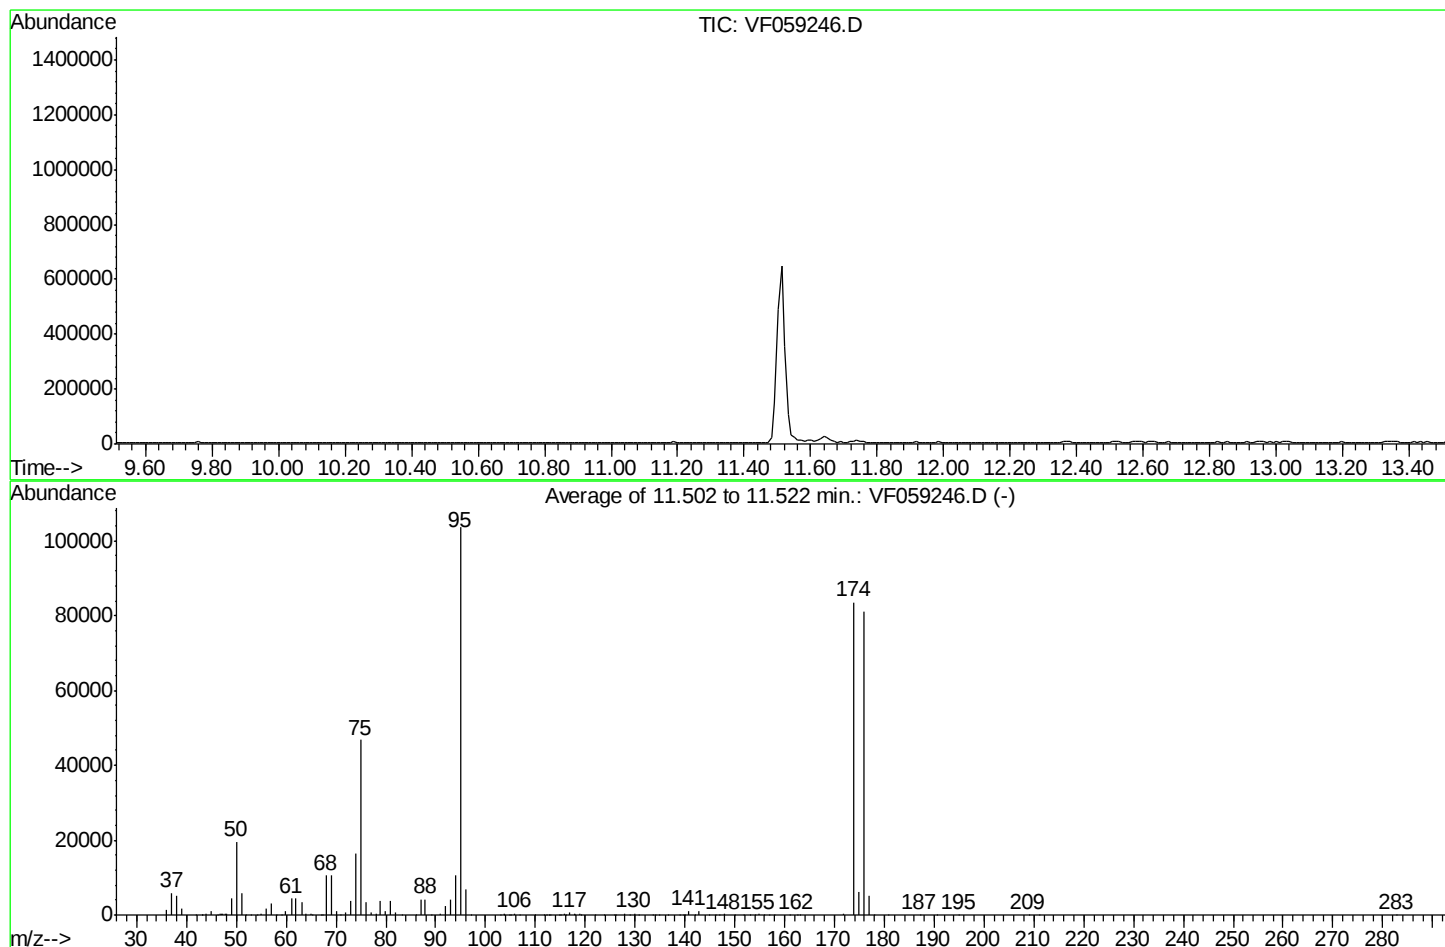

AutoFind: Scans 1113, 1114, 1115; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	19662	PASS
75	95	30	60	45.2	46864	PASS
95	95	100	100	100.0	103626	PASS
96	95	5	9	6.8	7001	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.7	83592	PASS
175	174	5	9	7.4	6211	PASS
176	174	95	101	97.1	81157	PASS
177	176	5	9	6.4	5233	PASS