


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF071718\
Data File : VF059509.D
Acq On : 17 Jul 2018 15:33
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F071718S.M
Title : SW846 8260
Last Update : Wed Jul 18 04:09:10 2018

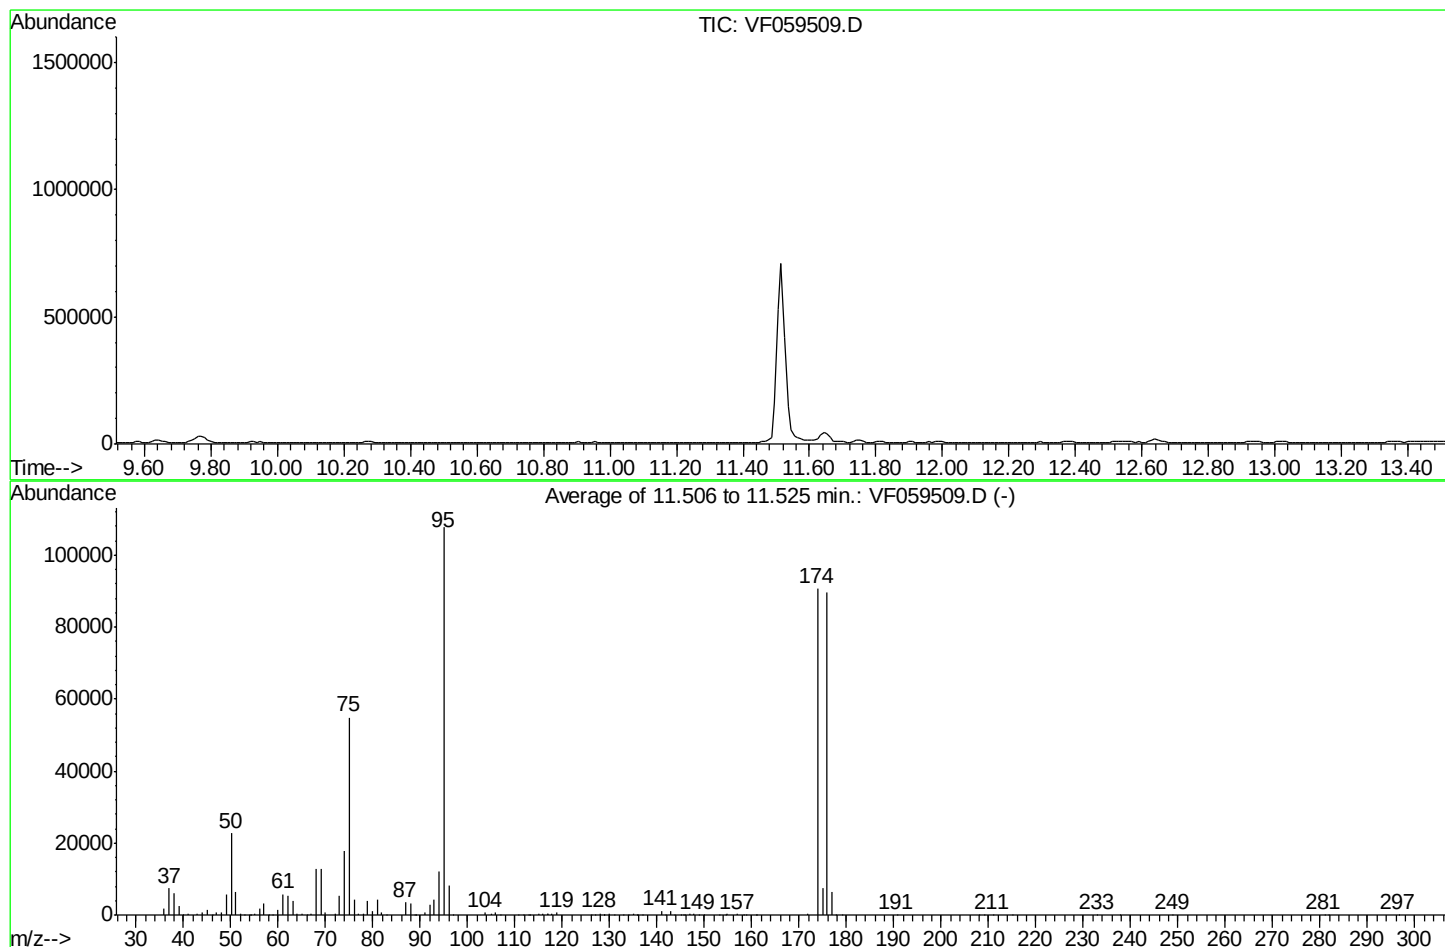

AutoFind: Scans 1113, 1114, 1115; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	22687	PASS
75	95	30	60	50.9	54839	PASS
95	95	100	100	100.0	107754	PASS
96	95	5	9	7.6	8182	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.1	90669	PASS
175	174	5	9	8.1	7329	PASS
176	174	95	101	99.0	89786	PASS
177	176	5	9	7.0	6256	PASS