


Data Path : W:\HPCHEM1\MSVOA F\DATA\VF091615\
Data File : VF045387.D
Acq On : 16 Sep 2015 10:47
Operator : FY/SY
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_F\METHODS\82F091615S.M
Title : SW846 8260
Last Update : Wed Sep 16 16:04:03 2015

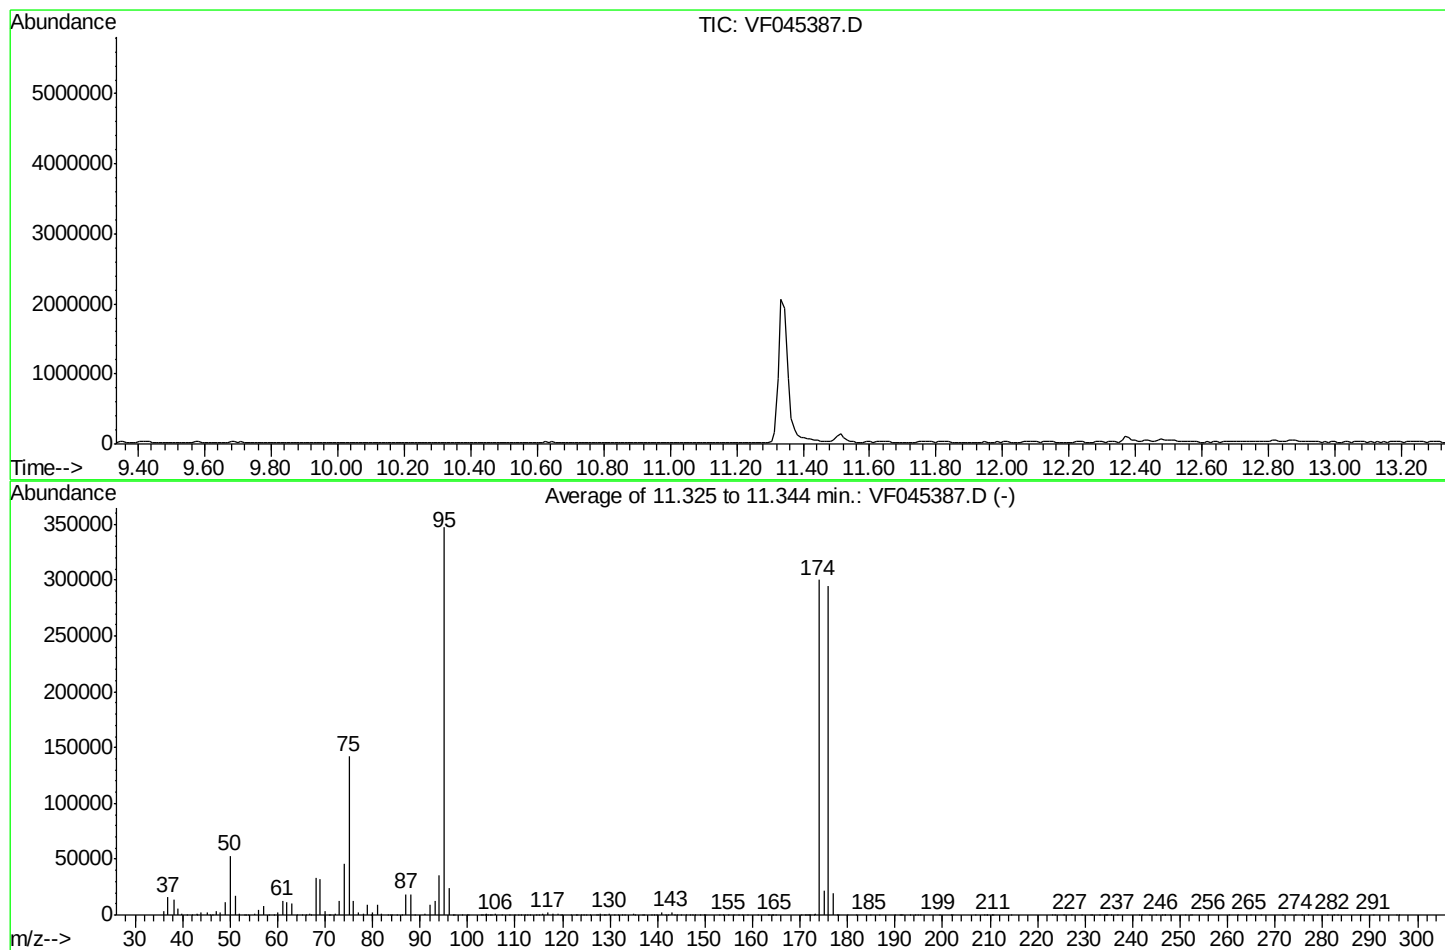

AutoFind: Scans 1095, 1096, 1097; Background Corrected with Scan 1090

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	53098	PASS
75	95	30	60	40.8	141872	PASS
95	95	100	100	100.0	347349	PASS
96	95	5	9	7.0	24243	PASS
173	174	0.00	2	0.3	803	PASS
174	95	50	100	86.4	300224	PASS
175	174	5	9	7.4	22237	PASS
176	174	95	101	98.1	294648	PASS
177	176	5	9	6.6	19453	PASS