


Data Path : W:\HPCHEM1\MSVOA F\DATA\VF091715\
Data File : VF045404.D
Acq On : 17 Sep 2015 10:13
Operator : FY/SY
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_F\METHODS\82F091615S.M
Title : SW846 8260
Last Update : Wed Sep 16 16:04:03 2015

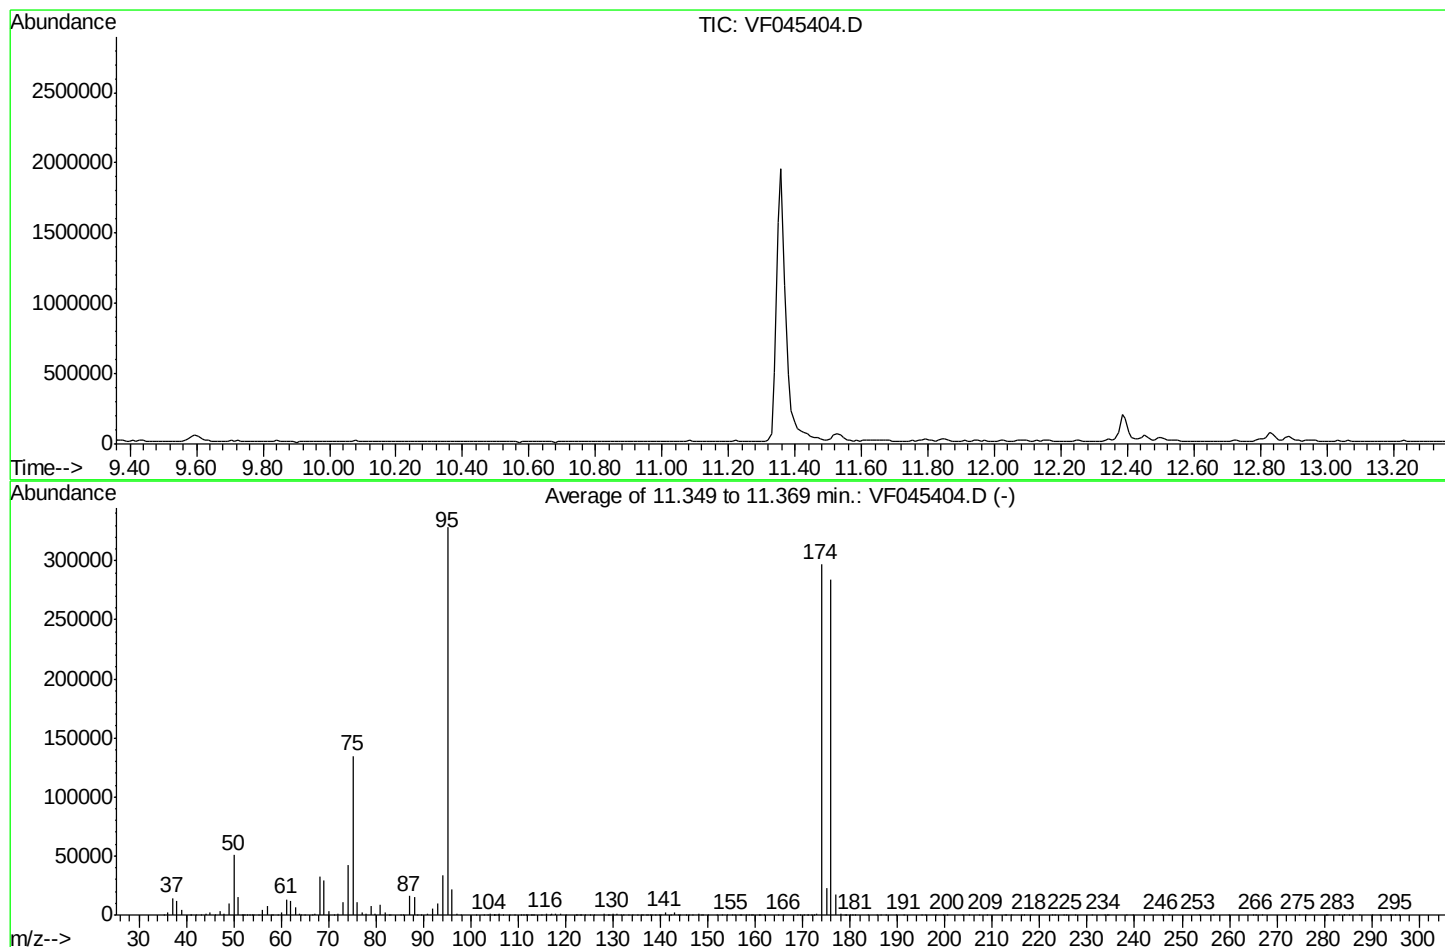

AutoFind: Scans 1098, 1099, 1100; Background Corrected with Scan 1092

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	50848	PASS
75	95	30	60	41.0	134768	PASS
95	95	100	100	100.0	328384	PASS
96	95	5	9	6.6	21640	PASS
173	174	0.00	2	0.5	1404	PASS
174	95	50	100	90.4	296938	PASS
175	174	5	9	7.6	22482	PASS
176	174	95	101	95.5	283669	PASS
177	176	5	9	6.2	17485	PASS