


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF121218\  
Data File : VF060995.D  
Acq On : 12 Dec 2018 14:34  
Operator : VA/AP  
Sample : BFB  
Misc : 5.00µ/5mL/MSVOA-F/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_F  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F112618S.M  
Title : SW846 8260  
Last Update : Tue Nov 27 01:36:26 2018

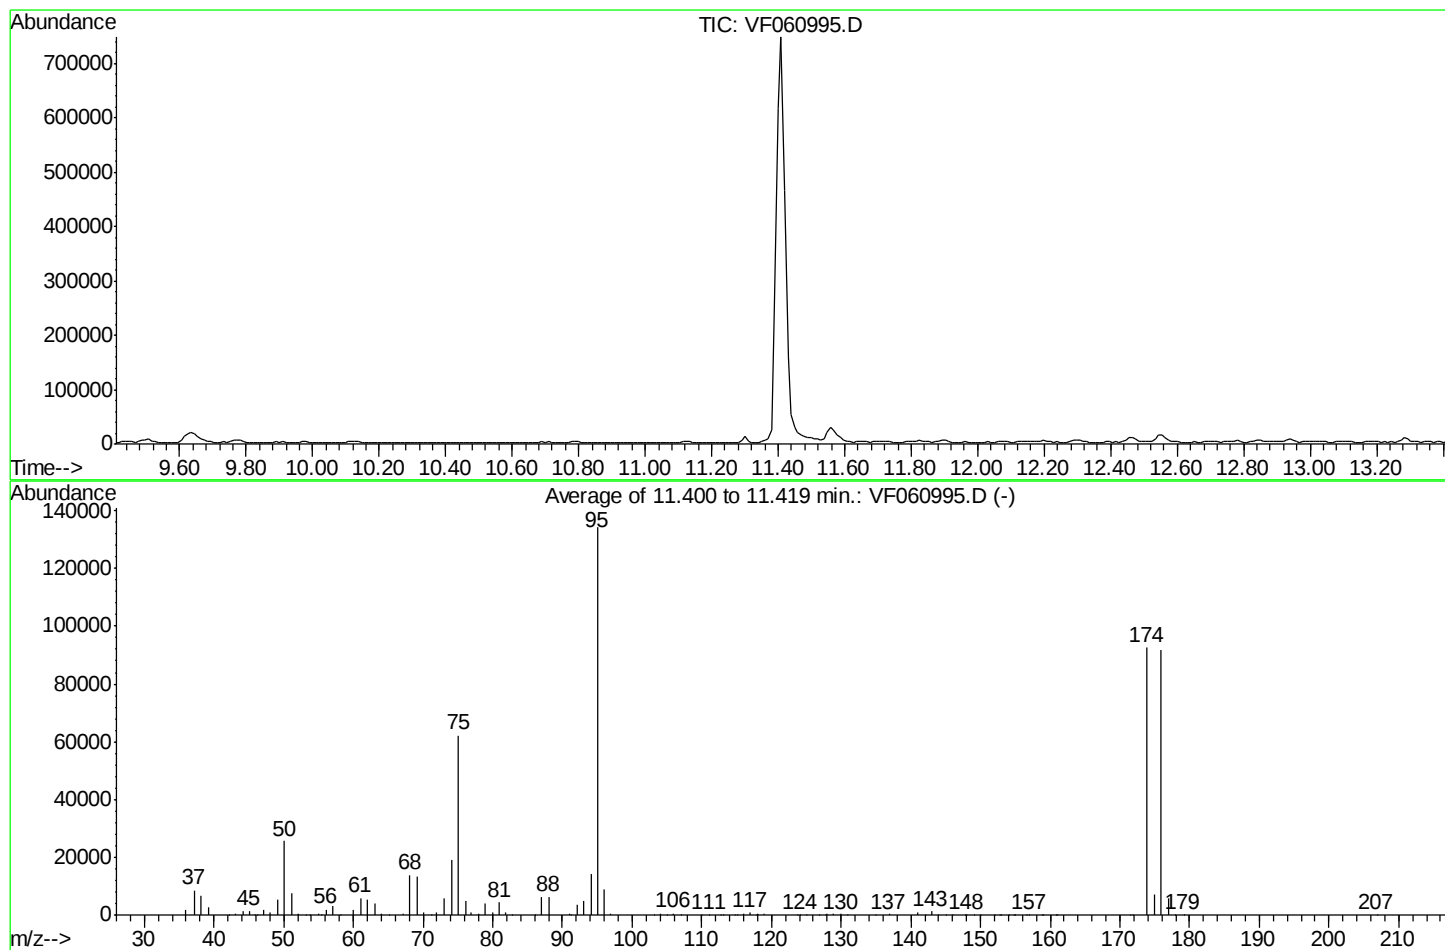

AutoFind: Scans 1092, 1093, 1094; Background Corrected with Scan 1086

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.1      | 25621   | PASS             |
| 75          | 95           | 30           | 60           | 46.3      | 62144   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 134240  | PASS             |
| 96          | 95           | 5            | 9            | 6.7       | 8949    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 69.0      | 92608   | PASS             |
| 175         | 174          | 5            | 9            | 7.6       | 7035    | PASS             |
| 176         | 174          | 95           | 101          | 99.3      | 91973   | PASS             |
| 177         | 176          | 5            | 9            | 6.4       | 5859    | PASS             |