


Data Path : W:\HPCHEM1\MSVOA H\DATA\VH091715\
Data File : VH057068.D
Acq On : 17 Sep 2015 15:58
Operator : SY/FY
Sample : BFB
Misc : 5mL/MSVOA H/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_H
ClientSampleId :
BFB

Integration File: rteint.p

Method : W:\HPCHEM1\MSVOA_H\METHODS\82H091715W.M
Title : SW846 8260
Last Update : Fri Sep 18 15:34:01 2015

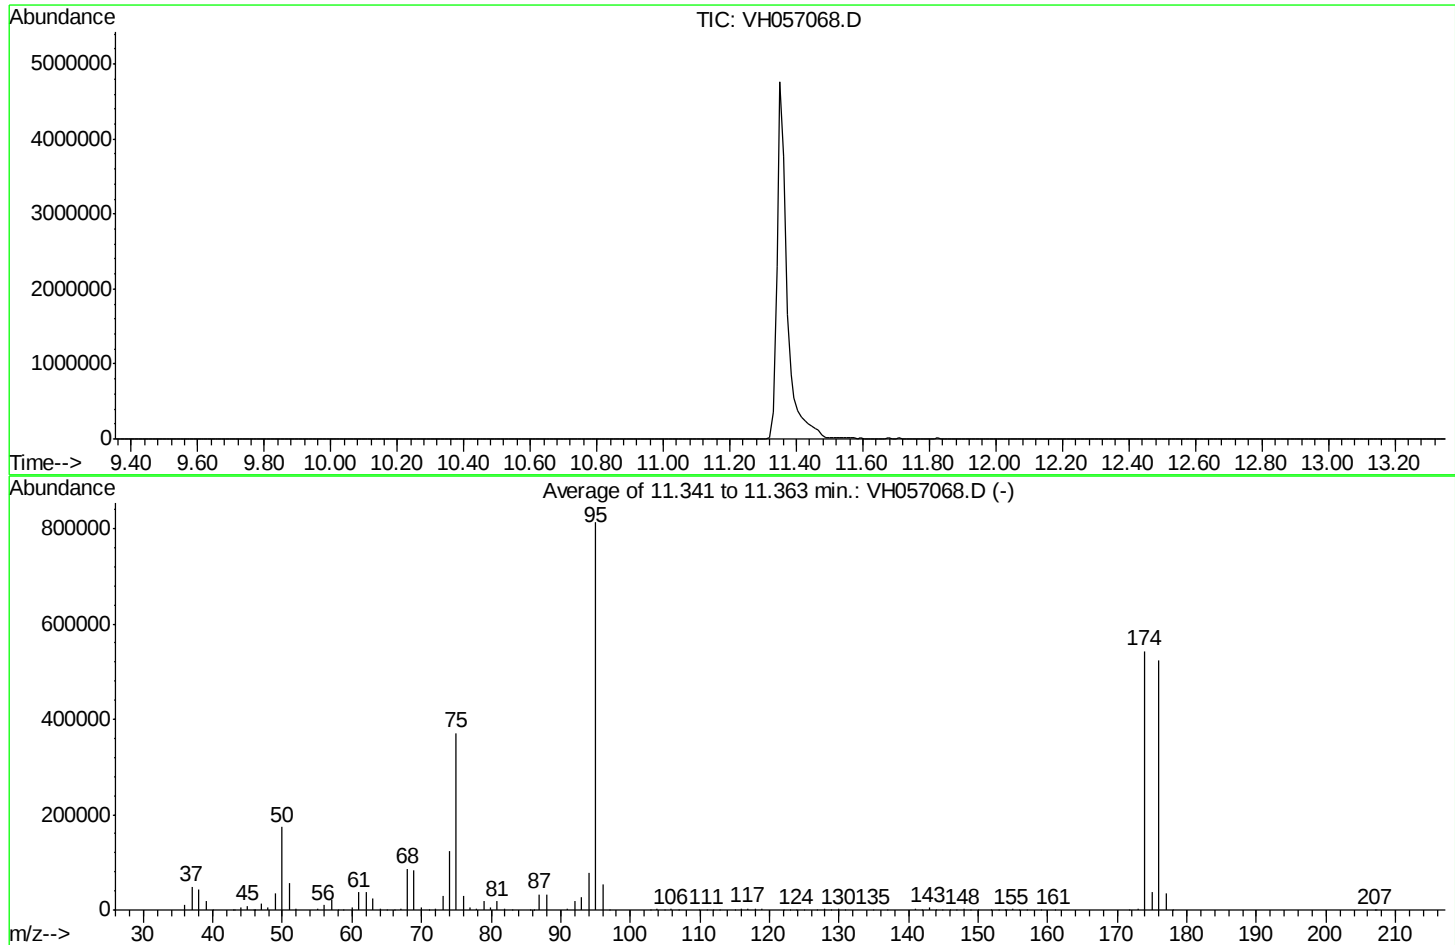

AutoFind: Scans 1039, 1040, 1041; Background Corrected with Scan 1035

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	173696	PASS
75	95	30	60	45.6	371050	PASS
95	95	100	100	100.0	813184	PASS
96	95	5	9	6.7	54362	PASS
173	174	0.00	2	0.5	2495	PASS
174	95	50	100	66.7	542592	PASS
175	174	5	9	7.1	38645	PASS
176	174	95	101	96.3	522368	PASS
177	176	5	9	6.8	35448	PASS