

Data Path : W:\HPCHEM1\MSVOA_H\DATA\VH092115\
 Data File : VH057090.D
 Acq On : 21 Sep 2015 13:09
 Operator : SY/FY
 Sample : G3705-01ME
 Misc : 3.61g/5mL/100uL/5mL/MSVOA_H/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_H
 ClientSampleId :
 LP-6ME


Quant Time: Sep 22 04:37:48 2015
 Quant Method : W:\HPCHEM1\MSVOA_H\METHODS\82H091715W.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 18 15:34:01 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.82	168	812360	50.00	ug/l	-0.03
34) 1,4-Difluorobenzene	5.54	114	1412558	50.00	ug/l	-0.03
63) Chlorobenzene-d5	9.70	117	1082101	50.00	ug/l	-0.02
72) 1,4-Dichlorobenzene-d4	12.49	152	327338	50.00	ug/l	0.00

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4		4.79	65	683792	47.14	ug/l	-0.03
Spiked Amount	50.000	Range	66 - 150	Recovery	=	94.28%	
35) Dibromofluoromethane		4.06	113	583975	51.92	ug/l	-0.02
Spiked Amount	50.000	Range	76 - 130	Recovery	=	103.84%	
48) Toluene-d8		7.50	98	1560987	48.27	ug/l	-0.02
Spiked Amount	50.000	Range	78 - 121	Recovery	=	96.54%	
62) 4-Bromofluorobenzene		11.35	95	537448	49.28	ug/l	0.00
Spiked Amount	50.000	Range	70 - 131	Recovery	=	98.56%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.35	85	443	0.72	ug/l	# 43
5) Bromomethane	1.28	94	256	Below	Cal	# 1
6) Chloroethane	1.33	64	651	Below	Cal	# 1
13) Acrolein	1.98	56	1379	0.89	ug/l	# 50
15) Acrylonitrile	2.88	53	1007	0.21	ug/l	# 7
17) Acetone	2.21	43	59642	Below	Cal	# 91
18) Carbon Disulfide	1.76	76	6891	0.31	ug/l	# 1
19) Methyl Acetate	2.31	43	229953	6.09	ug/l	# 96
25) 2-Butanone	4.29	43	54774	4.06	ug/l	# 99
40) Methacrylonitrile	4.73	41	2736	0.21	ug/l	# 76
41) 1,2-Dichloroethane	4.82	62	4310	0.26	ug/l	# 1
44) Methylcyclohexane	5.55	83	11678	1.31	ug/l	# 29
50) Toluene	7.56	92	140986	5.96	ug/l	# 93
53) 1,4-Dioxane	6.66	88	1292	9.50	ug/l	# 80
59) 2-Hexanone	9.41	43	231321	12.85	ug/l	# 17
74) n-Amyl Acetate	11.32	43	8660	0.27	ug/l	# 53
76) 1,2,3-Trichloropropane	11.84	75	32066	2.61	ug/l	# 45
81) trans-1,4-Dichloro-2-Buten	11.84	75	33348	3.72	ug/l	# 24
85) sec-Butylbenzene	12.23	105	8221	0.42	ug/l	# 92
86) p-Isopropyltoluene	12.39	119	36746	2.45	ug/l	# 92
88) 1,4-Dichlorobenzene	12.50	146	17426	1.66	ug/l	# 59
89) n-Butylbenzene	12.77	91	5441	0.45	ug/l	# 91
90) Hexachloroethane	12.87	117	1699	0.54	ug/l	# 29
92) 1,2-Dibromo-3-Chloropropan	13.55	75	236052	134.31	ug/l	# 1
93) 1,2,4-Trichlorobenzene	14.13	180	2988	5.10	ug/l	# 56
94) Hexachlorobutadiene	14.12	225	2188	2.31	ug/l	# 96
95) Naphthalene	14.38	128	12863	6.25	ug/l	# 92
96) 1,2,3-Trichlorobenzene	14.52	180	3295	7.88	ug/l	# 85

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 4.82 min Scan# 418

Delta R.T. -0.03 min

Lab File: VH057090.D

Acq: 21 Sep 2015 13:09

Instrument :

MSVOA_H

ClientSampleId :


LP-6ME

Tgt Ion:168 Resp: 812360

Ion Ratio Lower Upper

168 100

99 66.2 55.8 83.6

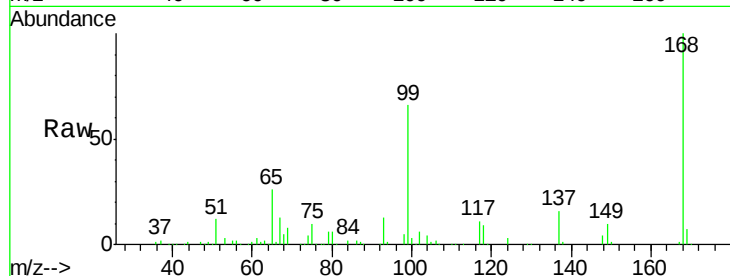

Abundance Ion 168.00 (167.70 to 168.70): V

Ion 99.00 (98.70 to 99.70): VHC

4.82

250000

200000

150000



100000

50000

0

Time-->

4.70 4.80 4.90 5.00

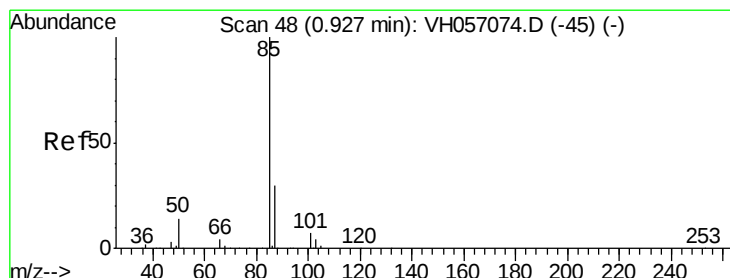

#2

Dichlorodifluoromethane

Concen: 0.72 ug/l

RT: 1.35 min Scan# 88

Delta R.T. 0.42 min

Lab File: VH057090.D


Acq: 21 Sep 2015 13:09

Tgt Ion: 85 Resp: 443

Ion Ratio Lower Upper

85 100

87 0.0 16.0 47.9#

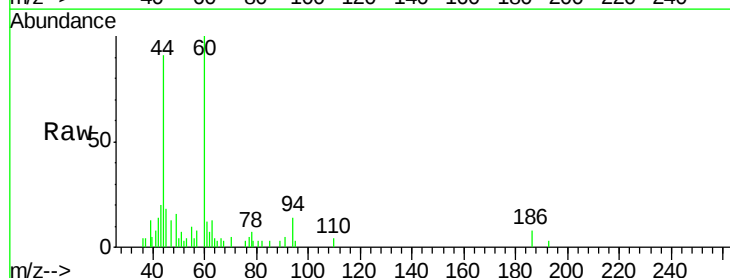

Abundance Ion 85.00 (84.70 to 85.70): VHC

Ion 87.00 (86.70 to 87.70): VHC

1.35

400

300


200


100

0

Time-->

1.30 1.35





#5

Bromomethane

Concen: Below Cal

RT: 1.28 min Scan# 81

Delta R.T. 0.01 min

Lab File: VH057090.D

Acq: 21 Sep 2015 13:09

Instrument :

MSVOA_H

ClientSampled :


LP-6ME

Tgt Ion: 94 Resp: 256

Ion Ratio Lower Upper




94 100

96 0.0 78.5 117.7#

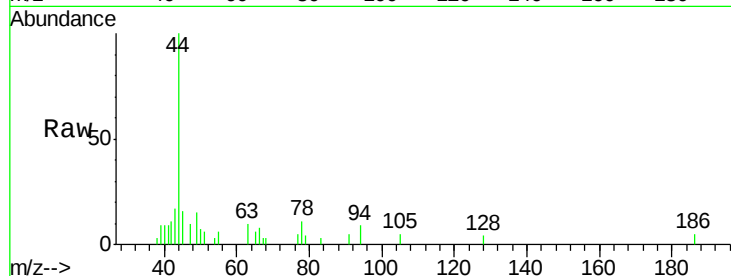

Abundance Ion 94.00 (93.70 to 94.70): VH0

Ion 96.00 (95.70 to 96.70): VH0

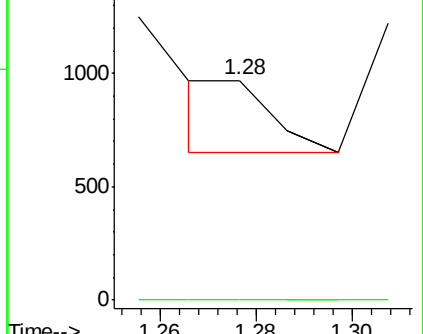

#6

Chloroethane

Concen: Below Cal

RT: 1.33 min Scan# 86

Delta R.T. -0.02 min

Lab File: VH057090.D


Acq: 21 Sep 2015 13:09

Tgt Ion: 64 Resp: 651

Ion Ratio Lower Upper



64 100


66 118.1 25.2 37.8#



Abundance Ion 64.00 (63.70 to 64.70): VH0

Ion 66.00 (65.70 to 66.70): VH0

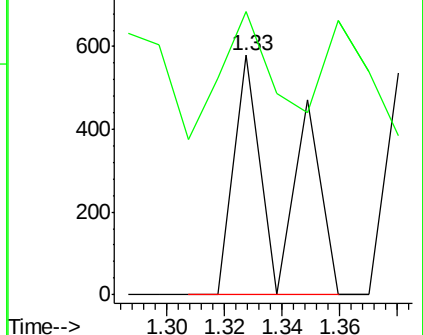

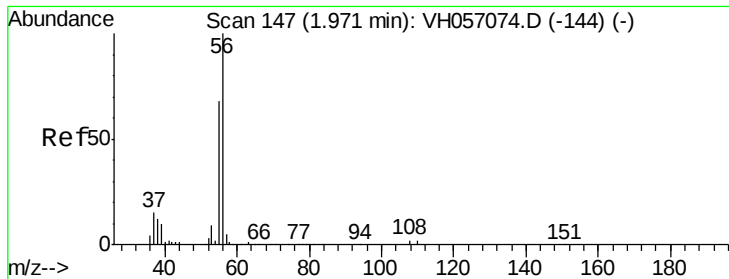

#13

Acrolein

Concen: 0.89 ug/l

RT: 1.98 min Scan# 148

Delta R.T. 0.01 min

Lab File: VH057090.D

Acq: 21 Sep 2015 13:09

Instrument :

MSVOA_H

ClientSampled :





LP-6ME

Tgt Ion: 56 Resp: 1379

Ion Ratio Lower Upper

56 100

55 106.3 52.9 79.3#

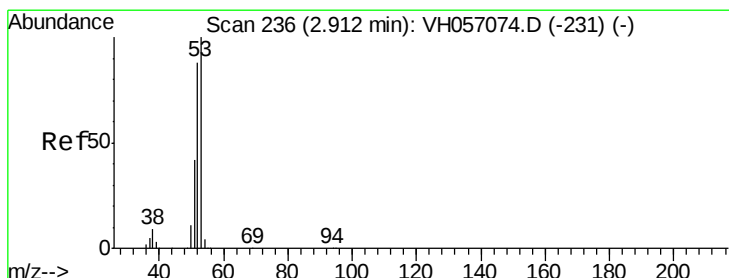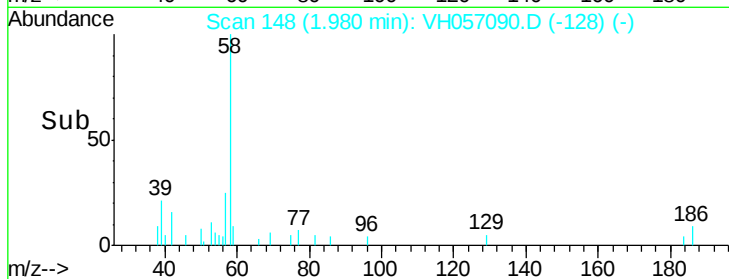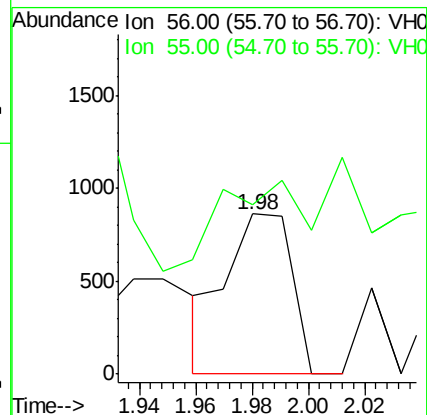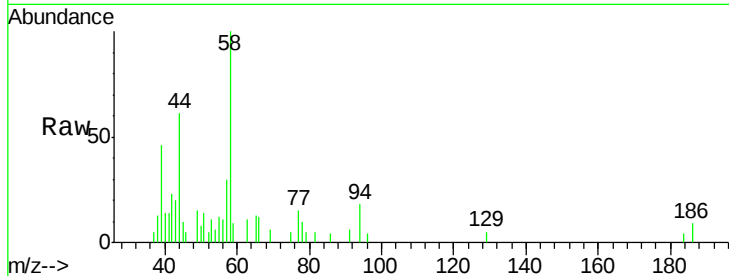

#15

Acrylonitrile

Concen: 0.21 ug/l

RT: 2.88 min Scan# 234

Delta R.T. -0.03 min

Lab File: VH057090.D

Acq: 21 Sep 2015 13:09




Tgt Ion: 53 Resp: 1007


Ion Ratio Lower Upper

53 100

52 0.0 67.6 101.4#

51 97.3 31.8 47.6#

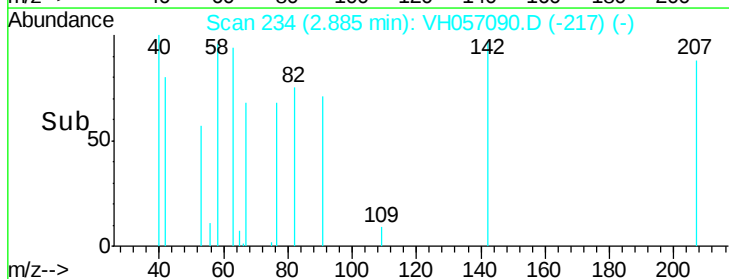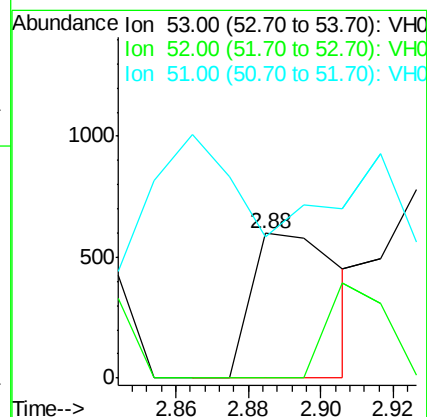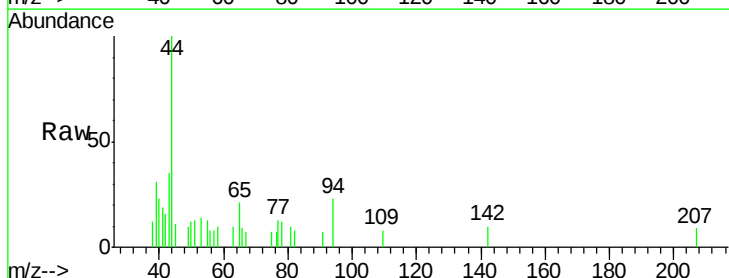



#17

Acetone

Concen: Below Cal

RT: 2.21 min Scan# 170

Delta R.T. -0.00 min

Lab File: VH057090.D

Acq: 21 Sep 2015 13:09

Instrument :

MSVOA_H

ClientSampleId :


LP-6ME

Tgt Ion: 43 Resp: 59642

Ion Ratio Lower Upper




43 100

58 17.9 17.7 26.5

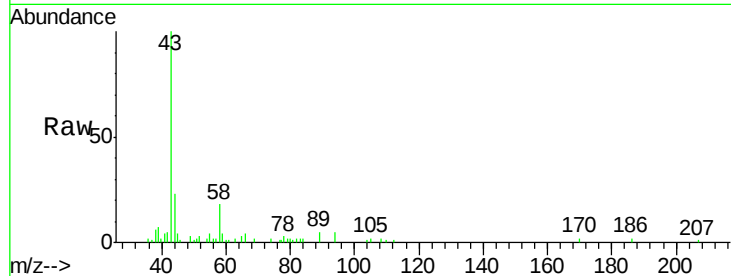

Abundance Ion 43.00 (42.70 to 43.70): VH057090.D (-151) (-)

Ion 58.00 (57.70 to 58.70): VH057090.D (-151) (-)

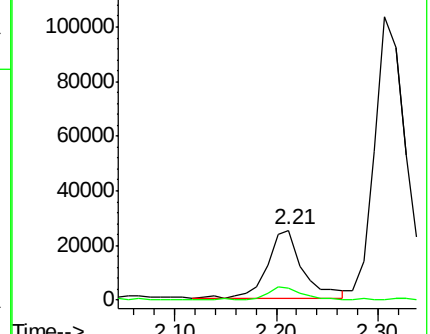

#18

Carbon Disulfide

Concen: 0.31 ug/l

RT: 1.76 min Scan# 127

Delta R.T. -0.02 min

Lab File: VH057090.D


Acq: 21 Sep 2015 13:09

Tgt Ion: 76 Resp: 6891

Ion Ratio Lower Upper



76 100


78 45.5 7.1 10.7#



Abundance Ion 76.00 (75.70 to 76.70): VH057090.D (-110) (-)

Ion 78.00 (77.70 to 78.70): VH057090.D (-110) (-)




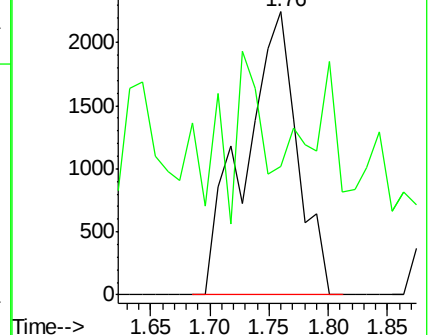




#19
Methyl Acetate
Concen: 6.09 ug/l
RT: 2.31 min Scan# 179
Delta R.T. -0.01 min
Lab File: VH057090.D
Acq: 21 Sep 2015 13:09




Instrument :
MSVOA_H
ClientSampleId :
LP-6ME


Tgt Ion: 43 Resp: 229953
Ion Ratio Lower Upper
43 100
74 21.0 13.3 24.7

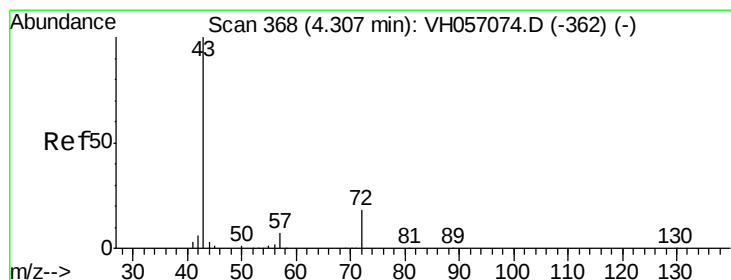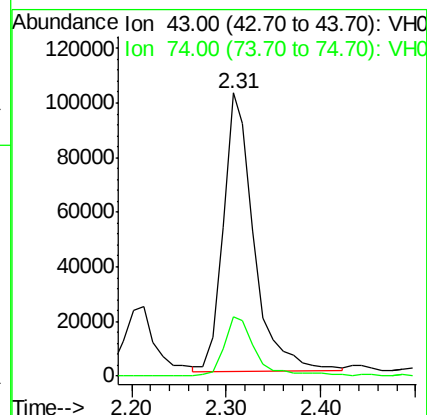

#25
2-Butanone
Concen: 4.06 ug/l
RT: 4.29 min Scan# 368
Delta R.T. -0.01 min
Lab File: VH057090.D
Acq: 21 Sep 2015 13:09

Tgt Ion: 43 Resp: 54774
Ion Ratio Lower Upper
43 100
72 19.1 0.0 39.2

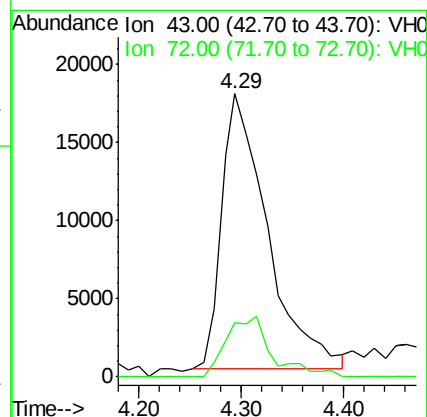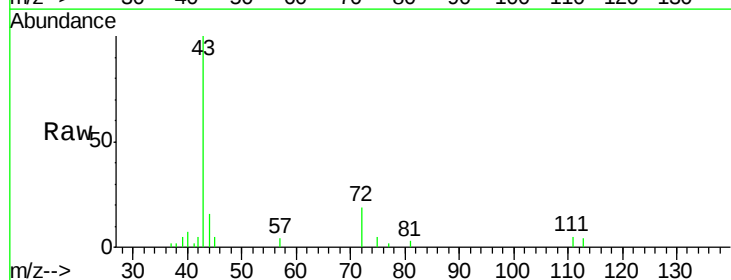



#33

1,2-Dichloroethane-d4

Concen: 47.14 ug/l

RT: 4.79 min Scan# 415

Delta R.T. -0.03 min

Lab File: VH057090.D

Acq: 21 Sep 2015 13:09

Instrument :

MSVOA_H

ClientSampleId :


LP-6ME

Tgt Ion: 65 Resp: 683792

Ion Ratio Lower Upper




65 100

67 48.9 43.2 64.8

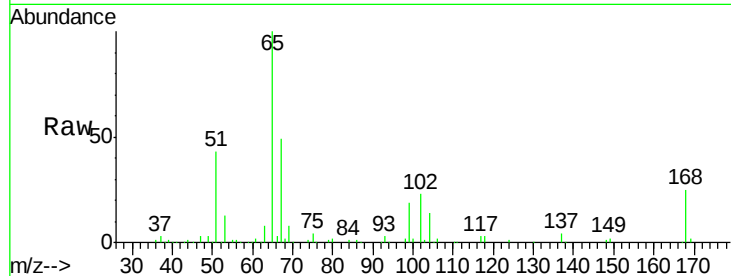

Abundance Ion 65.00 (64.70 to 65.70): VH0

Ion 67.00 (66.70 to 67.70): VH0

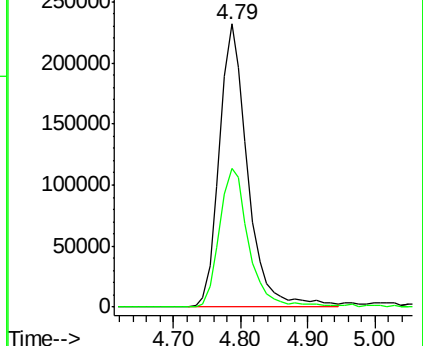

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 5.54 min Scan# 487

Delta R.T. -0.03 min

Lab File: VH057090.D

Acq: 21 Sep 2015 13:09


Tgt Ion: 114 Resp: 1412558

Ion Ratio Lower Upper

114 100

63 24.0 19.0 28.4



88 19.7 15.7 23.5




Abundance Ion 114.00 (113.70 to 114.70): V

Ion 63.00 (62.70 to 63.70): VH0

Ion 88.00 (87.70 to 88.70): VH0

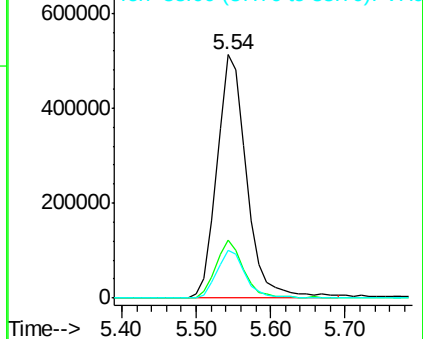







#35
 Dibromofluoromethane
 Concen: 51.92 ug/l
 RT: 4.06 min Scan# 346
 Delta R.T. -0.02 min
 Lab File: VH057090.D
 Acq: 21 Sep 2015 13:09

Instrument :
 MSVOA_H
 ClientSampleId :
 LP-6ME

Tgt Ion: 113 Resp: 583975
 Ion Ratio Lower Upper
 113 100
 111 101.4 84.0 126.0
 192 16.4 13.6 20.4

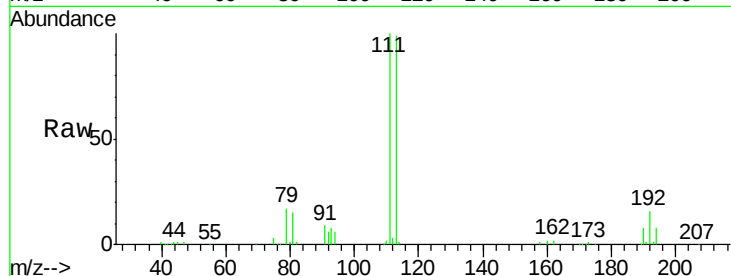


Abundance Ion 113.00 (112.70 to 113.70): V
 Ion 111.00 (110.70 to 111.70): V
 Ion 192.00 (191.70 to 192.70): V


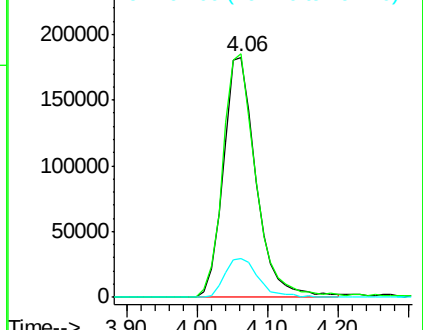



#40
 Methacrylonitrile
 Concen: 0.21 ug/l
 RT: 4.73 min Scan# 410
 Delta R.T. 0.01 min
 Lab File: VH057090.D
 Acq: 21 Sep 2015 13:09

Tgt Ion: 41 Resp: 2736
 Ion Ratio Lower Upper
 41 100
 39 56.1 25.1 75.2
 67 39.2 22.5 67.5
 52 0.0 19.0 57.0#



Abundance Ion 41.00 (40.70 to 41.70): VHC
 Ion 39.00 (38.70 to 39.70): VHC
 Ion 67.00 (66.70 to 67.70): VHC
 Ion 52.00 (51.70 to 52.70): VHC




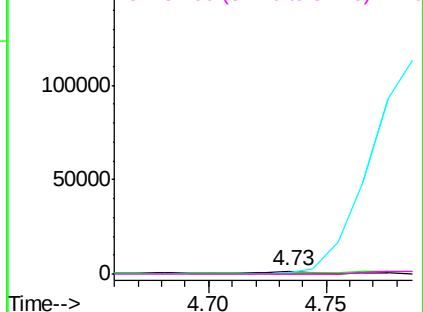


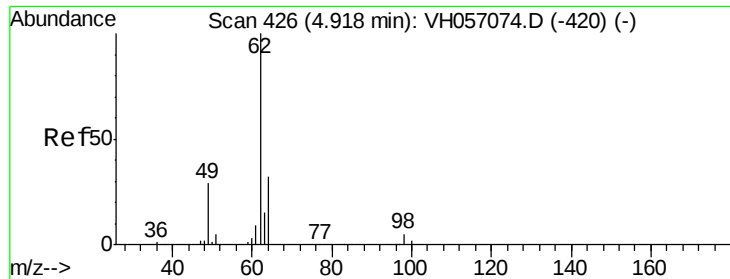

#41
1,2-Dichloroethane
Concen: 0.26 ug/l
RT: 4.82 min Scan# 418
Delta R.T. -0.10 min
Lab File: VH057090.D
Acq: 21 Sep 2015 13:09




Instrument :
MSVOA_H
ClientSampled :
LP-6ME


Tgt Ion: 62 Resp: 4310
Ion Ratio Lower Upper
62 100
98 502.6 7.3 10.9#

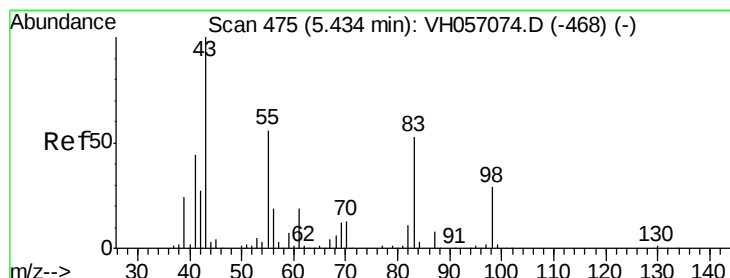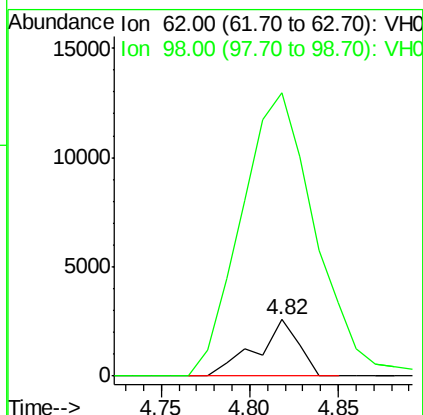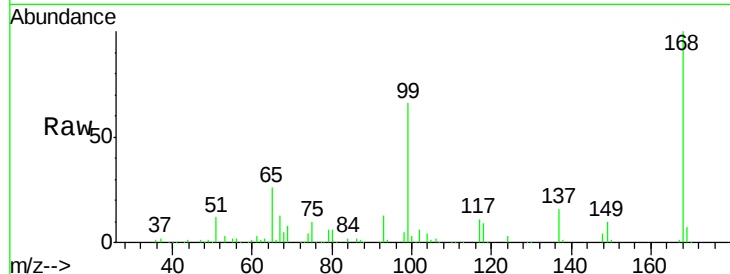

#44
Methylcyclohexane
Concen: 1.31 ug/l
RT: 5.55 min Scan# 488
Delta R.T. 0.12 min
Lab File: VH057090.D
Acq: 21 Sep 2015 13:09

Tgt Ion: 83 Resp: 11678
Ion Ratio Lower Upper
83 100
55 33.4 0.0 207.2
98 0.0 0.0 108.4

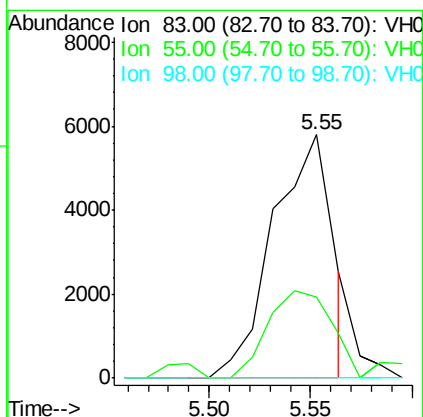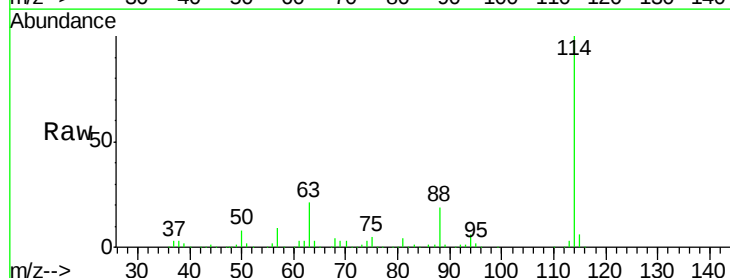

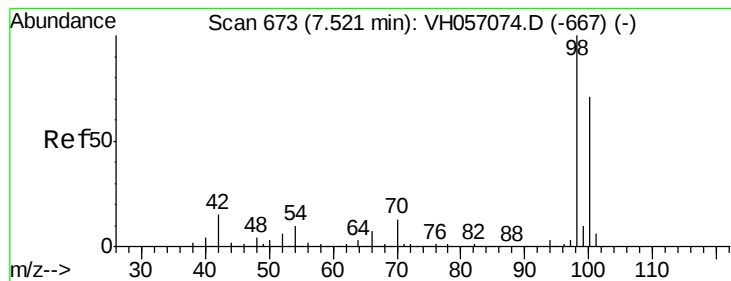

#48

Toluene-d8

Concen: 48.27 ug/l

RT: 7.50 min Scan# 673

Delta R.T. -0.02 min

Lab File: VH057090.D

Acq: 21 Sep 2015 13:09

Instrument :

MSVOA_H

ClientSampleId :


LP-6ME

Tgt Ion: 98 Resp: 1560987

Ion Ratio Lower Upper




98 100

100 72.1 56.7 85.1



Abundance Ion 98.00 (97.70 to 98.70): VH057090.D (-656) (-)

Ion 100.00 (99.70 to 100.70): VH057090.D (-656) (-)

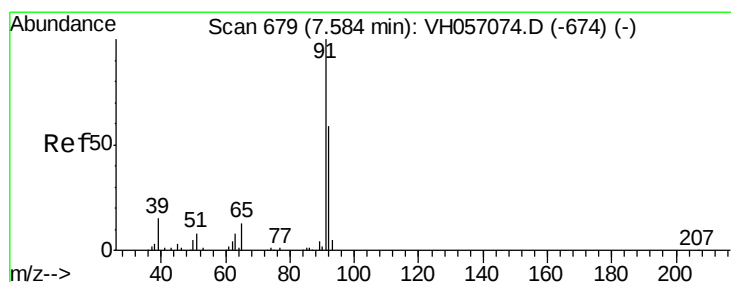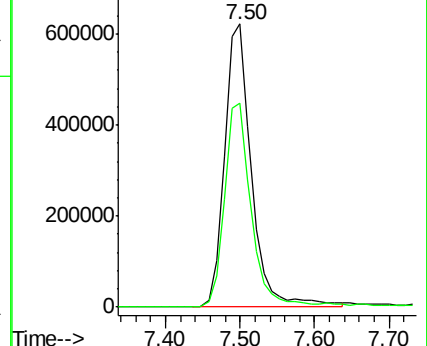

#50

Toluene

Concen: 5.96 ug/l

RT: 7.56 min Scan# 679

Delta R.T. -0.02 min

Lab File: VH057090.D


Acq: 21 Sep 2015 13:09

Tgt Ion: 92 Resp: 140986

Ion Ratio Lower Upper



92 100


91 166.6 125.8 188.6

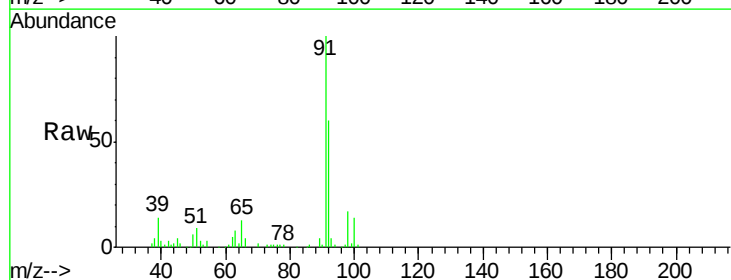

Abundance Ion 92.00 (91.70 to 92.70): VH057090.D (-662) (-)

Ion 91.00 (90.70 to 91.70): VH057090.D (-662) (-)




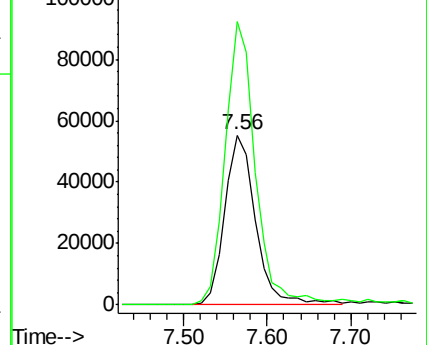


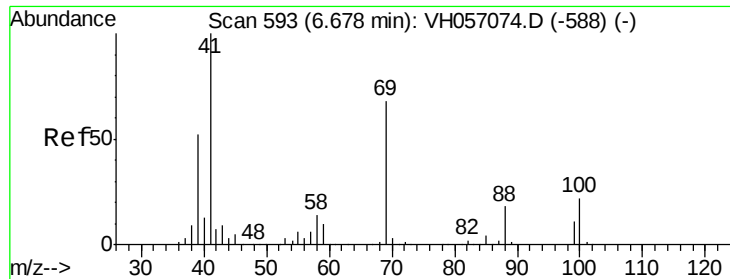

#53
 1,4-Dioxane
 Concen: 9.50 ug/l
 RT: 6.66 min Scan# 593
 Delta R.T. -0.02 min
 Lab File: VH057090.D
 Acq: 21 Sep 2015 13:09




Instrument :
 MSVOA_H
 ClientSampleId :
 LP-6ME


Tgt Ion: 88 Resp: 1292
 Ion Ratio Lower Upper
 88 100
 43 70.9 39.6 59.4#
 58 65.8 61.4 92.2

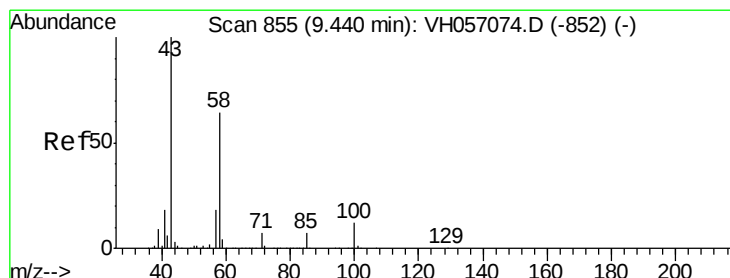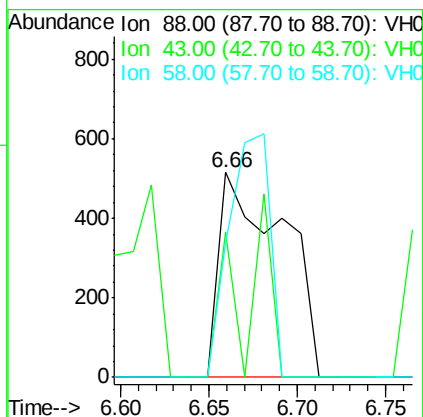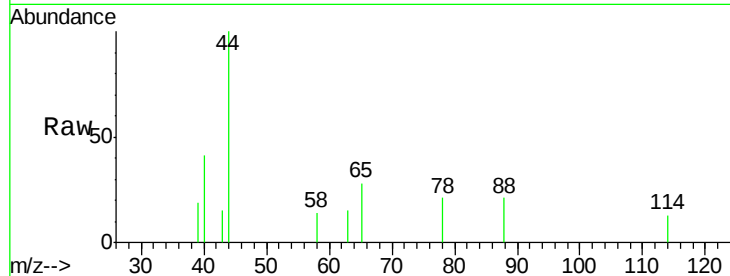

#59
 2-Hexanone
 Concen: 12.85 ug/l
 RT: 9.41 min Scan# 855
 Delta R.T. -0.03 min
 Lab File: VH057090.D
 Acq: 21 Sep 2015 13:09

Tgt Ion: 43 Resp: 231321
 Ion Ratio Lower Upper
 43 100
 58 17.8 27.1 81.2#
 57 97.9 8.1 24.3#

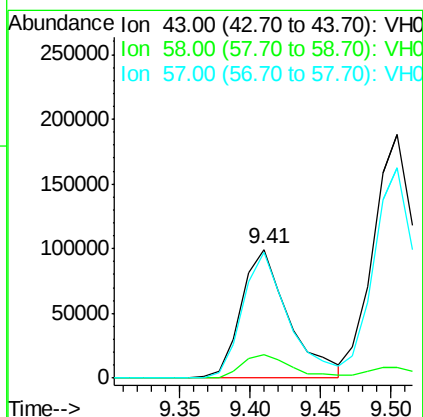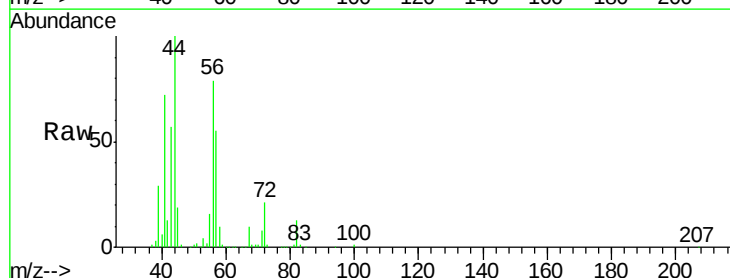



#62

4-Bromofluorobenzene

Concen: 49.28 ug/l

RT: 11.35 min Scan# 1039

Delta R.T. -0.01 min

Lab File: VH057090.D

Acq: 21 Sep 2015 13:09

Instrument :

MSVOA_H

ClientSampleId :

LP-6ME





Tgt Ion: 95 Resp: 537448

Ion Ratio Lower Upper

95 100

174 70.1 58.4 87.6

176 67.1 54.3 81.5

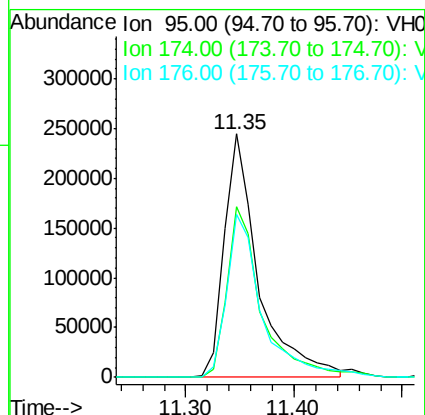

#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 9.70 min Scan# 883

Delta R.T. -0.02 min

Lab File: VH057090.D

Acq: 21 Sep 2015 13:09




Tgt Ion: 117 Resp: 1082101


Ion Ratio Lower Upper

117 100

82 60.1 51.0 76.6

119 31.4 26.7 40.1

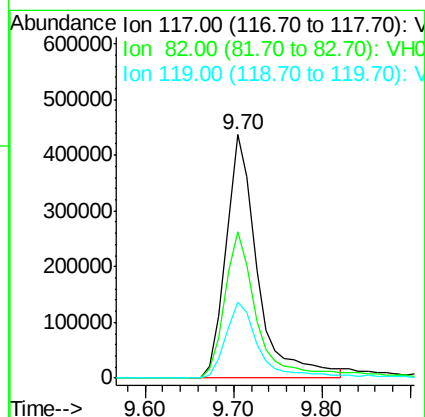




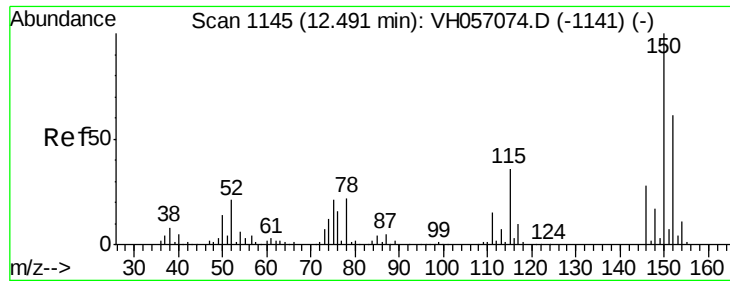


#72

1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.49 min Scan# 1147
Delta R.T. -0.00 min
Lab File: VH057090.D
Acq: 21 Sep 2015 13:09

Instrument :
MSVOA_H
ClientSampleId :
LP-6ME




Tgt Ion:152 Resp: 327338
Ion Ratio Lower Upper
152 100
115 61.4 28.2 84.6
150 159.4 0.0 332.0

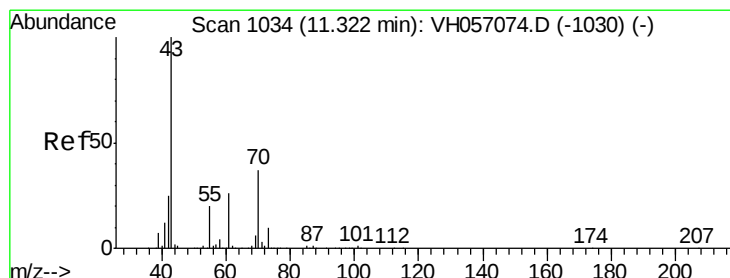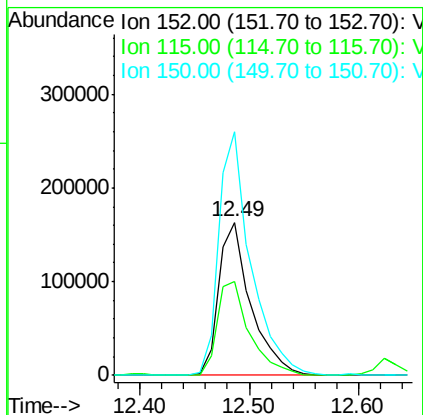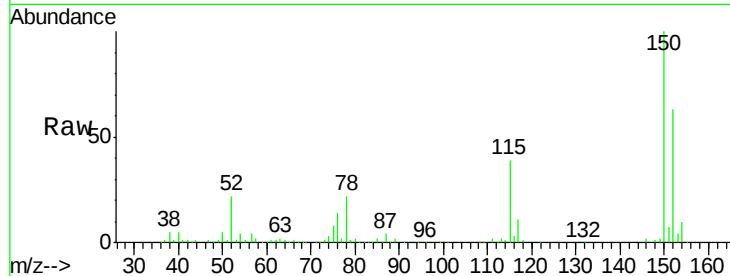


#74

n-Amyl Acetate
Concen: 0.27 ug/l
RT: 11.32 min Scan# 1036
Delta R.T. -0.01 min
Lab File: VH057090.D
Acq: 21 Sep 2015 13:09

Tgt Ion: 43 Resp: 8660
Ion Ratio Lower Upper
43 100
70 19.7 27.3 40.9#
55 71.8 15.3 22.9#
61 12.5 19.4 29.0#



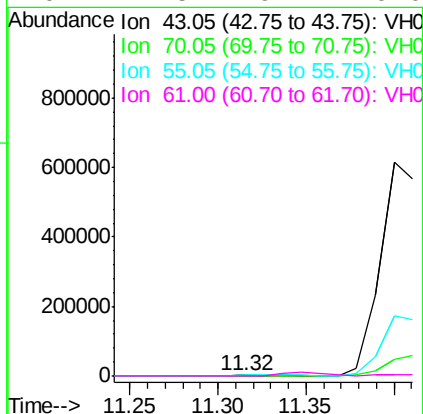
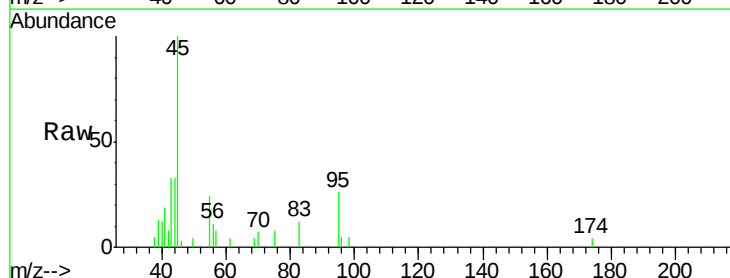




#76
 1,2,3-Trichloropropane
 Concen: 2.61 ug/l
 RT: 11.84 min Scan# 1086
 Delta R.T. 0.11 min
 Lab File: VH057090.D
 Acq: 21 Sep 2015 13:09




Instrument :
 MSVOA_H
 ClientSampleId :
 LP-6ME


Tgt Ion: 75 Resp: 32066
 Ion Ratio Lower Upper
 75 100
 77 0.0 14.9 44.9#

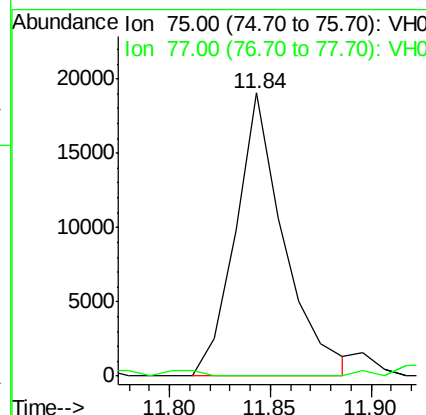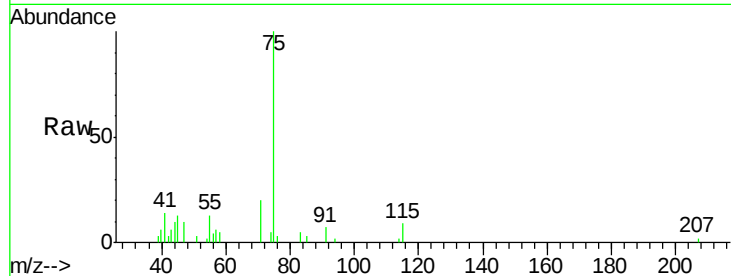

#81
 trans-1,4-Dichloro-2-Butene
 Concen: 3.72 ug/l
 RT: 11.84 min Scan# 1086
 Delta R.T. 0.04 min
 Lab File: VH057090.D
 Acq: 21 Sep 2015 13:09

Tgt Ion: 75 Resp: 33348
 Ion Ratio Lower Upper
 75 100
 53 0.0 32.0 96.2#
 89 0.0 21.1 63.3#



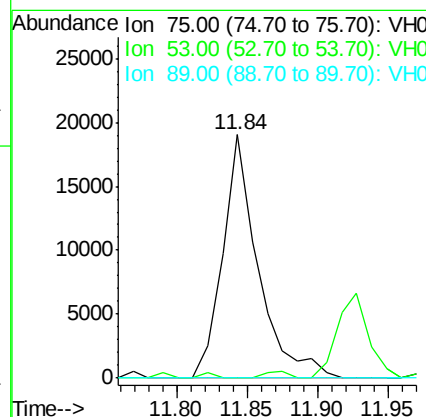





#85
 sec-Butylbenzene
 Concen: 0.42 ug/l
 RT: 12.23 min Scan# 1123
 Delta R.T. -0.02 min
 Lab File: VH057090.D
 Acq: 21 Sep 2015 13:09




Instrument :
 MSVOA_H
 ClientSampled :
 LP-6ME


Tgt Ion:105 Resp: 8221
 Ion Ratio Lower Upper
 105 100
 134 14.6 9.1 27.3

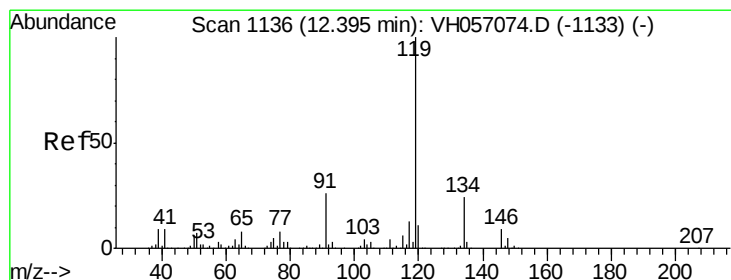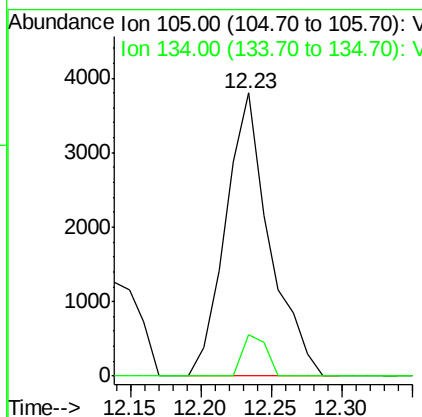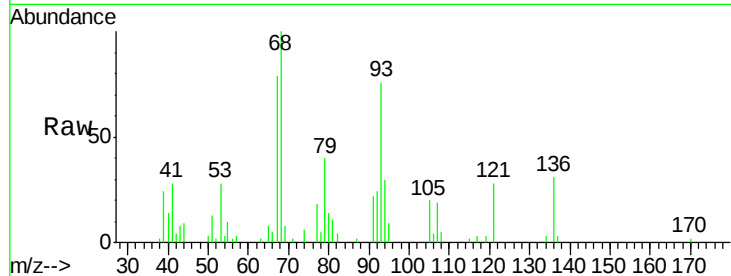

#86
 p-Isopropyltoluene
 Concen: 2.45 ug/l
 RT: 12.39 min Scan# 1138
 Delta R.T. -0.00 min
 Lab File: VH057090.D
 Acq: 21 Sep 2015 13:09

Tgt Ion:119 Resp: 36746
 Ion Ratio Lower Upper
 119 100
 134 21.4 13.0 38.9
 91 21.7 12.5 37.5

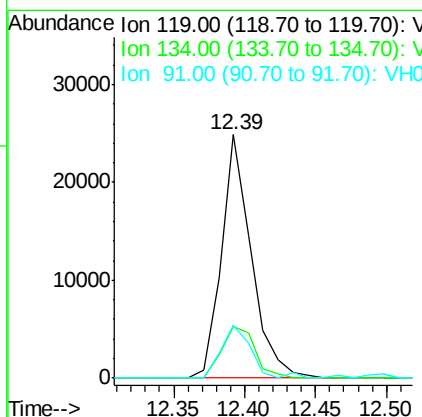

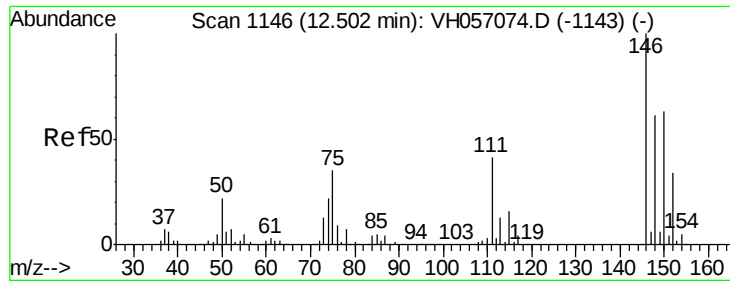

#88

1,4-Dichlorobenzene

Concen: 1.66 ug/l

RT: 12.50 min Scan# 1148

Delta R.T. -0.00 min

Lab File: VH057090.D

Acq: 21 Sep 2015 13:09

Instrument :

MSVOA_H

ClientSampled :

LP-6ME


Tgt Ion:146 Resp: 17426

Ion Ratio Lower Upper

146 100

111 70.3 19.8 59.3#




148 87.8 30.3 90.9

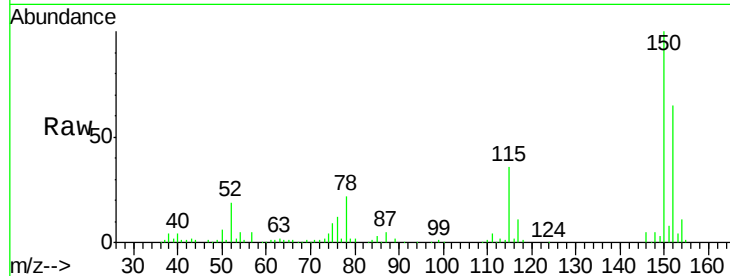

Abundance Ion 146.00 (145.70 to 146.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

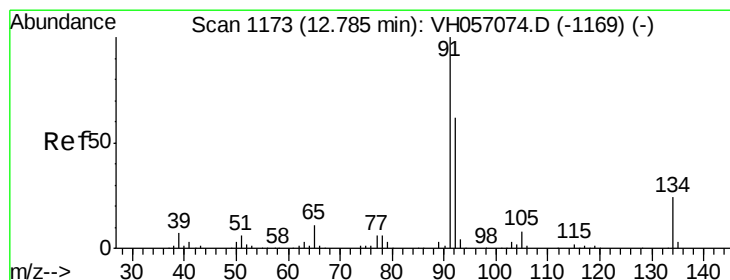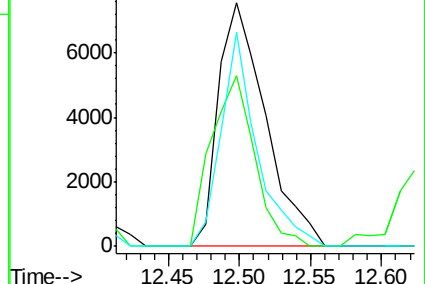

#89

n-Butylbenzene

Concen: 0.45 ug/l

RT: 12.77 min Scan# 1174

Delta R.T. -0.01 min

Lab File: VH057090.D

Acq: 21 Sep 2015 13:09


Tgt Ion: 91 Resp: 5441

Ion Ratio Lower Upper

91 100

92 67.6 31.3 93.9



134 29.2 10.5 31.6

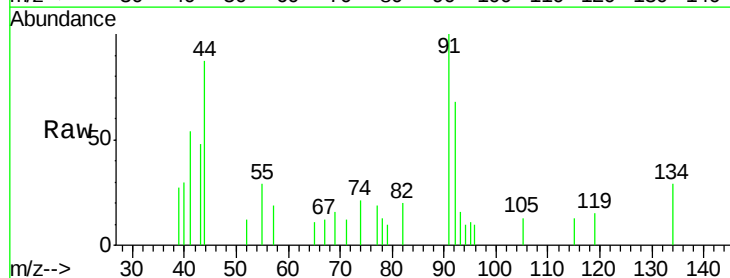


Abundance Ion 91.00 (90.70 to 91.70): V

Ion 92.00 (91.70 to 92.70): V

Ion 134.00 (133.70 to 134.70): V



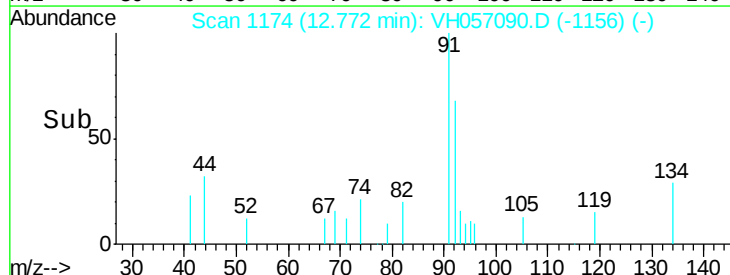
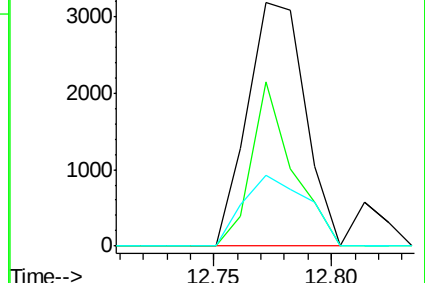




#90
Hexachloroethane
Concen: 0.54 ug/l
RT: 12.87 min Scan# 1183
Delta R.T. 0.02 min
Lab File: VH057090.D
Acq: 21 Sep 2015 13:09




Instrument :
MSVOA_H
ClientSampled :
LP-6ME


Tgt Ion:117 Resp: 1699
Ion Ratio Lower Upper
117 100
201 0.0 14.0 80.8#

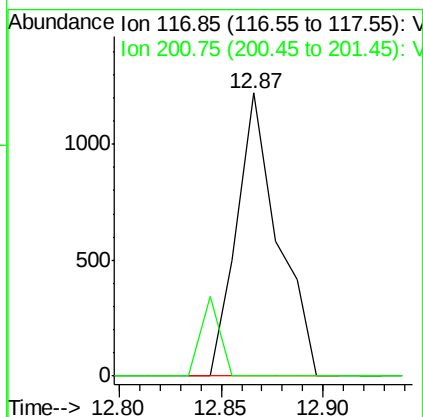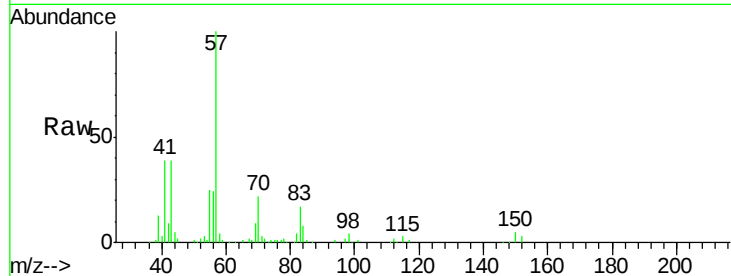

#92
1,2-Dibromo-3-Chloropropane
Concen: 134.31 ug/l
RT: 13.55 min Scan# 1248
Delta R.T. -0.02 min
Lab File: VH057090.D
Acq: 21 Sep 2015 13:09

Tgt Ion: 75 Resp: 236052
Ion Ratio Lower Upper
75 100
155 0.0 43.4 130.2#
157 0.0 62.8 188.4#



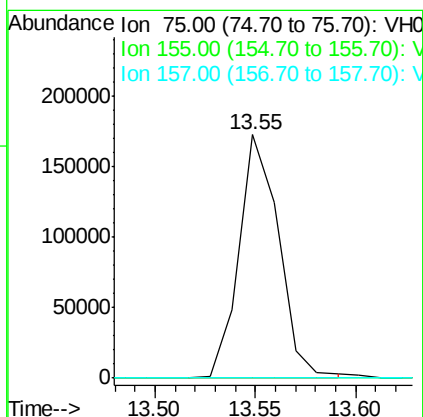





#93
 1,2,4-Trichlorobenzene
 Concen: 5.10 ug/l
 RT: 14.13 min Scan# 1303
 Delta R.T. 0.00 min
 Lab File: VH057090.D
 Acq: 21 Sep 2015 13:09




Instrument :
 MSVOA_H
 ClientSampleId :
 LP-6ME


Tgt Ion:180 Resp: 2988
 Ion Ratio Lower Upper
 180 100
 182 120.1 43.0 129.2
 145 0.0 17.3 52.0#

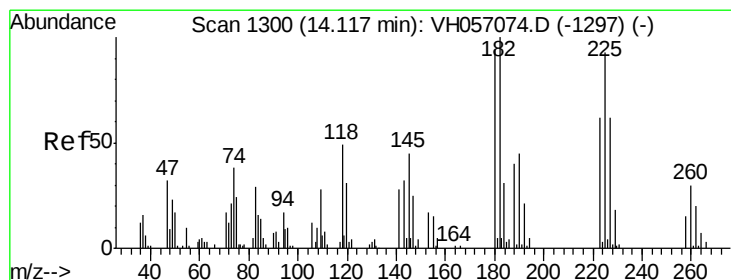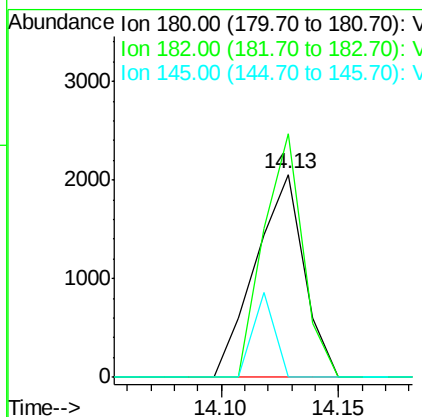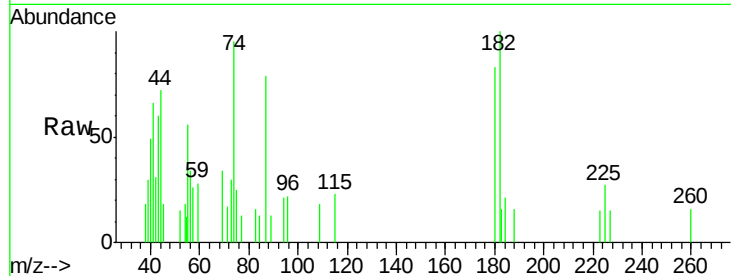

#94
 Hexachlorobutadiene
 Concen: 2.31 ug/l
 RT: 14.12 min Scan# 1302
 Delta R.T. 0.00 min
 Lab File: VH057090.D
 Acq: 21 Sep 2015 13:09

Tgt Ion:225 Resp: 2188
 Ion Ratio Lower Upper
 225 100
 223 56.2 30.3 90.8
 227 59.2 30.5 91.5


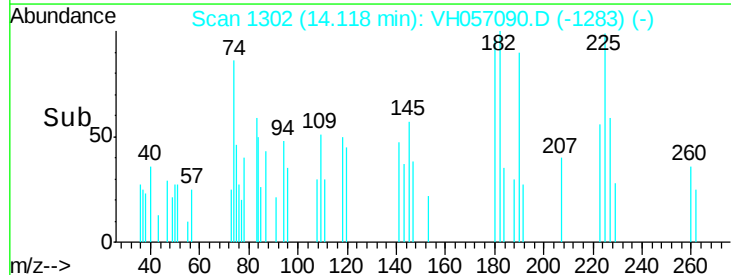
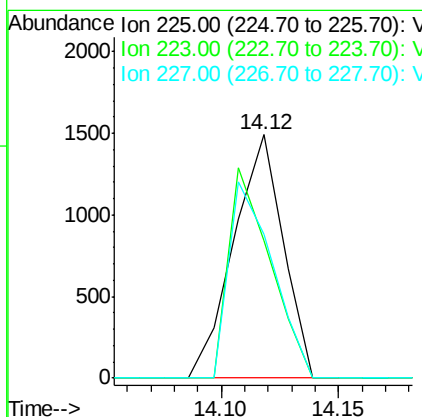





#95
Naphthalene
Concen: 6.25 ug/l
RT: 14.38 min Scan# 1327
Delta R.T. 0.00 min
Lab File: VH057090.D
Acq: 21 Sep 2015 13:09

Instrument :
MSVOA_H
ClientSampleId :
LP-6ME

Tgt Ion:128 Resp: 12863
Ion Ratio Lower Upper
128 100
127 11.3 9.6 14.4
129 16.3 8.7 13.1#

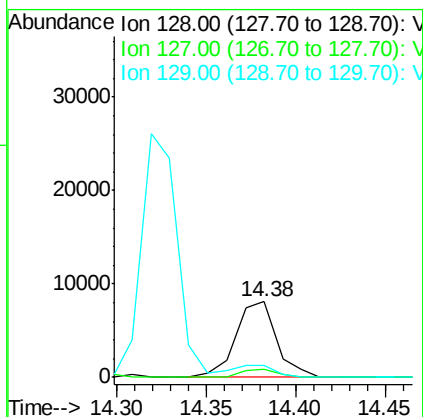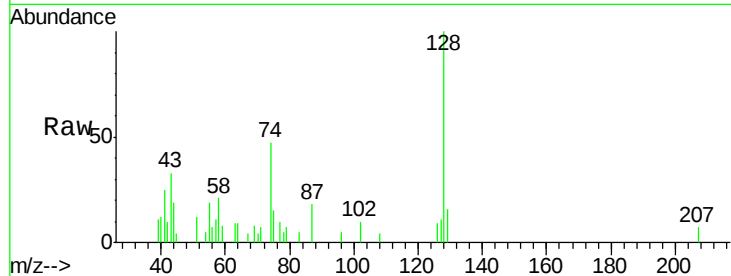

#96
1,2,3-Trichlorobenzene
Concen: 7.88 ug/l
RT: 14.52 min Scan# 1340
Delta R.T. -0.01 min
Lab File: VH057090.D
Acq: 21 Sep 2015 13:09

Tgt Ion:180 Resp: 3295
Ion Ratio Lower Upper
180 100
182 79.3 47.1 141.3
145 18.8 12.5 37.5

