


Data Path : W:\HPCHEM1\MSVOA_H\DATA\VH092215\
 Data File : VH057100.D
 Acq On : 22 Sep 2015 10:58
 Operator : SY/FY
 Sample : BFB
 Misc : 5mL/MSVOA_H/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_H
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : W:\HPCHEM1\MSVOA_H\METHODS\82H091715W.M
 Title : SW846 8260
 Last Update : Fri Sep 18 15:34:01 2015

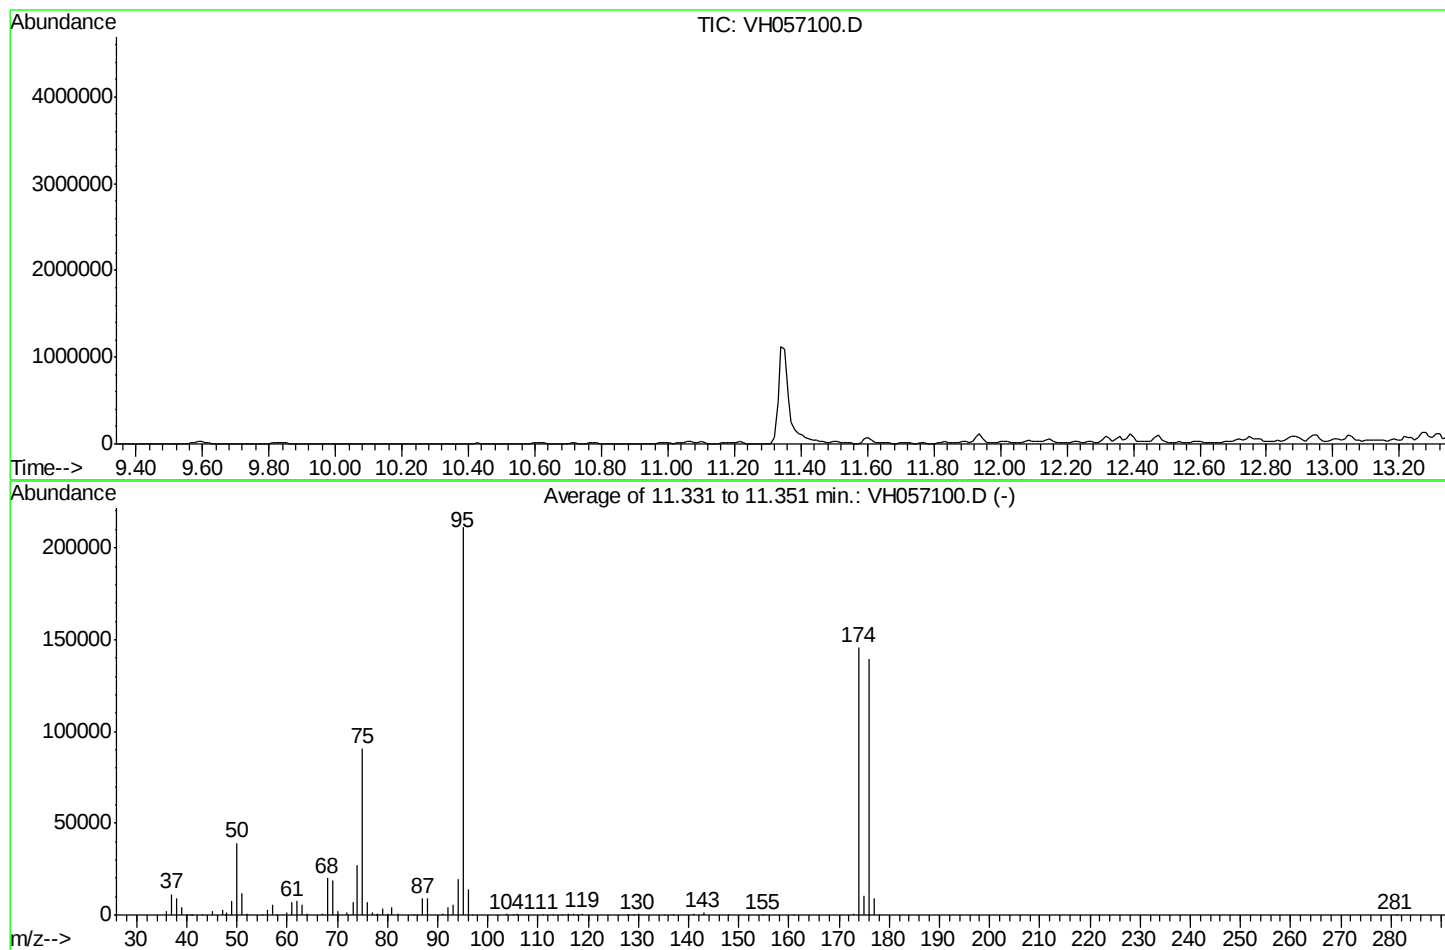

AutoFind: Scans 1038, 1039, 1040; Background Corrected with Scan 1034

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	39171	PASS
75	95	30	60	42.8	90368	PASS
95	95	100	100	100.0	211152	PASS
96	95	5	9	6.5	13706	PASS
173	174	0.00	2	0.5	671	PASS
174	95	50	100	69.0	145661	PASS
175	174	5	9	7.2	10490	PASS
176	174	95	101	95.7	139365	PASS
177	176	5	9	6.3	8848	PASS