


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL010220\
 Data File : VL034542.D
 Acq On : 2 Jan 2020 10:25
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL123019AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Dec 30 14:58:50 2019
 Last Update : Mon Dec 30 14:58:50 2019

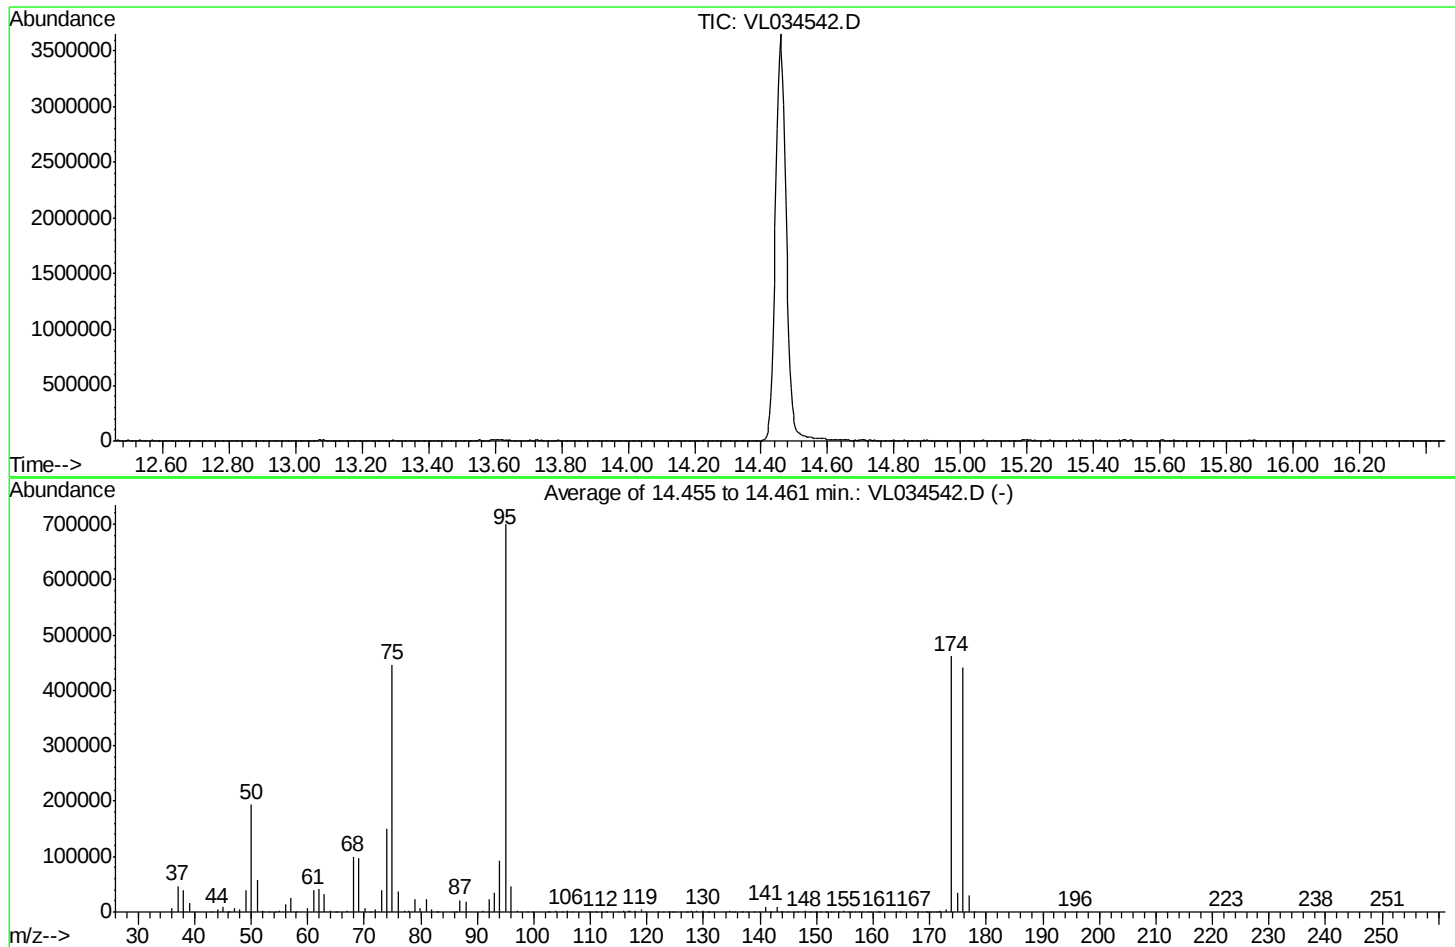

AutoFind: Scans 3629, 3630, 3631; Background Corrected with Scan 3606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.6	193088	PASS
75	95	30	66	63.9	446890	PASS
95	95	100	100	100.0	699505	PASS
96	95	5	9	6.7	46709	PASS
173	174	0.00	2	0.8	3847	PASS
174	95	50	120	65.9	461226	PASS
175	174	4	9	7.4	34053	PASS
176	174	93	101	95.5	440597	PASS
177	176	5	9	7.0	30853	PASS