


Data Path : W:\HPCHEM1\MSVOA L\DATA\VL010816\
Data File : VL026646.D
Acq On : 8 Jan 2016 13:22
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL010816AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Jan 11 17:14:02 2016
Last Update : Mon Jan 11 17:14:02 2016

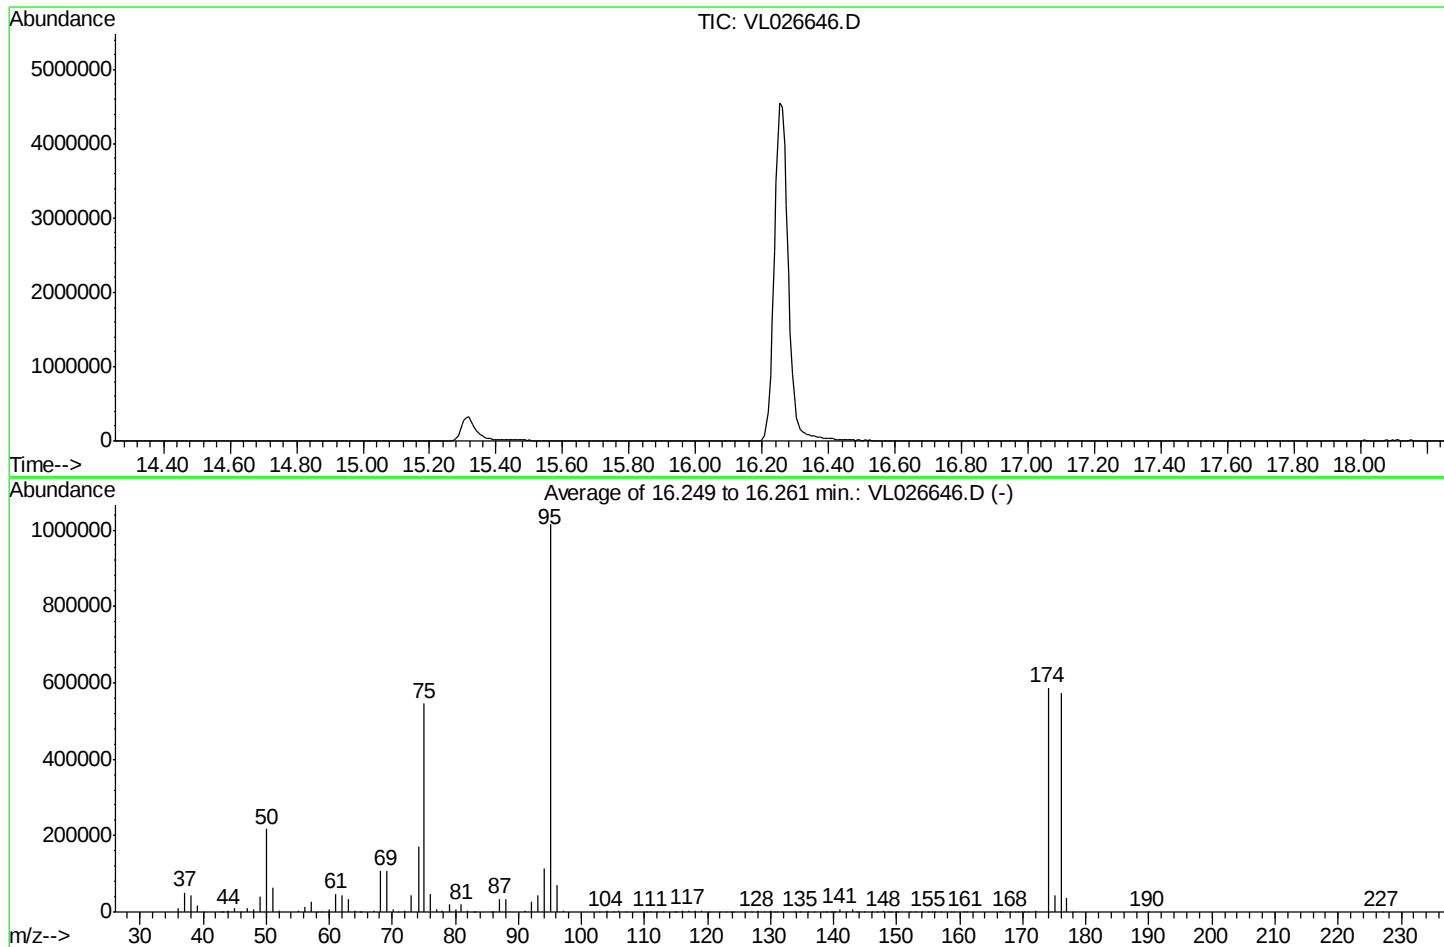

AutoFind: Scans 2159, 2160, 2161; Background Corrected with Scan 2142

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.3	216512	PASS
75	95	30	66	53.8	546069	PASS
95	95	100	100	100.0	1014634	PASS
96	95	5	9	6.8	69501	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	57.9	587178	PASS
175	174	4	9	7.4	43312	PASS
176	174	93	101	97.4	571925	PASS
177	176	5	9	6.5	36917	PASS