


Data Path : W:\HPCHEM1\MSVOA L\Data\VL011216\
 Data File : VL026667.D
 Acq On : 12 Jan 2016 8:31
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL010816AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Jan 11 17:14:02 2016
 Last Update : Mon Jan 11 17:14:02 2016

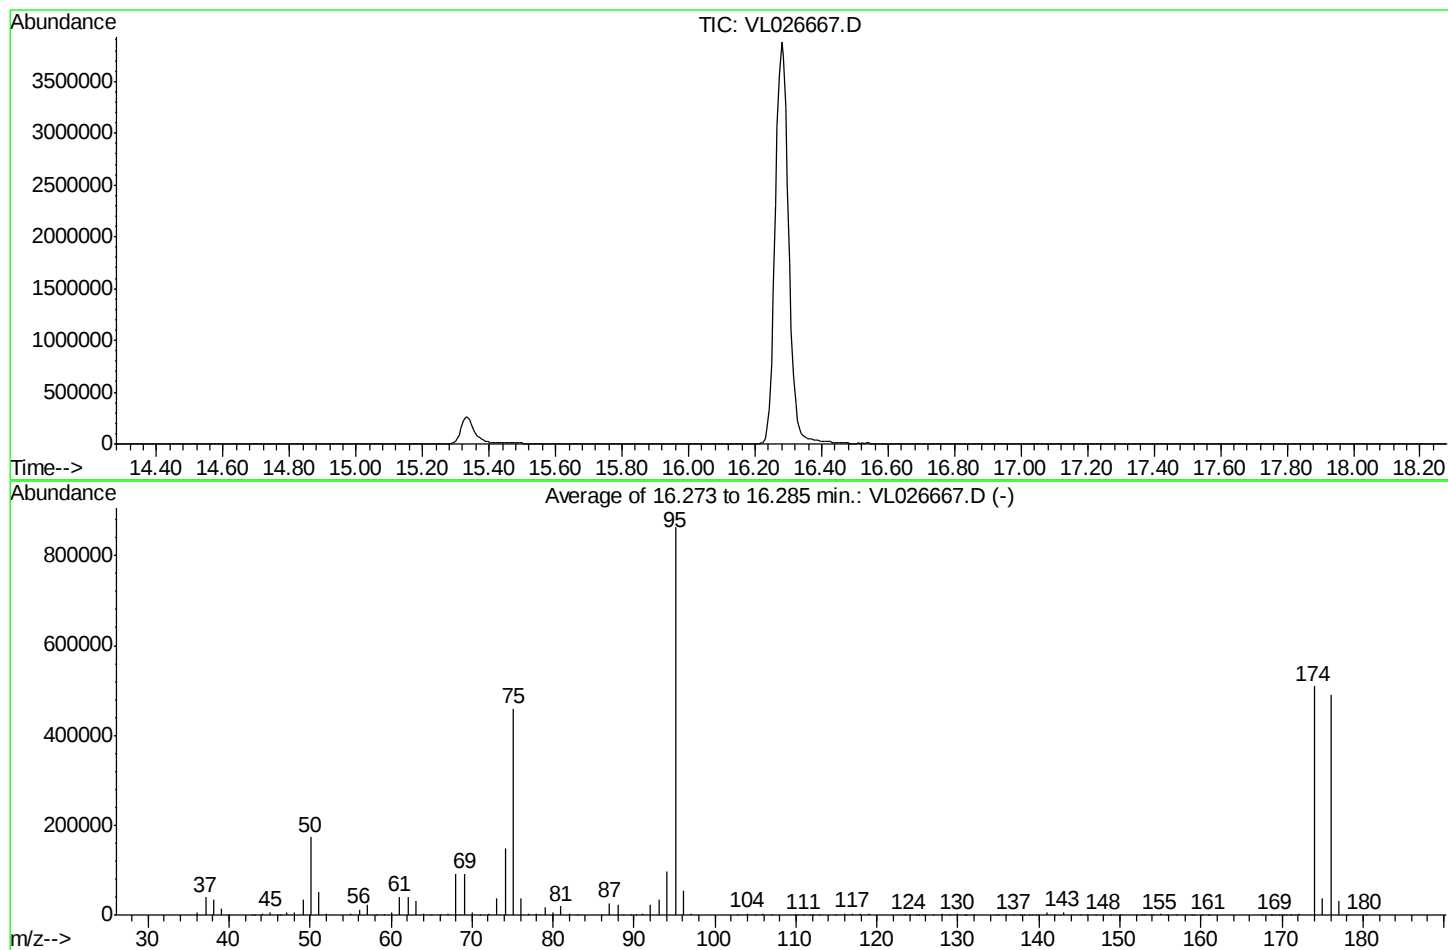

AutoFind: Scans 2163, 2164, 2165; Background Corrected with Scan 2148

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	20.1	173504	PASS
75	95	30	66	53.3	460202	PASS
95	95	100	100	100.0	863189	PASS
96	95	5	9	6.4	55293	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	59.0	509077	PASS
175	174	4	9	7.5	38400	PASS
176	174	93	101	96.5	491200	PASS
177	176	5	9	6.4	31464	PASS