

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
 Data File : VL041907.D
 Acq On : 14 Jan 2025 23:52
 Operator : SY/MD
 Sample : Q1073-03 4X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :


Quant Time: Jan 15 04:22:25 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue Jan 14 23:15:42 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.790	49	138825	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.968	114	414276	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.885	117	367457	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.380	95	288793	9.978	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.800%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.554	85	3138	0.166	ppbv	96
3) Chlorodifluoromethane	1.460	51	4006999	202.276	ppbv #	58
4) Chloromethane	1.466	50	429498	60.393	ppbv #	44
5) Vinyl Chloride	1.473	62	5273	0.732	ppbv #	1
6) Bromomethane	1.473	94	68783	20.035	ppbv #	63
7) Chloroethane	1.466	64	2499652	891.896	ppbv #	56
8) Dichlorotetrafluoroethane	1.554	85	3138	0.190	ppbv	85
9) Propene	1.483	41	4136	0.507	ppbv #	68
10) Heptane	4.981	43	2877	0.132	ppbv	92
13) Ethanol	1.890	45	71049	118.865	ppbv #	31
15) Acetone	1.839	43	115916	6.952	ppbv	93
16) 1,3-Butadiene	1.599	39	5957	0.796	ppbv #	26
17) tert-Butyl alcohol	2.046	59	9302	0.453	ppbv #	83
19) Isopropyl Alcohol	1.890	45	71049	7.187	ppbv	90
20) Methylene Chloride	2.062	84	1646	0.250	ppbv #	74
23) Vinyl Acetate	2.460	43	1466	0.177	ppbv #	50
25) Ethyl Acetate	2.829	43	11788	0.262	ppbv #	82
26) Hexane	2.829	57	17822	1.002	ppbv #	34
34) 2-Butanone	2.564	43	50071	1.901	ppbv	98
35) Carbon Tetrachloride	3.768	117	362	0.014	ppbv #	74
36) Benzene	3.667	78	6801	0.179	ppbv #	89
39) 1,2-Dichloropropane	3.965	63	102316	7.677	ppbv #	22
41) Tetrahydrofuran	3.069	42	3692	0.258	ppbv #	67
51) 2-Hexanone	7.454	43	13871	0.502	ppbv #	98
52) Tetrachloroethene	8.228	164	547	0.042	ppbv #	74
53) Toluene	6.940	91	30861	0.746	ppbv	98
56) 1,1,1,2-Tetrachloroethane	8.674	131	27	0.001	ppbv #	1
58) Ethyl Benzene	9.361	91	1800165	31.347	ppbv	94
59) m/p-Xylene	9.361	91	1800165	39.108	ppbv #	78
60) o-Xylene	9.969	91	8606	0.188	ppbv	100
61) Styrene	9.875	104	299816	14.628	ppbv	98
62) Isopropylbenzene	10.545	105	24044	0.340	ppbv	99
64) n-propylbenzene	10.992	120	1829	0.102	ppbv	65
74) 1,2,4-Trimethylbenzene	11.539	105	6607	0.126	ppbv #	53
80) Naphthalene,2-methyl-	14.465	142	148	0.006	ppbv #	57

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jan 15 04:22:25 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug 26 06:05:16 2022
QLast Update : Tue Jan 14 23:15:42 2025
Response via : Initial Calibration









#1
 Bromochloromethane
 Concen: 10.000 ppbv
 RT: 2.790 min Scan# 81
 Delta R.T. -0.007 min
 Lab File: VL041907.D
 Acq: 14 Jan 2025 23:52




Instrument :
 MSVOA_L
 ClientSampleId :


Tgt Ion: 49 Resp: 138825
 Ion Ratio Lower Upper
 49 100
 128 49.8 24.3 73.0
 130 61.6 31.1 93.2



#2
 Dichlorodifluoromethane
 Concen: 0.166 ppbv
 RT: 1.554 min Scan# 453
 Delta R.T. 0.052 min
 Lab File: VL041907.D
 Acq: 14 Jan 2025 23:52

Tgt Ion: 85 Resp: 3138
 Ion Ratio Lower Upper
 85 100
 87 33.1 24.9 37.3


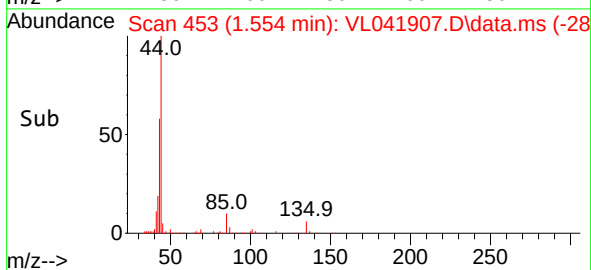






#3
Chlorodifluoromethane
Concen: 202.276 ppbv
RT: 1.460 min Scan# 41
Delta R.T. -0.019 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 51 Resp: 4006999
Ion Ratio Lower Upper
51 100
67 0.0 15.0 22.4#

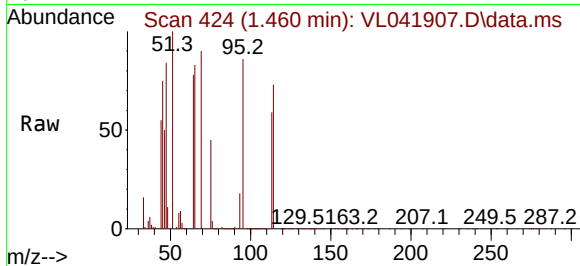

#4
Chloromethane
Concen: 60.393 ppbv
RT: 1.466 min Scan# 426
Delta R.T. -0.071 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52

Tgt Ion: 50 Resp: 429498
Ion Ratio Lower Upper
50 100
52 0.0 24.6 36.8#




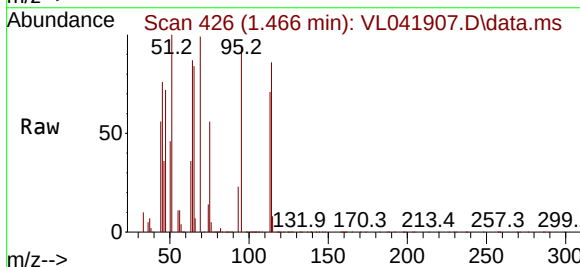




#5
 Vinyl Chloride
 Concen: 0.732 ppbv
 RT: 1.473 min Scan# 41
 Delta R.T. -0.110 min
 Lab File: VL041907.D
 Acq: 14 Jan 2025 23:52




Instrument :
 MSVOA_L
 ClientSampleId :


Tgt Ion: 62 Resp: 5273
 Ion Ratio Lower Upper
 62 100
 64 8404.2 26.1 39.1#

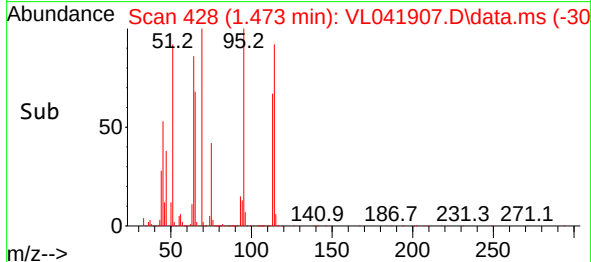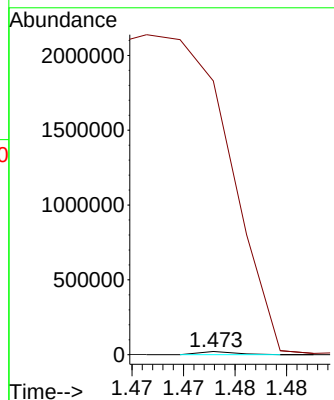

#6
 Bromomethane
 Concen: 20.035 ppbv
 RT: 1.473 min Scan# 428
 Delta R.T. -0.201 min
 Lab File: VL041907.D
 Acq: 14 Jan 2025 23:52

Tgt Ion: 94 Resp: 68783
 Ion Ratio Lower Upper
 94 100
 96 52.8 69.5 104.3#


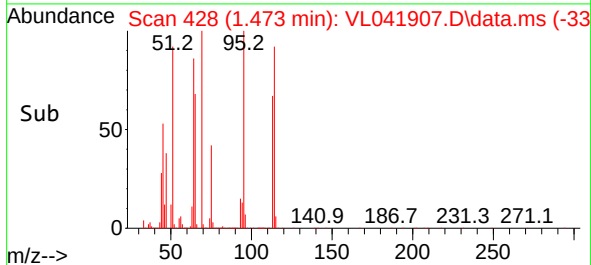
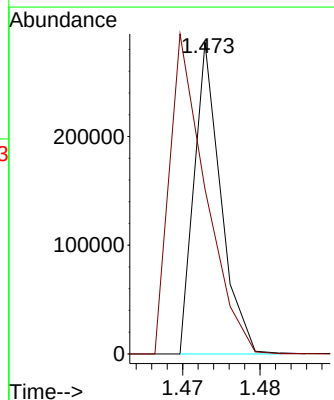





#7
Chloroethane
Concen: 891.896 ppbv
RT: 1.466 min Scan# 41
Delta R.T. -0.243 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 64 Resp: 2499652
Ion Ratio Lower Upper
64 100
66 7.7 25.7 38.5#

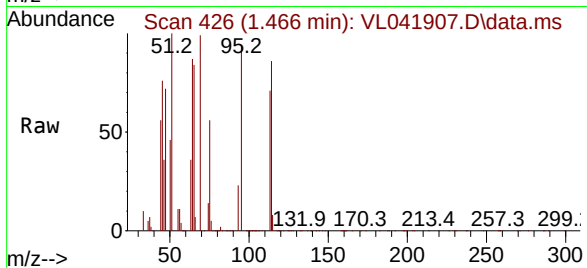

#8
Dichlorotetrafluoroethane
Concen: 0.190 ppbv
RT: 1.554 min Scan# 453
Delta R.T. -0.003 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52

Tgt Ion: 85 Resp: 3138
Ion Ratio Lower Upper
85 100
135 51.1 50.0 75.0




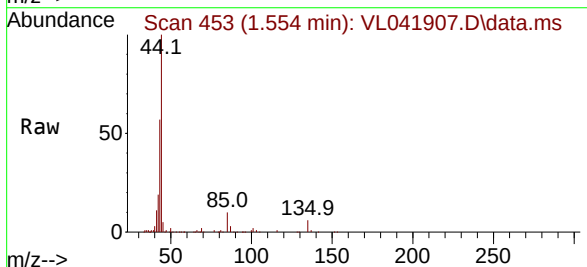




#9
Propene
Concen: 0.507 ppbv
RT: 1.483 min Scan# 41
Delta R.T. -0.003 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 41 Resp: 4136
Ion Ratio Lower Upper
41 100
42 90.0 52.0 78.0#

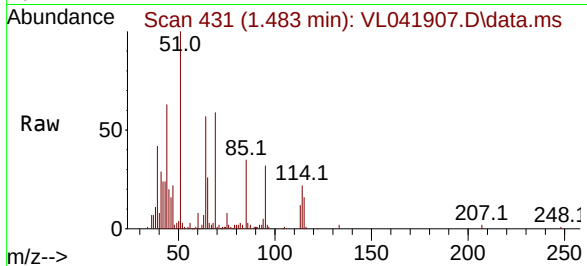

#10
Heptane
Concen: 0.132 ppbv
RT: 4.981 min Scan# 1512
Delta R.T. -0.019 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52

Tgt Ion: 43 Resp: 2877
Ion Ratio Lower Upper
43 100
57 56.8 41.0 61.4




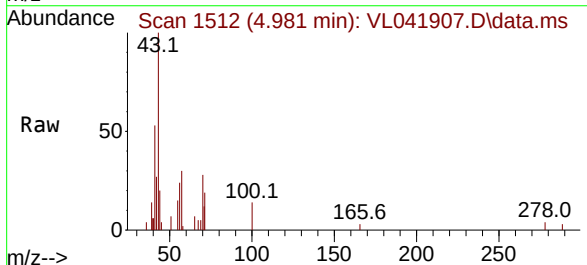




#13
Ethanol
Concen: 118.865 ppbv
RT: 1.890 min Scan# 51
Delta R.T. 0.165 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 45 Resp: 71049
Ion Ratio Lower Upper
45 100
46 0.0 18.1 72.5#

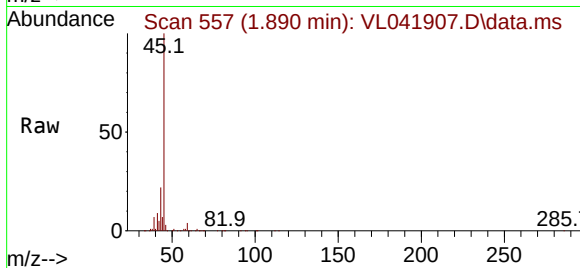

#15
Acetone
Concen: 6.952 ppbv
RT: 1.839 min Scan# 541
Delta R.T. -0.003 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52

Tgt Ion: 43 Resp: 115916
Ion Ratio Lower Upper
43 100
58 31.0 21.9 32.9




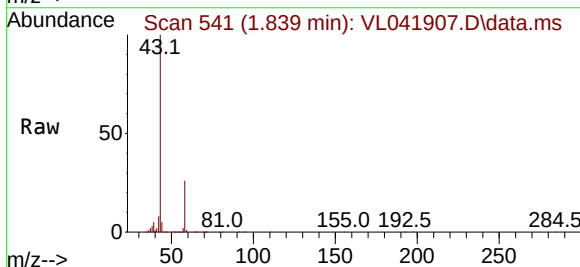




#16
1,3-Butadiene
Concen: 0.796 ppbv
RT: 1.599 min Scan# 41
Delta R.T. -0.013 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 39 Resp: 5957
Ion Ratio Lower Upper
39 100
54 12.7 61.6 92.4#

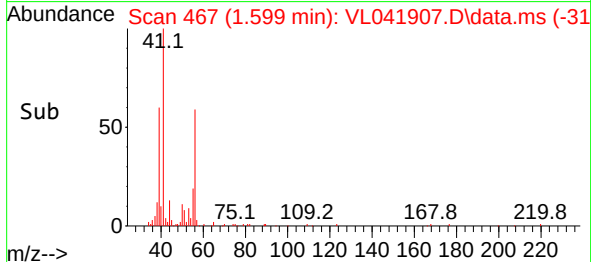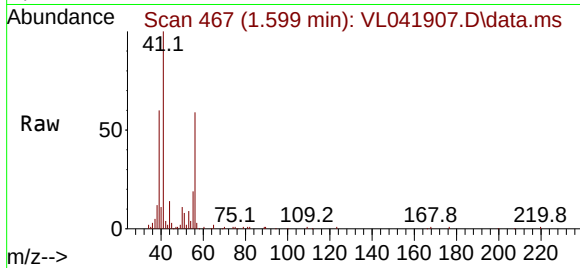

#17
tert-Butyl alcohol
Concen: 0.453 ppbv
RT: 2.046 min Scan# 605
Delta R.T. 0.000 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52

Tgt Ion: 59 Resp: 9302
Ion Ratio Lower Upper
59 100
57 16.0 7.8 11.8#




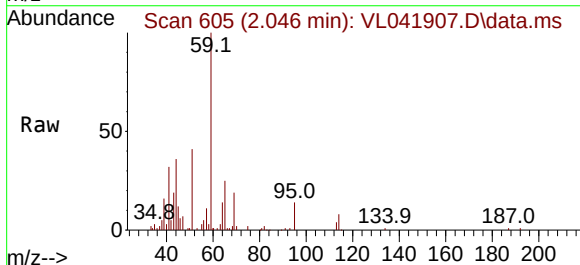




#19
Isopropyl Alcohol
Concen: 7.187 ppbv
RT: 1.890 min Scan# 51
Delta R.T. 0.000 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 45 Resp: 71049
Ion Ratio Lower Upper
45 100
58 50.6 35.0 52.6

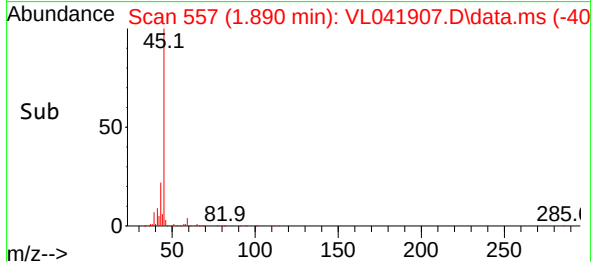

#20
Methylene Chloride
Concen: 0.250 ppbv
RT: 2.062 min Scan# 610
Delta R.T. -0.006 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52


Tgt Ion: 84 Resp: 1646
Ion Ratio Lower Upper
84 100
49 113.7 123.1 184.7#
51 44.4 35.8 53.8
86 43.0 53.7 80.5#

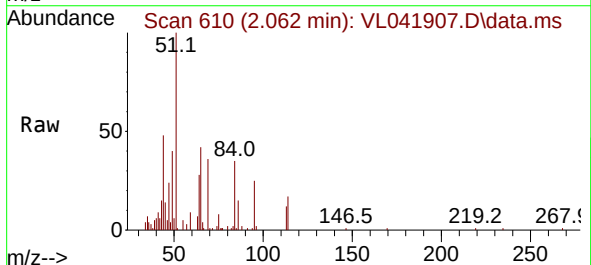






#23
 Vinyl Acetate
 Concen: 0.177 ppbv
 RT: 2.460 min Scan# 71
 Delta R.T. -0.010 min
 Lab File: VL041907.D
 Acq: 14 Jan 2025 23:52


Instrument :
 MSVOA_L
 ClientSampleId :





Tgt Ion: 43	Resp: 1466
Ion Ratio	Lower Upper
43 100	
86 5.8	6.2 9.4#
42 0.0	8.5 12.7#
44 55.9	4.8 7.2#

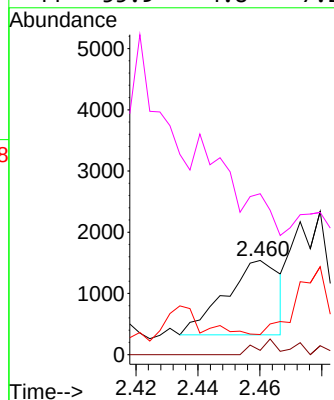


#25
 Ethyl Acetate
 Concen: 0.262 ppbv
 RT: 2.829 min Scan# 847
 Delta R.T. -0.016 min
 Lab File: VL041907.D
 Acq: 14 Jan 2025 23:52




Tgt	Ion: 43	Resp:	11788
Ion	Ratio	Lower	Upper
43	100		
45	3.7	8.2	12.2#
61	1.9	7.4	11.0#
70	3.1	7.0	10.4#

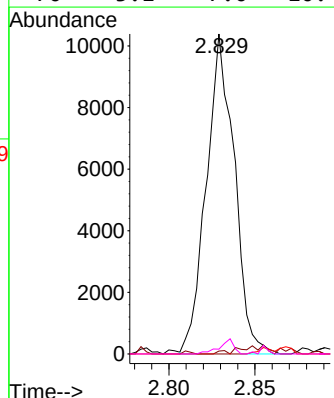






#26
Hexane
Concen: 1.002 ppbv
RT: 2.829 min Scan# 84
Delta R.T. -0.006 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52

Instrument :
MSVOA_L
ClientSampleId :



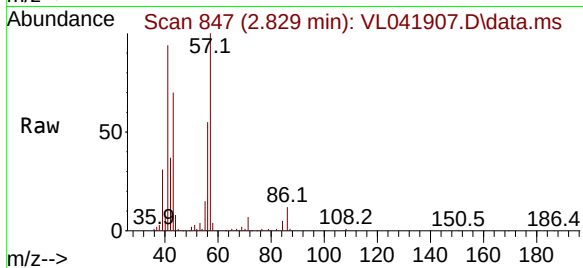



Tgt Ion: 57 Resp: 17822
Ion Ratio Lower Upper
57 100
41 92.4 73.8 110.8
43 67.1 197.3 295.9#
56 51.9 42.7 64.1



#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 3.968 min Scan# 1199
Delta R.T. -0.006 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52

Tgt Ion:114 Resp: 414276
Ion Ratio Lower Upper
114 100
63 24.7 19.8 29.6
88 18.0 14.4 21.6




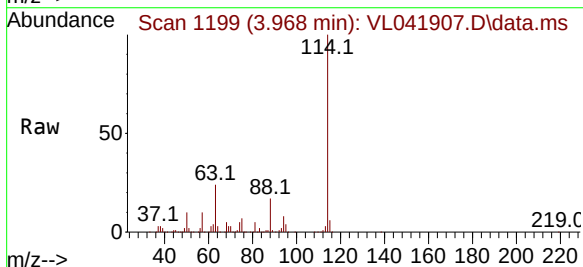




#34
2-Butanone
Concen: 1.901 ppbv
RT: 2.564 min Scan# 7
Delta R.T. -0.003 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 43 Resp: 50071
Ion Ratio Lower Upper
43 100
72 24.3 18.6 28.0

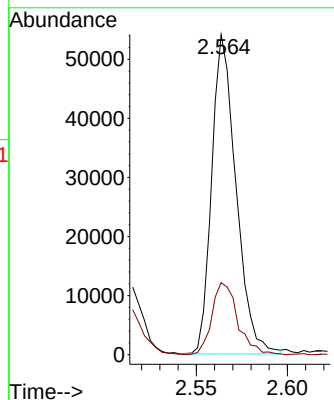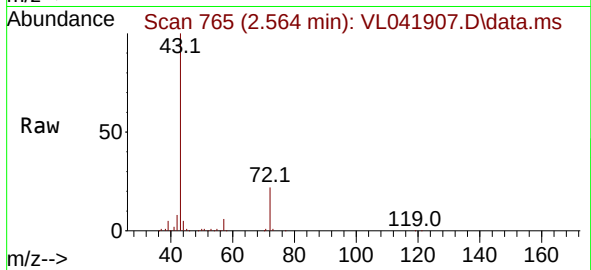

#35
Carbon Tetrachloride
Concen: 0.014 ppbv
RT: 3.768 min Scan# 1137
Delta R.T. -0.010 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52

Tgt Ion: 117 Resp: 362
Ion Ratio Lower Upper
117 100
119 73.2 76.9 115.3#
121 11.5 23.8 35.6#

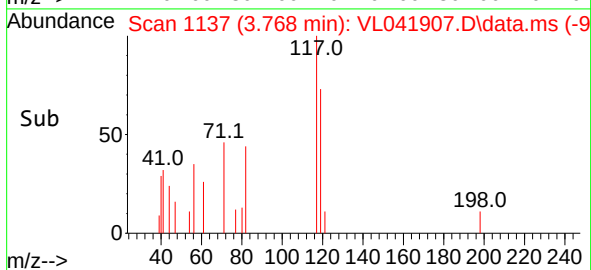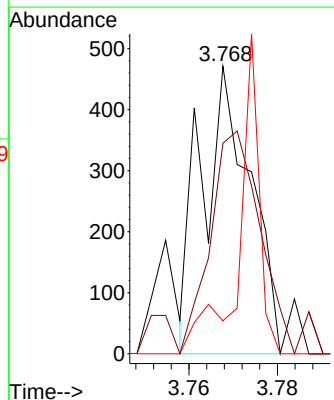



#36

Benzene

Concen: 0.179 ppbv

RT: 3.667 min Scan# 1106

Delta R.T. -0.003 min

Lab File: VL041907.D





Acq: 14 Jan 2025 23:52

Instrument :

MSVOA_L

ClientSampleId :

Tgt Ion: 78	Resp: 6801
Ion Ratio	Lower Upper
78 100	
77 21.5	18.1 27.1
50 8.9	15.2 22.8

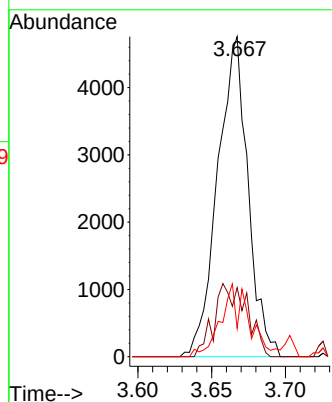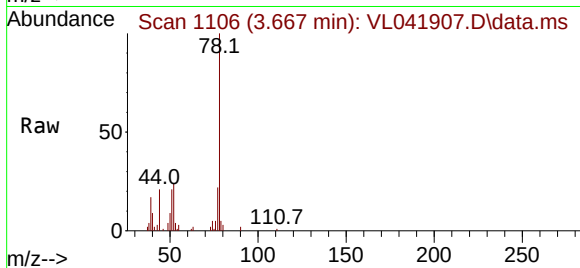

#39

1,2-Dichloropropane

Concen: 7.677 ppbv




RT: 3.965 min Scan# 1198


Delta R.T. -0.366 min

Lab File: VL041907.D

Acq: 14 Jan 2025 23:52

Tgt Ion: 63	Resp: 102316
Ion Ratio	Lower Upper
63 100	
41 0.3	63.7 95.5
62 17.1	55.4 83.2



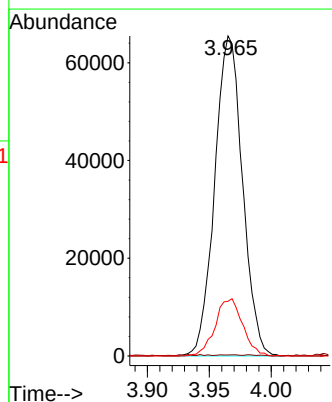
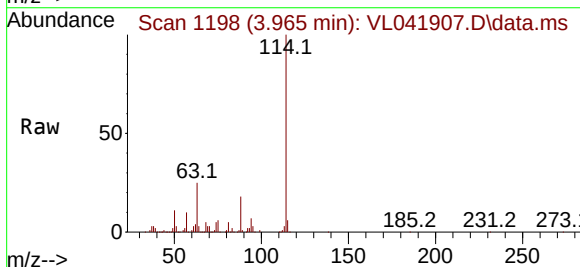




#41
Tetrahydrofuran
Concen: 0.258 ppbv
RT: 3.069 min Scan# 91
Delta R.T. 0.003 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 42 Resp: 3692
Ion Ratio Lower Upper
42 100
72 22.5 32.3 48.5#
71 14.8 29.9 44.9#

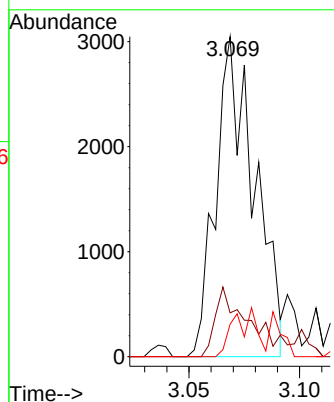

#51
2-Hexanone
Concen: 0.502 ppbv
RT: 7.454 min Scan# 2276
Delta R.T. 0.000 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52


Tgt Ion: 43 Resp: 13871
Ion Ratio Lower Upper
43 100
58 52.1 40.4 60.6
98 0.8 0.2 0.2#

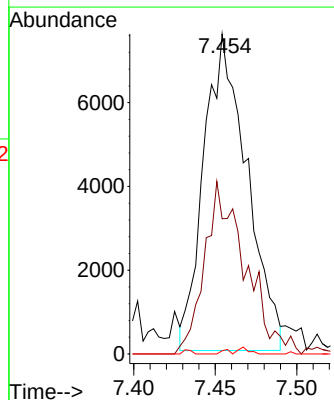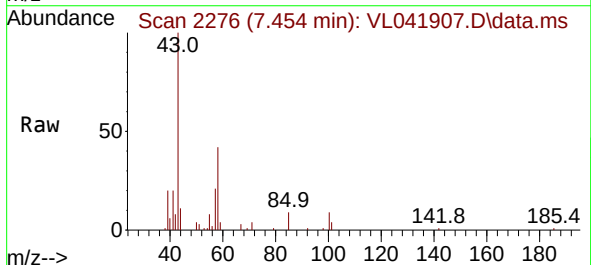






#52
Tetrachloroethene
Concen: 0.042 ppbv
RT: 8.228 min Scan# 2117
Delta R.T. -0.013 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52

Instrument :
MSVOA_L
ClientSampleId :







Tgt Ion:164 Resp: 547
Ion Ratio Lower Upper
164 100
166 92.2 100.8 151.2#
129 89.5 82.0 123.0
131 64.2 80.2 120.2#

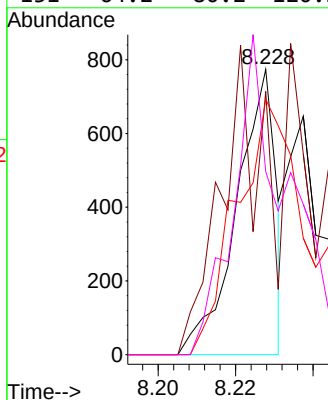

#53
Toluene
Concen: 0.746 ppbv
RT: 6.940 min Scan# 2117
Delta R.T. -0.013 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52


Tgt Ion: 91 Resp: 30861
Ion Ratio Lower Upper
91 100
92 61.0 47.4 71.0

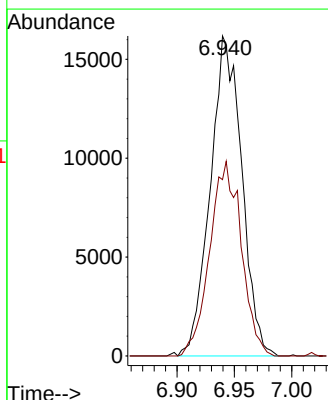






#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.885 min Scan# 21
Delta R.T. -0.010 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52

Instrument :
MSVOA_L
ClientSampleId :







Tgt Ion:117 Resp: 367457
Ion Ratio Lower Upper
117 100
82 64.3 54.2 81.4
119 31.6 25.0 37.6

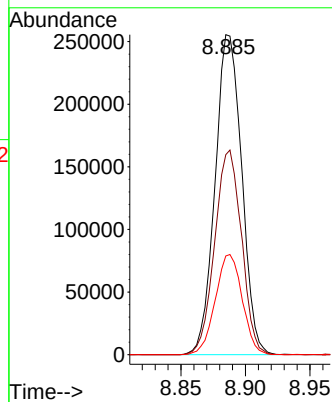

#56
1,1,1,2-Tetrachloroethane
Concen: 0.001 ppbv
RT: 8.674 min Scan# 2653
Delta R.T. -0.265 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52

Tgt Ion:131 Resp: 27
Ion Ratio Lower Upper
131 100
133 103.7 76.0 114.0
119 430522.2 49.7 74.5#

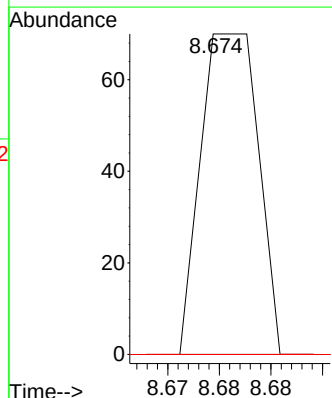



#58

Ethyl Benzene

Concen: 31.347 ppbv

RT: 9.361 min Scan# 2865

Delta R.T. -0.006 min

Lab File: VL041907.D

Acq: 14 Jan 2025 23:52

Instrument :

MSVOA_L





ClientSampleId :

Tgt Ion: 91 Resp: 1800165

Ion Ratio Lower Upper

91 100

106 32.0 23.1 34.7

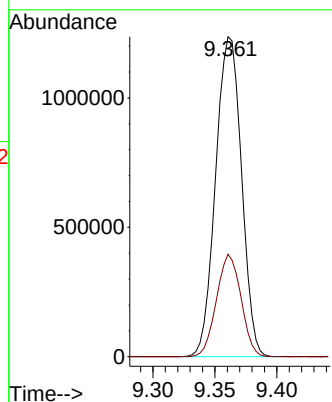

#59

m/p-Xylene

Concen: 39.108 ppbv

RT: 9.361 min Scan# 2865

Delta R.T. -0.204 min

Lab File: VL041907.D




Acq: 14 Jan 2025 23:52


Tgt Ion: 91 Resp: 1800165

Ion Ratio Lower Upper

91 100

106 30.3 36.0 54.0#


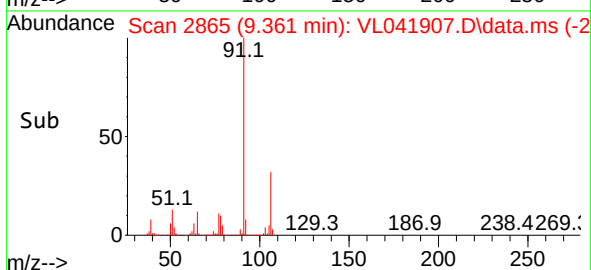






#60
o-Xylene
Concen: 0.188 ppbv
RT: 9.969 min Scan# 3056
Delta R.T. -0.010 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 91 Resp: 8606
Ion Ratio Lower Upper
91 100
106 42.4 21.3 63.9

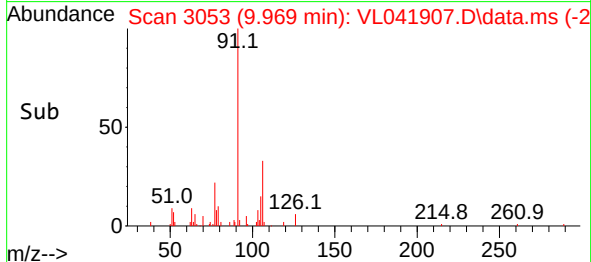

#61
Styrene
Concen: 14.628 ppbv
RT: 9.875 min Scan# 3024
Delta R.T. -0.010 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52

Tgt Ion:104 Resp: 299816
Ion Ratio Lower Upper
104 100
78 52.7 41.0 61.6
103 47.2 37.2 55.8




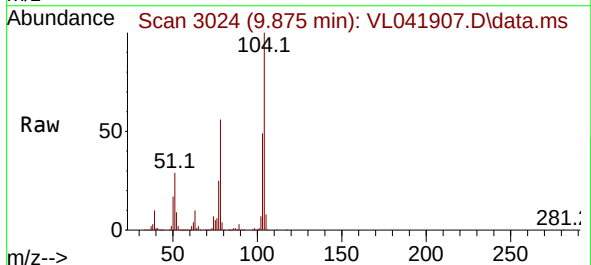




#62
Isopropylbenzene
Concen: 0.340 ppbv
RT: 10.545 min Scan# 31
Delta R.T. -0.006 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion:105 Resp: 24044
Ion Ratio Lower Upper
105 100
120 24.7 20.3 30.5

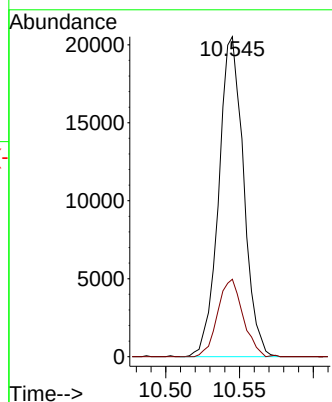

#64
n-propylbenzene
Concen: 0.102 ppbv
RT: 10.992 min Scan# 3369
Delta R.T. -0.010 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52

Tgt Ion:120 Resp: 1829
Ion Ratio Lower Upper
120 100
91 558.8 374.1 561.1


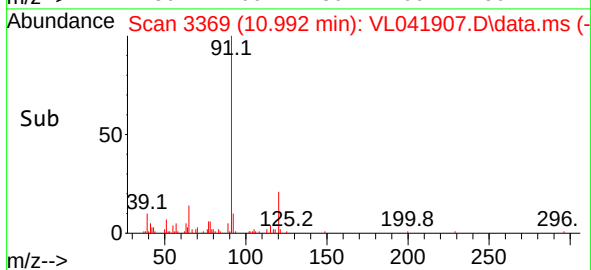
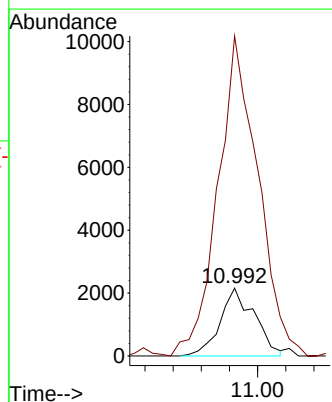



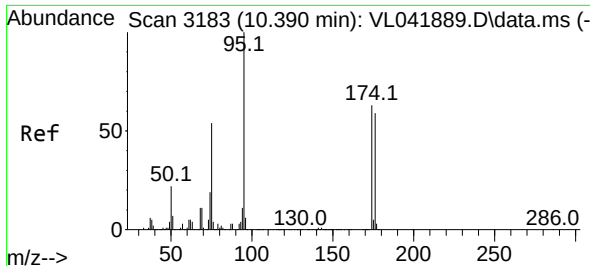

#68
1-Bromo-4-Fluorobenzene
Concen: 9.978 ppbv
RT: 10.380 min Scan# 3183
Delta R.T. -0.010 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 95 Resp: 288793
Ion Ratio Lower Upper
95 100
174 60.5 49.0 73.4
175 4.9 3.8 5.8

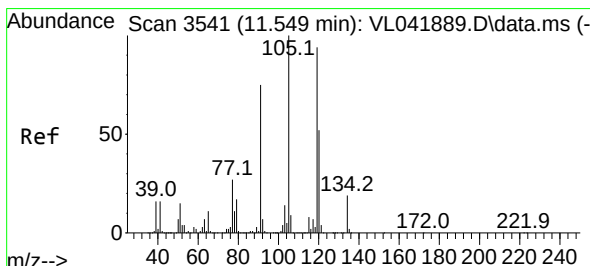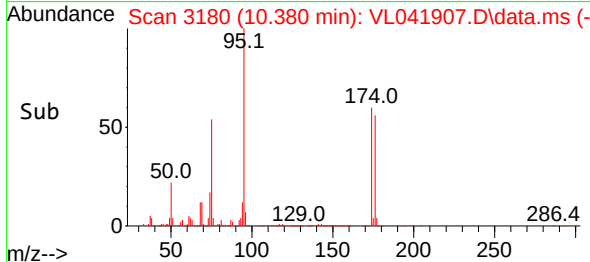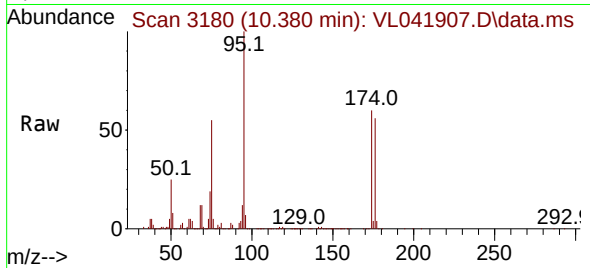

#74
1,2,4-Trimethylbenzene
Concen: 0.126 ppbv
RT: 11.539 min Scan# 3538
Delta R.T. -0.010 min
Lab File: VL041907.D
Acq: 14 Jan 2025 23:52

Tgt Ion: 105 Resp: 6607
Ion Ratio Lower Upper
105 100
120 42.0 41.4 62.2
91 12.3 60.2 90.2#
77 10.0 22.0 33.0#

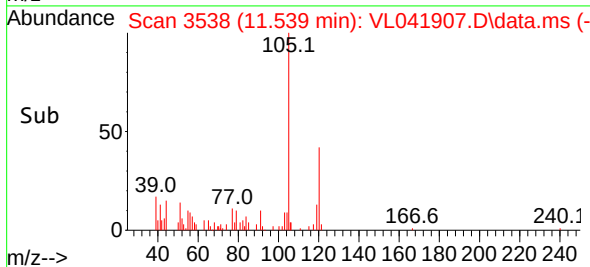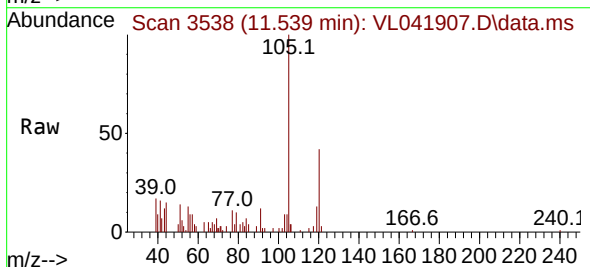



#80

Naphthalene, 2-methyl-

Concen: 0.006 ppbv

RT: 14.465 min Scan# 44

Delta R.T. -0.006 min


Lab File: VL041907.D

Acq: 14 Jan 2025 23:52

Instrument :

MSVOA_L

ClientSampleId :

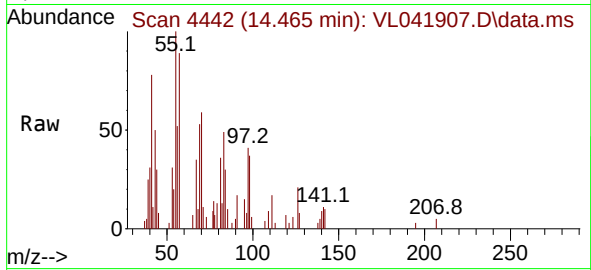

Tgt Ion:142 Resp: 148

Ion Ratio Lower Upper

142 100

141 129.1 68.1 102.1#

115 59.5 31.7 47.5#

