
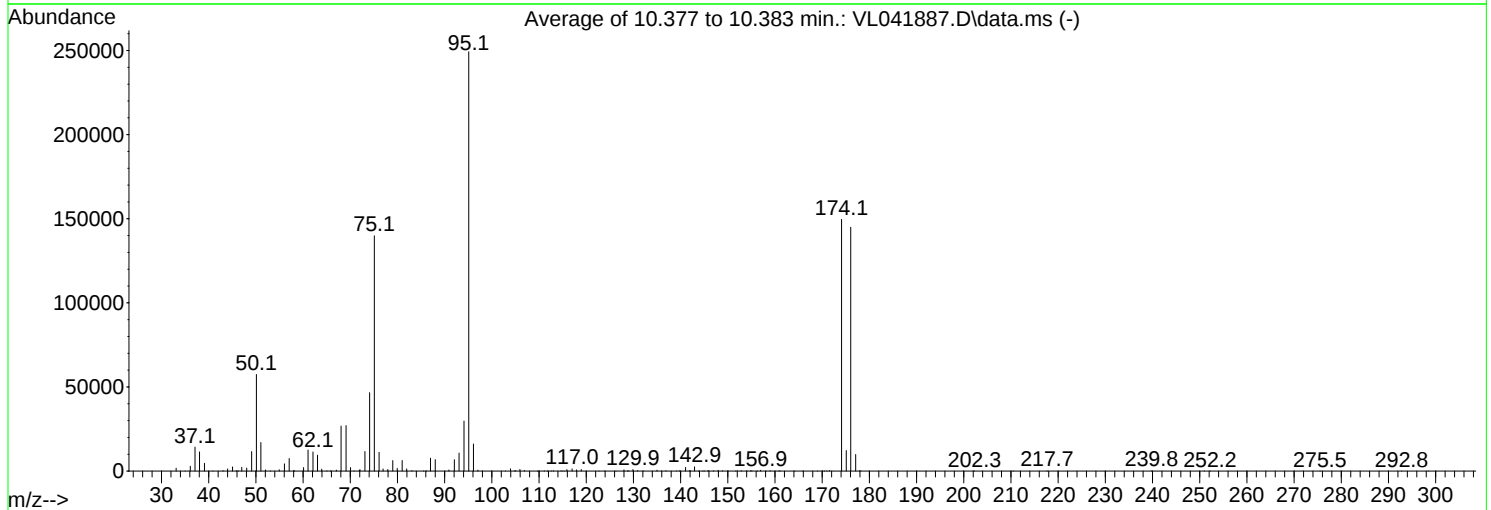


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
Data File : VL041887.D
Acq On : 14 Jan 2025 07:50
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Jan 14 23:15:42 2025

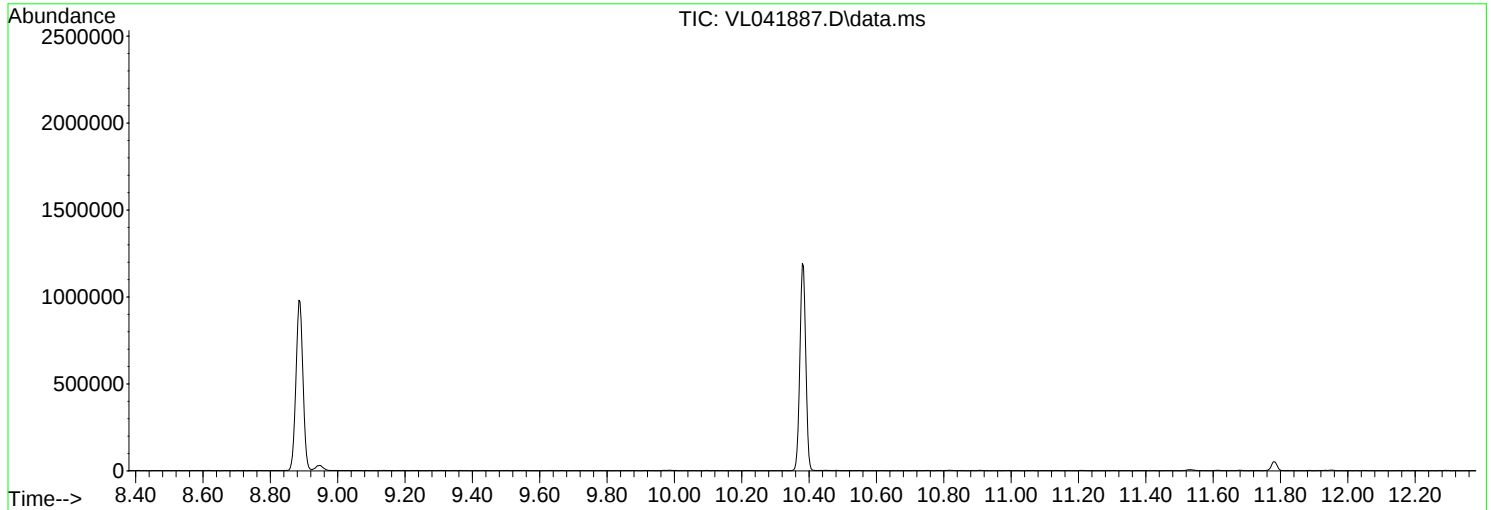

AutoFind: Scans 3179, 3180, 3181; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.0	57448	PASS
75	95	30	66	56.1	139893	PASS
95	95	100	100	100.0	249280	PASS
96	95	5	9	6.5	16102	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	60.0	149632	PASS
175	174	4	9	8.2	12223	PASS
176	174	93	101	96.8	144917	PASS
177	176	5	9	6.8	9838	PASS

Average of 10.377 to 10.383 min.: VL041887.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1721	46.25	187	58.00	217	69.10	27064
35.00	34	47.00	2270	58.20	169	70.05	2086
36.10	2904	48.05	1800	60.10	2093	70.80	62
37.10	14256	49.10	11606	61.05	12532	71.90	478
38.05	11416	50.10	57448	62.10	11347	72.05	855
39.10	4640	51.05	16983	63.05	9441	73.10	11647
40.90	20	52.05	698	63.95	1185	74.10	46637
43.05	223	53.10	70	65.05	142	75.10	139893
44.00	1302	54.95	811	65.80	140	76.10	11160
45.05	2448	56.05	4320	67.05	599	76.95	1289
45.85	203	57.05	7492	68.05	26765	77.95	981

Average of 10.377 to 10.383 min.: VL041887.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.00	6243	93.05	10708	106.90	325	117.00	1338
79.95	1666	94.10	29779	109.70	72	117.95	731
81.00	6311	95.10	249280	110.00	50	118.95	953
81.95	1325	96.10	16102	111.10	152	122.70	24
83.05	258	97.05	586	111.80	111	123.95	57
85.55	75	98.00	64	112.60	51	126.30	40
86.10	108	102.90	20	113.05	210	128.00	751
87.00	7686	103.95	1357	114.65	88	128.75	209
88.00	6856	104.80	96	114.90	24	129.00	149
90.90	686	105.05	252	115.30	44	129.90	917
92.05	6774	105.95	966	115.90	891	130.90	280

Average of 10.377 to 10.383 min.: VL041887.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
132.10	22	144.00	36	152.85	252	165.90	17
135.00	547	144.70	54	154.05	188	169.00	21
136.00	45	145.00	117	154.85	333	170.10	20
136.90	224	145.80	267	155.10	178	170.45	75
139.10	30	146.00	132	156.30	48	171.00	82
139.80	185	146.95	170	156.95	484	171.55	299
141.05	2202	147.95	449	158.10	23	174.10	149632
141.85	250	148.85	204	158.95	237	175.10	12223
142.10	215	150.05	156	160.85	178	176.05	144917
142.95	2558	151.60	28	161.10	61	177.10	9838
143.80	73	152.00	94	164.20	20	177.95	205

Average of 10.377 to 10.383 min.: VL041887.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
178.20	123						
202.00	26						
202.30	27						
210.50	25						
217.65	77						
239.80	44						
251.00	21						
252.20	26						
275.50	23						
292.80	18						
298.50	17						

Instrument :

MSVOA_L

ClientSampleId :

BFB