
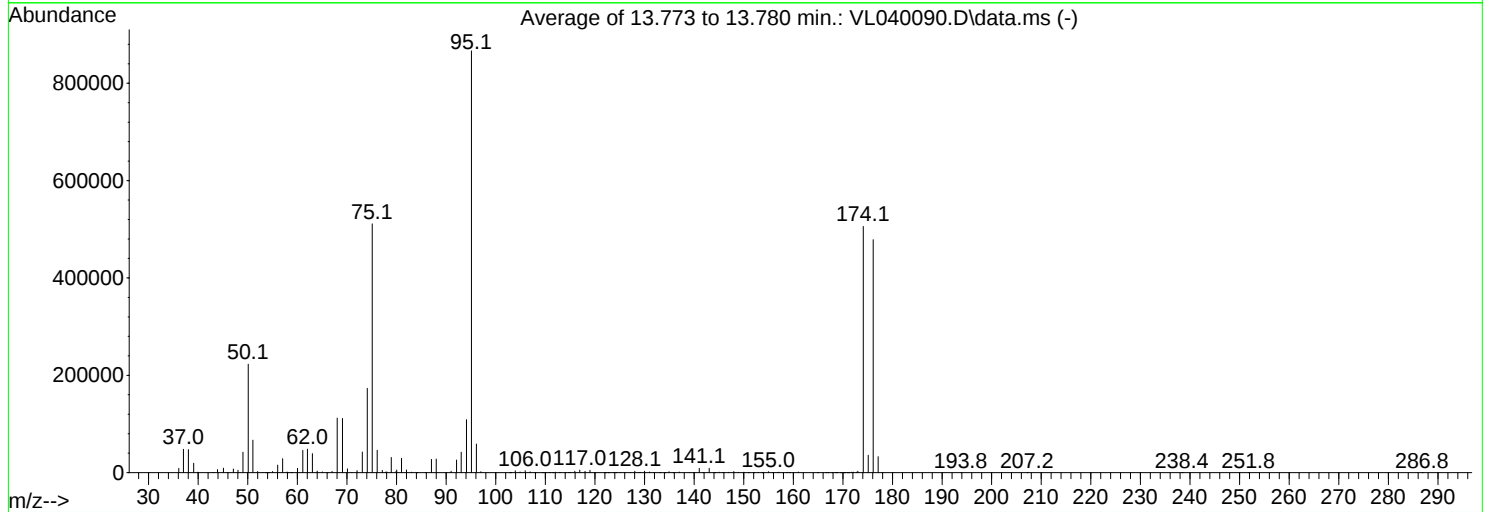


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011623\
 Data File : VL040090.D
 Acq On : 16 Jan 2023 9:39
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011623AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Mon Jan 16 14:40:47 2023

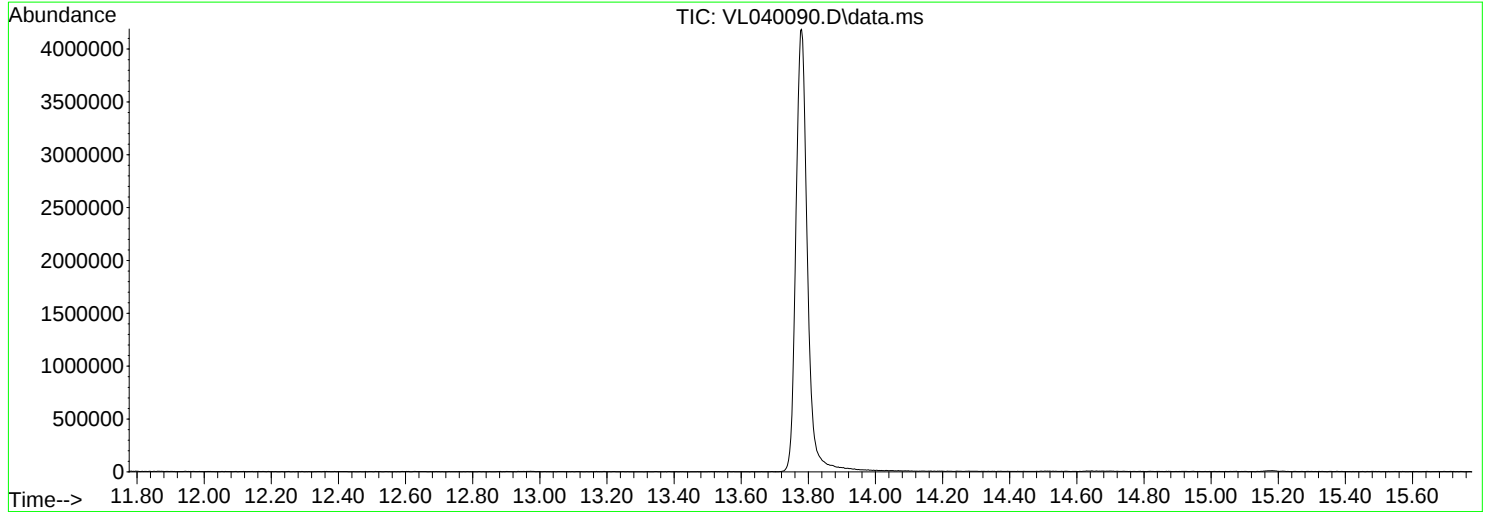

AutoFind: Scans 3474, 3475, 3476; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.7	222805	PASS
75	95	30	66	59.0	511275	PASS
95	95	100	100	100.0	866560	PASS
96	95	5	9	6.8	58731	PASS
173	174	0.00	2	0.6	2994	PASS
174	95	50	120	58.4	505963	PASS
175	174	4	9	7.1	35693	PASS
176	174	93	101	94.6	478763	PASS
177	176	5	9	6.9	32816	PASS

Average of 13.773 to 13.780 min.: VL040090.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	8832	48.05	5099	57.95	1443	68.05	11206
37.05	48043	49.05	42037	58.30	451	69.10	11143
38.05	47357	50.10	222805	58.80	76	70.10	793
39.10	19563	51.05	66808	60.05	8948	71.00	25
39.95	928	52.00	2459	61.10	45755	72.05	4176
42.85	299	53.05	349	62.05	48387	73.10	42491
43.20	344	53.60	65	63.05	39136	74.10	173227
43.90	6130	54.15	148	64.00	3183	75.10	511275
45.10	9379	55.00	2323	65.05	1736	76.10	45939
46.05	824	56.05	15526	66.00	153	77.15	4731
47.10	7612	57.05	28469	67.00	2698	77.80	898

Average of 13.773 to 13.780 min.: VL040090.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.05	1641	88.00	27904	103.95	3887	112.00	916
78.95	31192	90.10	200	104.90	1251	112.90	769
79.90	2557	91.00	3019	105.95	3873	113.10	371
80.05	5390	92.10	26053	106.95	1686	113.95	178
81.00	29648	93.05	41952	107.90	80	114.65	325
82.00	5733	94.10	108963	109.40	87	114.90	259
83.05	1030	95.10	866560	109.90	158	115.15	566
84.10	93	96.10	58731	110.15	263	115.95	2985
85.80	201	97.00	1824	110.80	501	116.95	5380
86.05	329	102.80	99	111.10	371	118.00	2813
87.05	27344	103.00	172	111.50	121	119.00	4954

Average of 13.773 to 13.780 min.: VL040090.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.90	146	128.05	3069	139.15	541	146.95	729
121.90	95	128.85	808	139.90	757	148.00	2484
122.20	117	129.10	686	141.05	8989	148.90	554
122.70	82	130.00	2883	141.80	348	150.05	1034
123.00	249	131.00	1485	141.95	426	150.90	102
123.75	347	131.90	238	143.05	8930	152.00	159
124.00	221	133.10	60	143.90	338	152.95	641
124.20	123	134.10	104	144.20	116	153.70	58
125.15	258	134.95	1880	145.05	1121	153.95	545
126.00	360	135.80	136	145.70	255	155.00	1856
127.15	320	137.00	1392	146.00	752	155.85	148

Average of 13.773 to 13.780 min.: VL040090.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.90	410	168.50	128	173.00	2994		
157.10	1005	168.80	172	174.10	505963		
158.00	222	169.50	132	175.10	35693		
158.60	211	169.80	381	176.10	478763		
158.85	529	170.10	115	177.10	32816		
159.20	159	170.40	168	178.05	793		
161.00	1443	170.90	156	193.80	61		
164.90	155	171.20	133	207.15	166		
166.60	67	171.80	981	238.40	86		
167.00	139	172.10	1180	251.80	56		
167.80	50	172.80	959	286.80	74		