


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011624\
Data File : VL040981.D
Acq On : 16 Jan 2024 9:53
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL122023AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Jan 17 00:20:56 2024

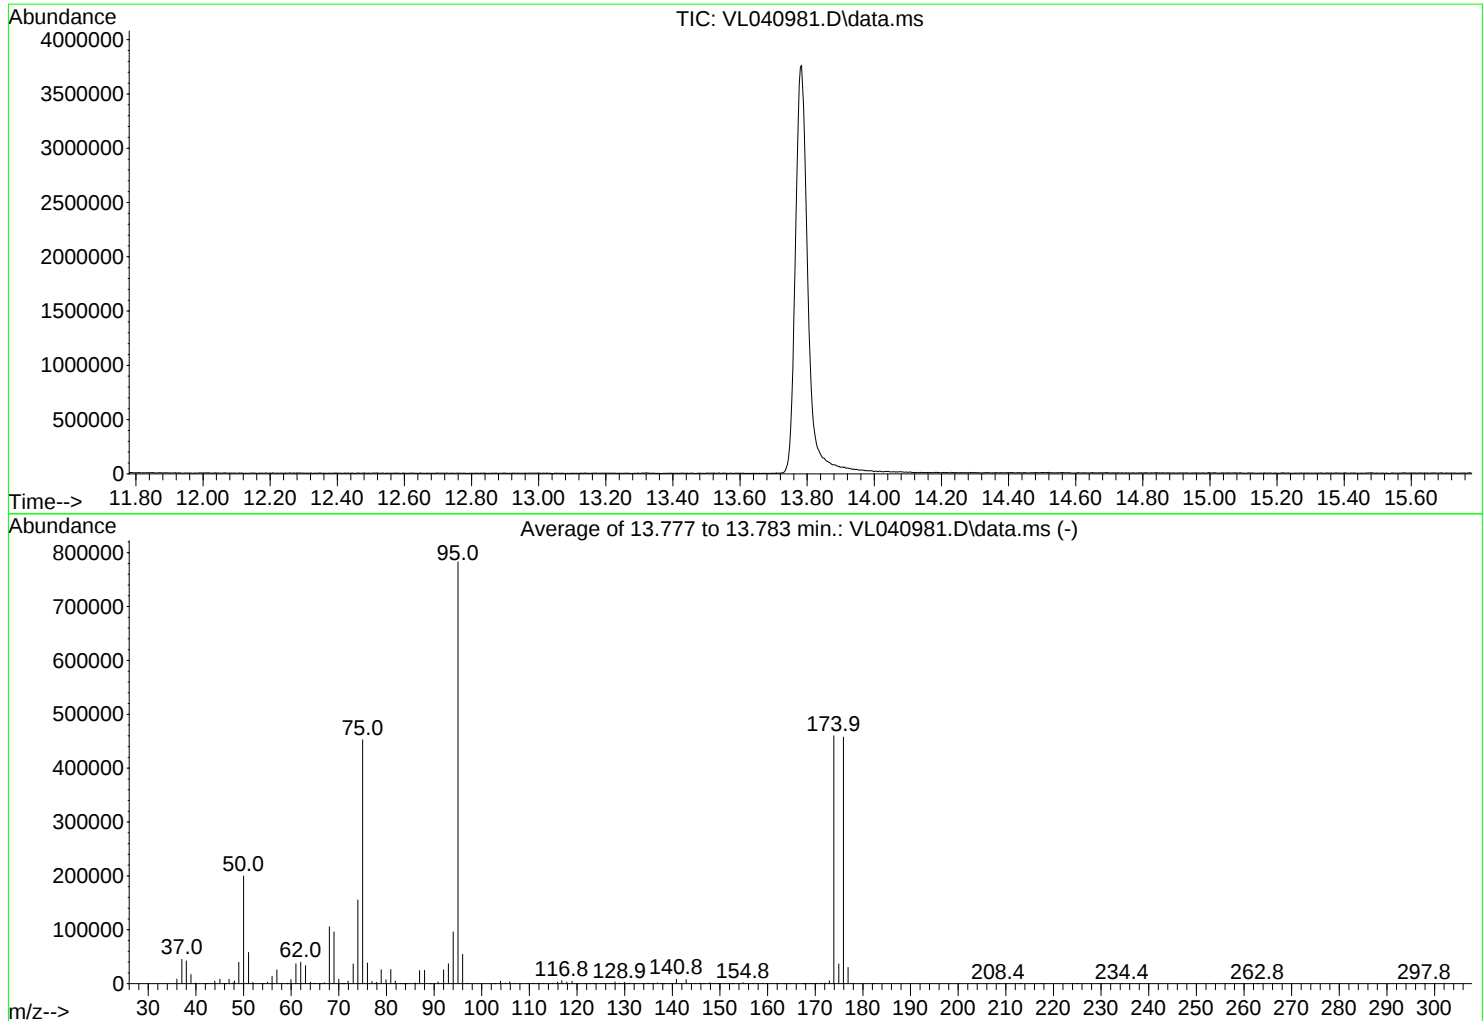

AutoFind: Scans 3475, 3476, 3477; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.5	199829	PASS
75	95	30	66	57.8	452779	PASS
95	95	100	100	100.0	783061	PASS
96	95	5	9	7.0	54616	PASS
173	174	0.00	2	1.2	5344	PASS
174	95	50	120	58.8	460139	PASS
175	174	4	9	8.0	36600	PASS
176	174	93	101	99.5	457728	PASS
177	176	5	9	6.6	30083	PASS

Average of 13.777 to 13.783 min.: VL040981.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	8473	46.20	126	55.05	2575	65.00	561
37.05	45179	46.95	8027	56.00	13814	65.20	341
38.00	42077	47.80	1385	57.00	25528	65.80	5
38.95	16980	48.10	4752	58.05	781	66.10	5
39.90	1138	49.00	39872	59.10	61	66.80	489
42.20	58	50.00	199829	59.95	7359	67.00	1881
42.75	176	51.05	57805	61.00	36920	68.00	105352
43.20	436	51.95	2133	62.00	39963	69.00	96061
43.95	4811	53.20	171	63.00	33709	70.00	8194
45.05	8476	53.85	269	64.05	2787	70.80	149
45.80	64	54.10	88	64.80	184	71.10	125

Average of 13.777 to 13.783 min.: VL040981.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
71.95	4719	81.85	4866	93.00	36709	106.90	657
73.00	36621	82.90	502	94.00	96064	109.70	551
74.00	155328	83.20	303	95.00	783061	110.60	248
75.00	452779	83.70	75	96.00	54616	110.95	807
76.00	38416	84.20	70	96.90	688	112.00	878
76.95	3809	86.00	1223	97.10	441	112.80	487
77.70	679	86.95	24395	102.70	114	113.00	184
77.95	2599	88.00	24701	102.95	471	114.85	717
78.90	25781	89.20	159	103.95	4527	115.90	2757
79.90	7021	90.85	3237	104.95	1291	116.80	5774
80.90	26069	92.00	25715	105.85	3421	117.85	2977

Average of 13.777 to 13.783 min.: VL040981.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.95	4355	127.95	3263	136.90	1505	144.80	730
119.90	63	128.95	921	137.70	60	145.70	401
121.95	443	129.95	2811	138.20	75	145.95	898
122.70	147	130.70	215	138.95	450	146.50	88
123.50	137	131.00	835	139.70	170	146.85	196
123.95	428	131.90	143	139.95	299	147.85	1864
125.00	397	133.80	123	140.85	8419	148.70	435
125.70	164	134.80	698	141.80	240	148.90	160
126.00	244	135.05	970	141.95	725	149.75	621
126.80	196	135.80	182	142.90	7504	151.95	184
127.20	81	136.00	211	144.00	740	152.60	117

Average of 13.777 to 13.783 min.: VL040981.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
152.95	380	164.60	95	173.90	460139	262.80	82
153.75	457	167.50	145	174.95	36600	297.80	71
154.85	1682	167.70	123	175.90	457728		
156.70	255	168.45	437	176.90	30083		
157.05	470	168.95	304	177.85	757		
157.80	252	169.20	155	182.30	60		
158.95	871	170.30	559	208.40	120		
159.75	171	171.20	638	213.00	63		
160.85	577	171.50	469	217.50	86		
162.00	68	172.10	1317	224.90	93		
163.40	64	172.95	5344	234.40	101		