
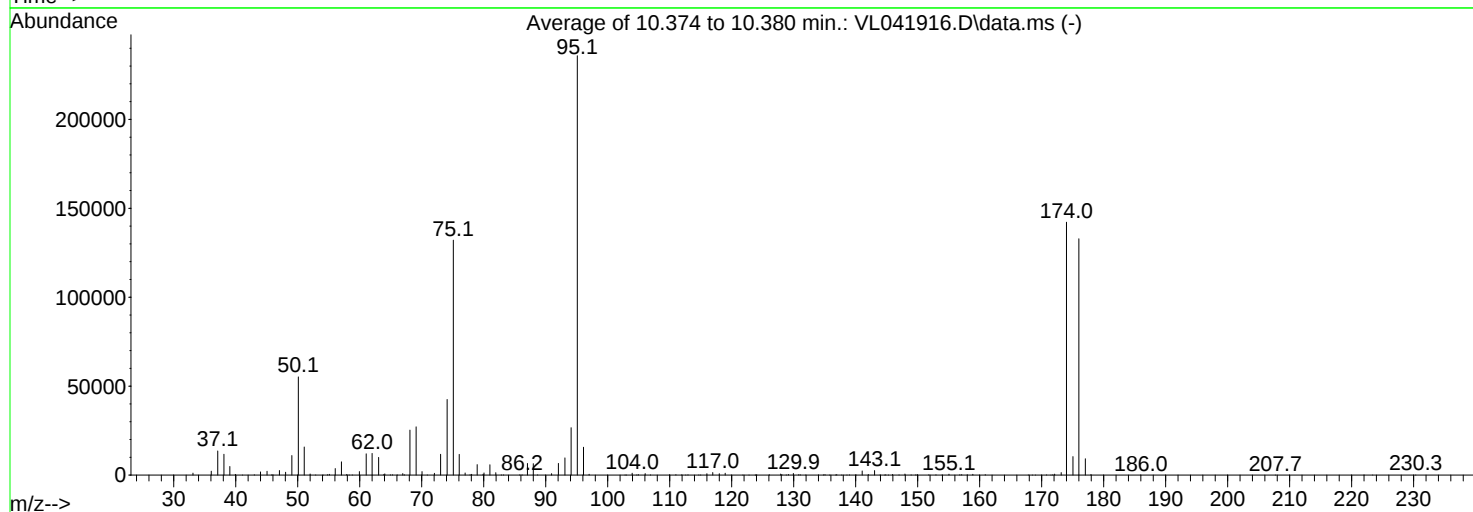


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL012025\
Data File : VL041916.D
Acq On : 20 Jan 2025 11:53
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Jan 14 23:15:42 2025

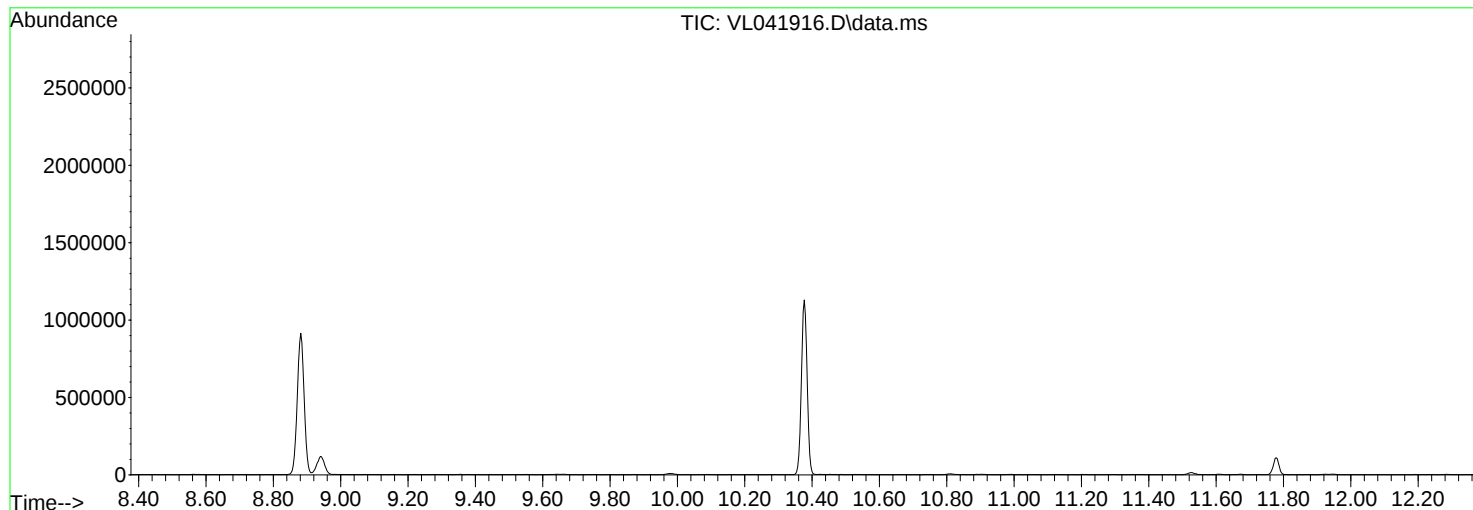

AutoFind: Scans 3178, 3179, 3180; Background Corrected with Scan 3162

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.4	55184	PASS
75	95	30	66	56.0	132096	PASS
95	95	100	100	100.0	235797	PASS
96	95	5	9	6.6	15656	PASS
173	174	0.00	2	1.0	1393	PASS
174	95	50	120	60.3	142187	PASS
175	174	4	9	7.3	10388	PASS
176	174	93	101	93.5	132891	PASS
177	176	5	9	6.9	9178	PASS

Average of 10.374 to 10.380 min.: VL041916.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1107	46.00	102	56.05	3670	64.95	134
36.05	2199	47.05	2563	57.05	7457	65.30	170
37.10	13556	48.05	1605	57.90	327	66.10	25
38.10	11733	49.05	10988	58.30	77	66.95	852
39.05	4830	50.10	55184	58.80	90	67.20	172
39.95	370	51.05	15805	59.95	1991	68.10	25293
41.10	23	52.00	636	61.05	11968	69.10	27133
43.00	179	52.90	64	62.00	12180	70.05	1989
44.00	1799	54.10	19	63.05	9929	70.90	75
45.05	2141	54.80	196	63.90	413	72.05	995
45.80	119	55.10	425	64.05	691	73.05	11680

Average of 10.374 to 10.380 min.: VL041916.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
74.10	42520	82.85	84	95.10	235797	111.00	233
75.10	132096	83.20	84	96.10	15656	111.95	109
76.05	11635	85.80	99	97.00	455	112.60	38
77.00	1199	86.20	124	102.80	65	112.95	156
77.80	191	87.05	6549	103.00	67	114.70	65
78.05	424	88.00	6433	103.95	1064	115.00	53
78.95	5884	88.70	114	104.70	80	116.00	784
79.90	503	90.95	831	104.95	234	116.95	1425
80.05	1216	92.05	6559	106.05	845	118.00	789
81.00	5795	93.10	9663	106.90	127	118.95	1062
81.95	1363	94.10	26640	110.00	172	121.80	30

Average of 10.374 to 10.380 min.: VL041916.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
122.80	30	131.05	220	140.05	144	148.95	110
123.80	38	131.95	47	141.05	2335	149.70	132
123.90	54	134.00	94	142.05	269	149.95	241
124.05	103	134.80	142	143.05	2530	151.80	130
126.10	135	135.05	268	143.95	121	152.95	170
127.90	561	135.80	28	144.70	42	153.95	93
128.10	250	136.80	117	144.85	174	155.05	514
128.80	81	136.95	276	145.30	50	156.80	190
129.15	337	137.75	41	145.95	316	157.10	262
129.95	913	138.60	24	147.00	115	158.00	129
130.80	204	139.00	106	147.95	591	158.90	443

Average of 10.374 to 10.380 min.: VL041916.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
160.90	251	176.00	132891				
167.85	55	177.05	9178				
168.50	21	177.95	278				
169.00	35	186.00	25				
170.80	120	207.70	28				
171.50	45	222.00	20				
171.80	182	223.40	28				
172.10	542	230.35	45				
173.15	1393						
174.00	142187						
175.05	10388						

Instrument :

MSVOA_L

ClientSampleId :

BFB