

Data Path : W:\HPCHEM1\MSVOA_L\DATA\VL012218\
 Data File : VL031425.D
 Acq On : 22 Jan 2018 21:14
 Operator : SY/AP
 Sample : QC011618 CAN 10319
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC011618 CAN 10319

Quant Time: Jan 23 06:05:41 2018
 Quant Method : W:\HPCHEM1\MSVOA_L\METHODS\VL012218AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Jan 22 17:52:32 2018
 QLast Update : Mon Jan 22 17:52:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.90	49	1317894	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.44	114	2876390	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.41	117	2859892	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.75	95	2312855	10.10	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.00%


Target Compounds						Qvalue
15) Acetone	4.04	43	7336	0.04	ppbv #	51
20) Methylene Chloride	4.53	84	12925	0.19	ppbv #	82
39) 1,2-Dichloropropane	7.44	63	791237	8.24	ppbv #	21
80) Naphthalene,2-methyl-	25.27	142	2610	0.04	ppbv #	31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA_L\DATA\VL012218\
Data File : VL031425.D
Acq On : 22 Jan 2018 21:14
Operator : SY/AP
Sample : QC011618 CAN 10319
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC011618 CAN 10319

Quant Time: Jan 23 06:05:41 2018
Quant Method : W:\HPCHEM1\MSVOA_L\METHODS\VL012218AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Jan 22 17:52:32 2018
QLast Update : Mon Jan 22 17:52:32 2018
Response via : Initial Calibration

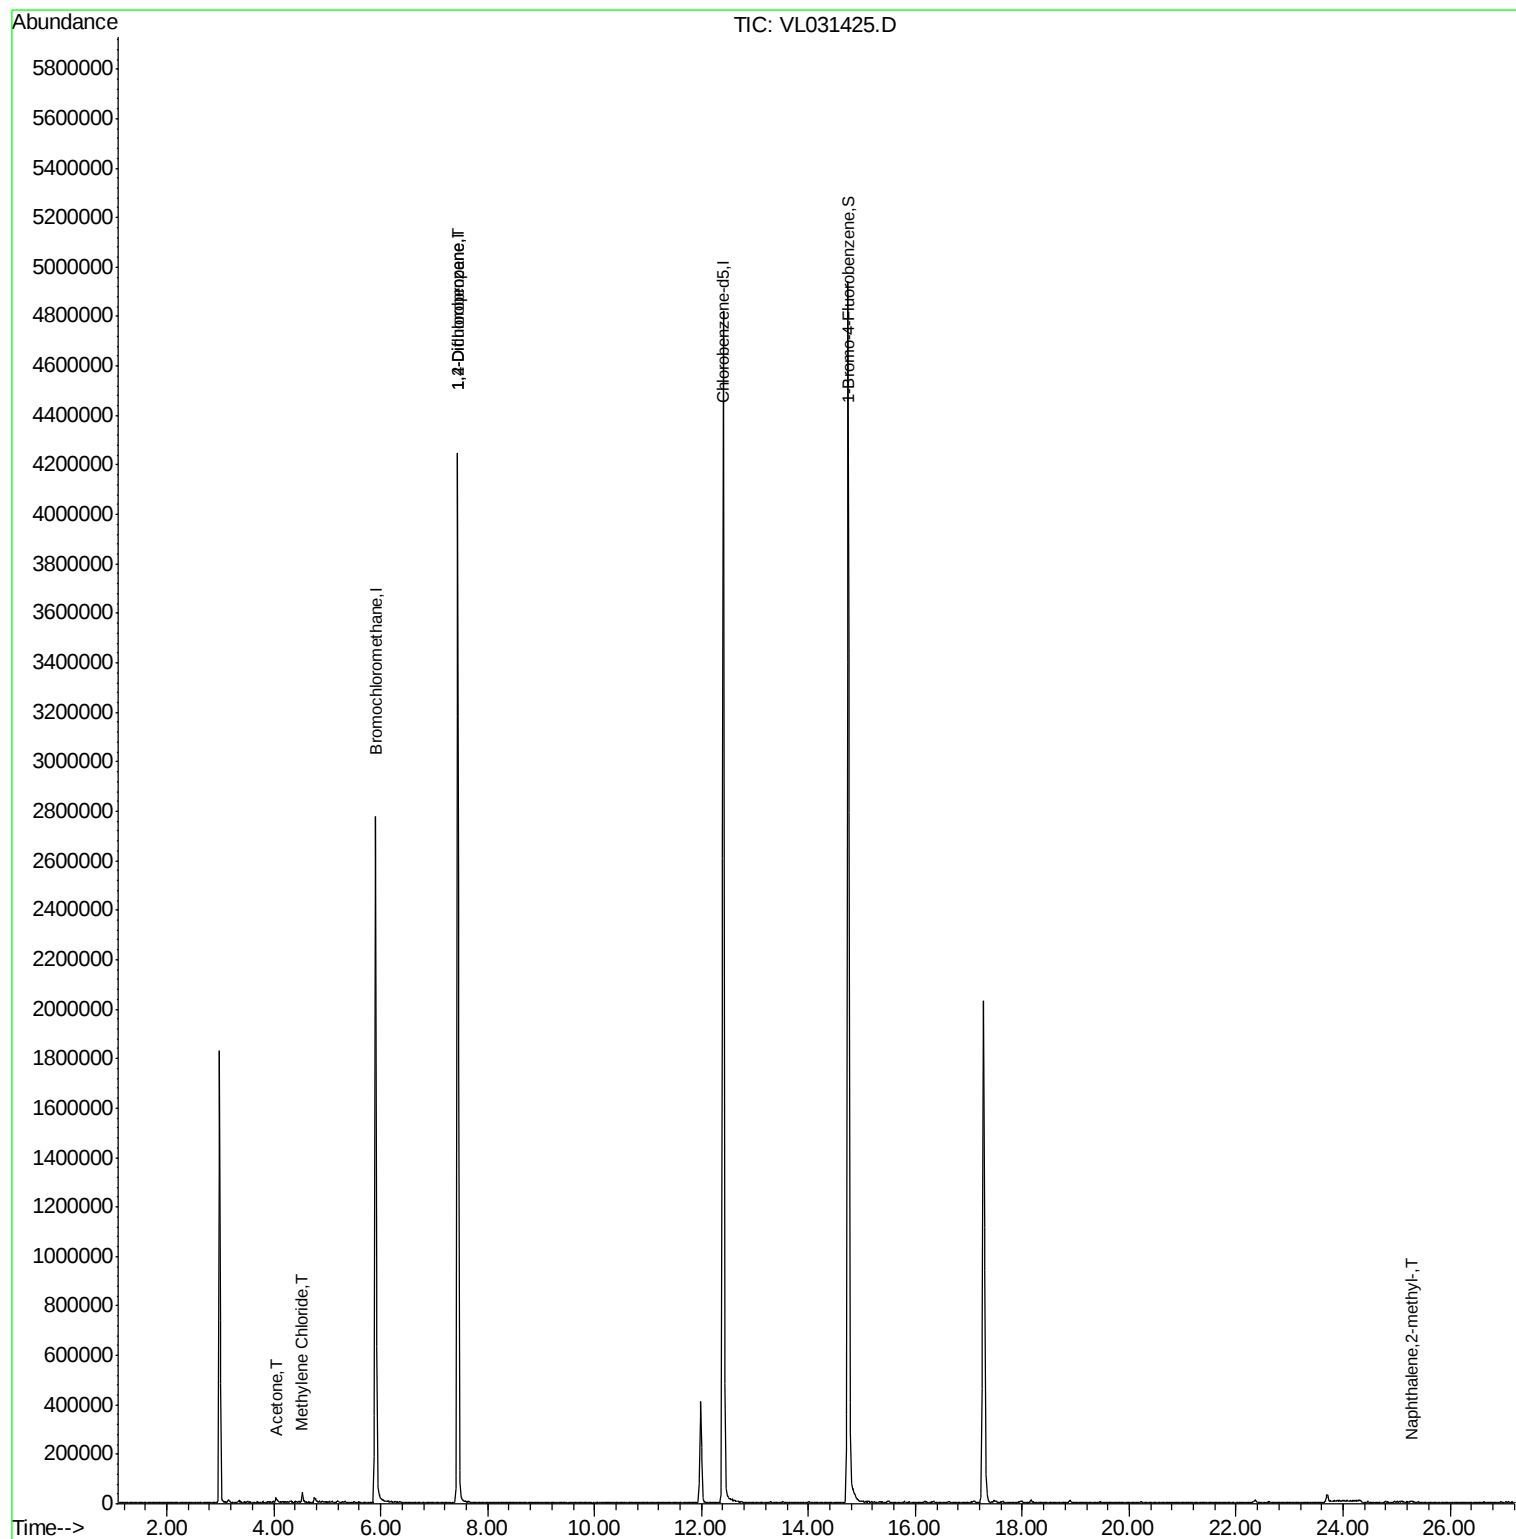

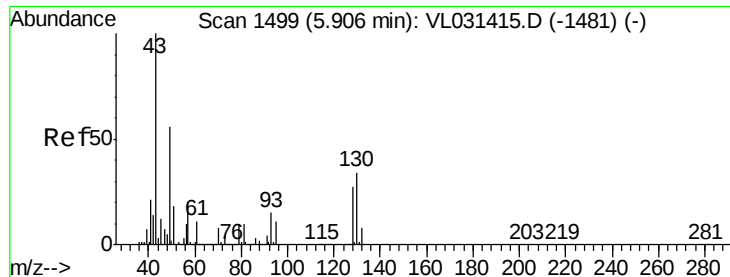

#1

Bromochloromethane

Concen: 10.00 ppbv

RT: 5.90 min Scan# 1498

Delta R.T. -0.01 min

Lab File: VL031425.D

Acq: 22 Jan 2018 21:14

Instrument :

MSVOA_L

ClientSampleId :

QC011618 CAN 10319


Tgt Ion: 49 Resp: 1317894

Ion Ratio Lower Upper

49 100

128 45.9 23.5 70.6




130 59.3 29.9 89.7

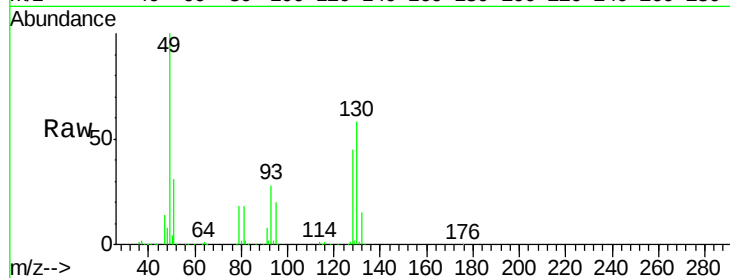

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): V

Ion 130.00 (129.70 to 130.70): V

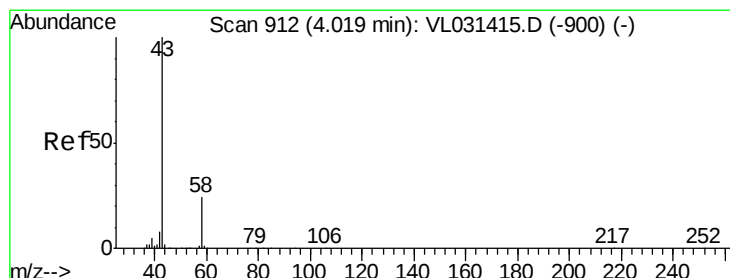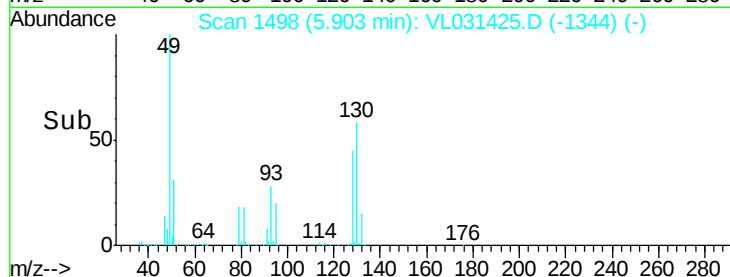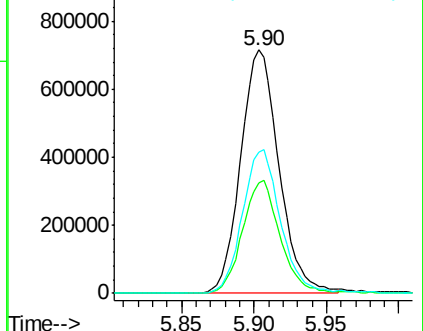

#15

Acetone

Concen: 0.04 ppbv

RT: 4.04 min Scan# 919

Delta R.T. 0.02 min

Lab File: VL031425.D


Acq: 22 Jan 2018 21:14

Tgt Ion: 43 Resp: 7336

Ion Ratio Lower Upper



43 100


58 0.0 19.4 29.2#

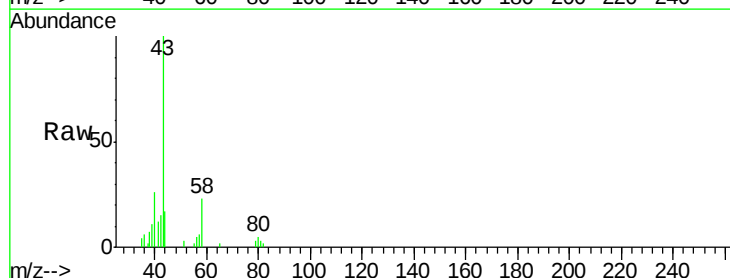

Abundance Ion 43.10 (42.80 to 43.80): VL0

Ion 58.10 (57.80 to 58.80): VL0



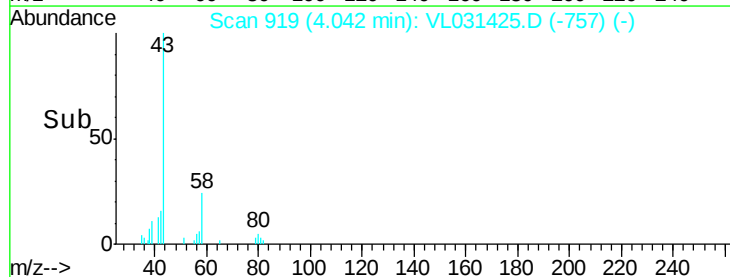
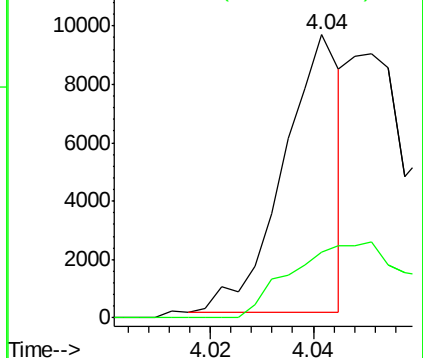


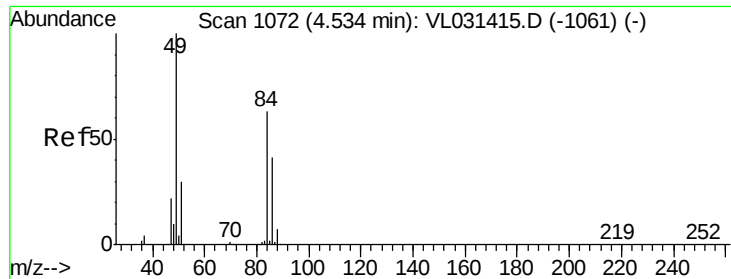

#20
Methylene Chloride
Concen: 0.19 ppbv
RT: 4.53 min Scan# 1072
Delta R.T. -0.00 min
Lab File: VL031425.D
Acq: 22 Jan 2018 21:14




Instrument :
MSVOA_L
ClientSampleId :
QC011618 CAN 10319


Tgt Ion: 84 Resp: 12925
Ion Ratio Lower Upper
84 100
49 130.2 123.4 185.0
51 34.2 35.6 53.4#
86 48.6 49.4 74.2#

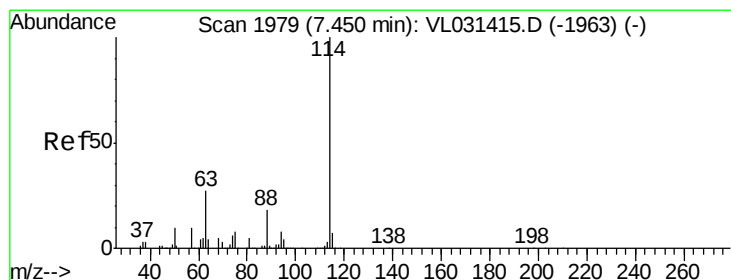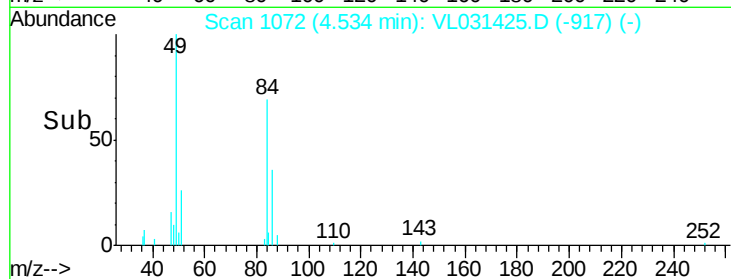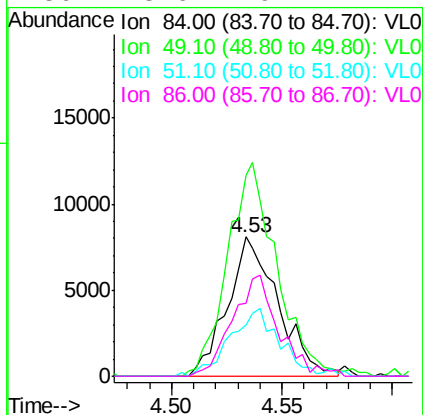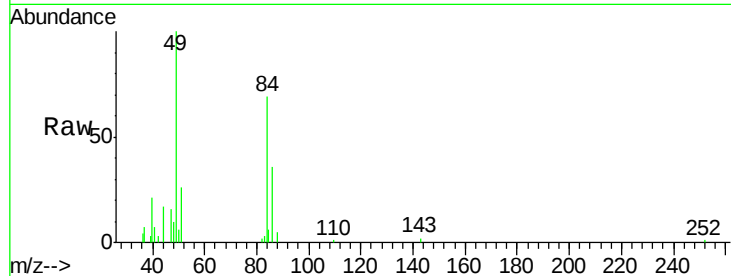

#33
1,4-Difluorobenzene
Concen: 10.00 ppbv
RT: 7.44 min Scan# 1977
Delta R.T. -0.01 min
Lab File: VL031425.D
Acq: 22 Jan 2018 21:14

Tgt Ion: 114 Resp: 2876390
Ion Ratio Lower Upper
114 100
63 27.7 22.5 33.7
88 18.2 14.6 22.0


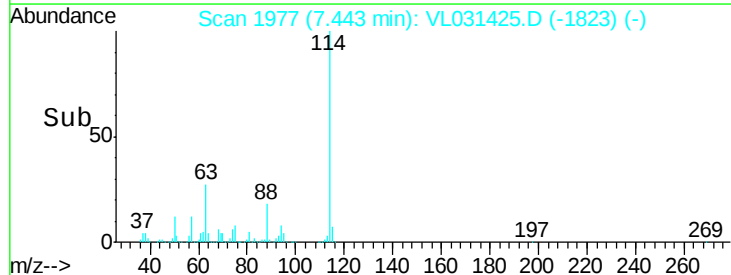
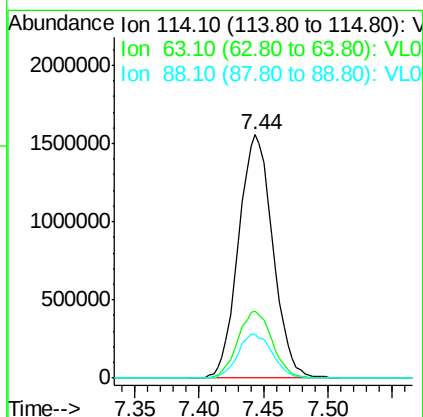
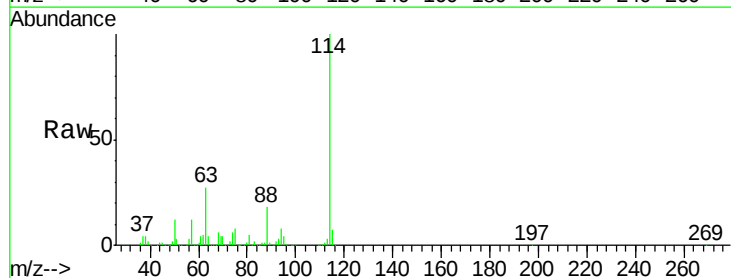


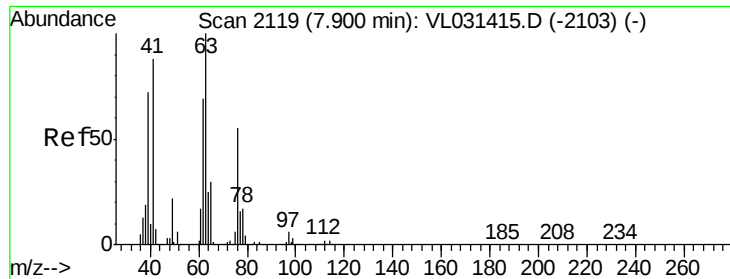

#39
 1,2-Dichloropropane
 Concen: 8.24 ppbv
 RT: 7.44 min Scan# 1977
 Delta R.T. -0.45 min
 Lab File: VL031425.D
 Acq: 22 Jan 2018 21:14




Instrument :
 MSVOA_L
 ClientSampleId :
 QC011618 CAN 10319


Tgt Ion: 63 Resp: 791237
 Ion Ratio Lower Upper
 63 100
 41 0.0 67.6 101.4#
 62 17.2 51.8 77.6#

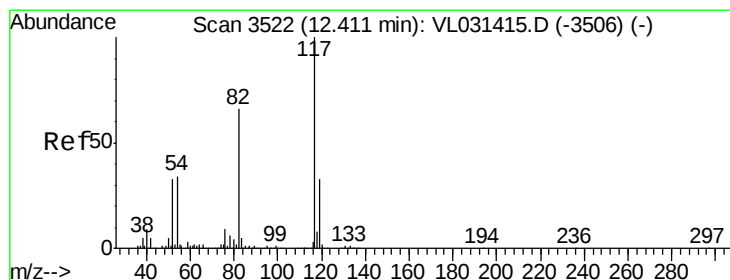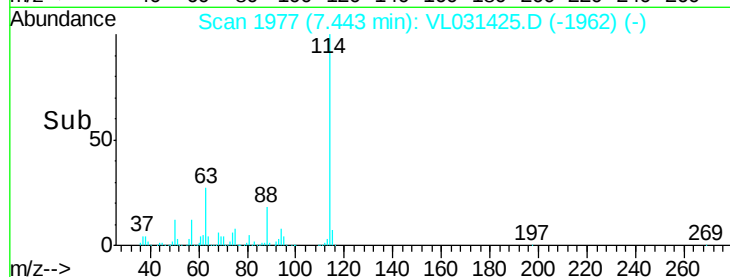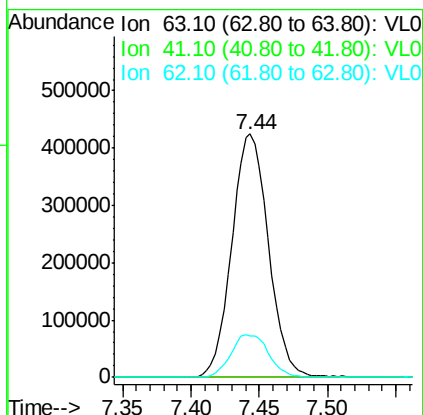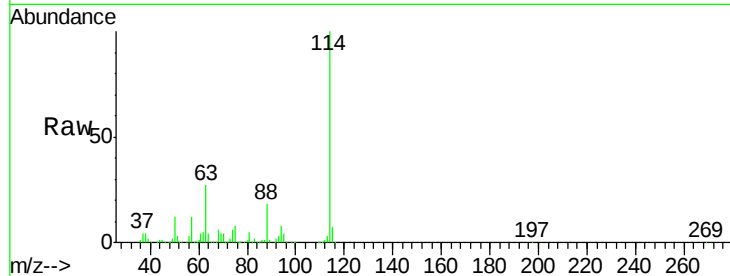

#55
 Chlorobenzene-d5
 Concen: 10.00 ppbv
 RT: 12.41 min Scan# 3521
 Delta R.T. -0.01 min
 Lab File: VL031425.D
 Acq: 22 Jan 2018 21:14

Tgt Ion: 117 Resp: 2859892
 Ion Ratio Lower Upper
 117 100
 82 67.3 51.8 77.6
 119 32.2 24.2 36.2

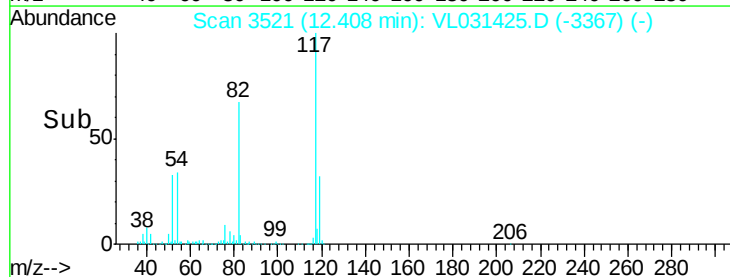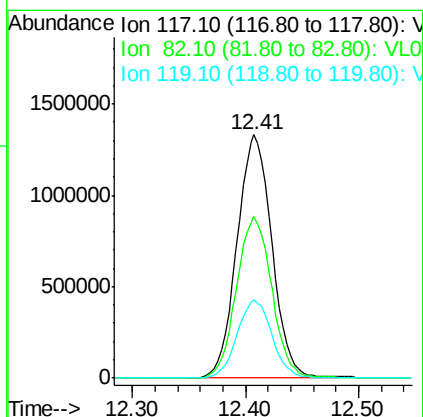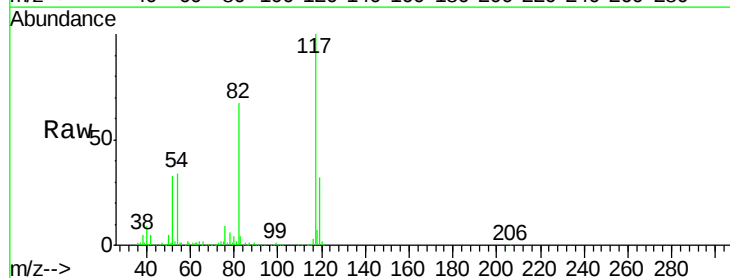

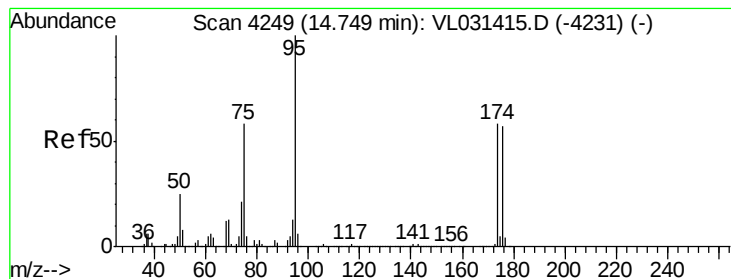

#68

1-Bromo-4-Fluorobenzene

Concen: 10.10 ppbv

RT: 14.75 min Scan# 4249

Delta R.T. 0.00 min

Lab File: VL031425.D

Acq: 22 Jan 2018 21:14

Instrument :

MSVOA_L

ClientSampleId :

QC011618 CAN 10319


Tgt Ion: 95 Resp: 2312855

Ion Ratio Lower Upper

95 100

174 61.4 48.2 72.4




175 4.4 3.6 5.4

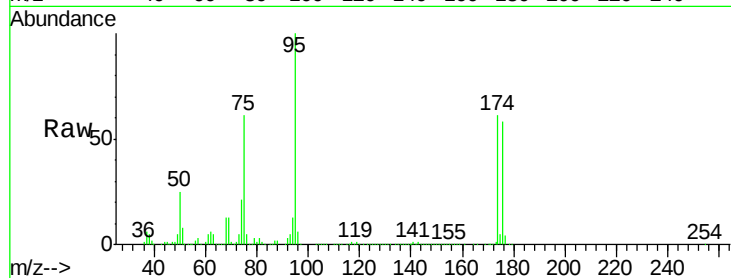

Abundance Ion 95.10 (94.80 to 95.80): VL0

Ion 174.00 (173.70 to 174.70): V

Ion 175.00 (174.70 to 175.70): V

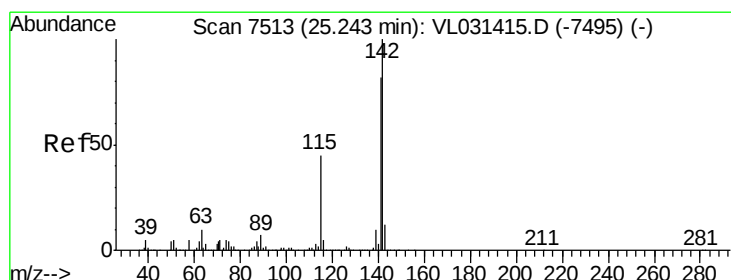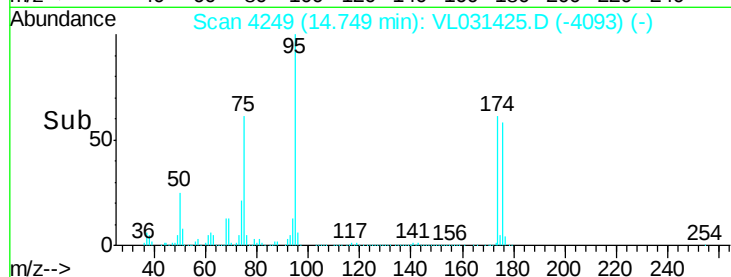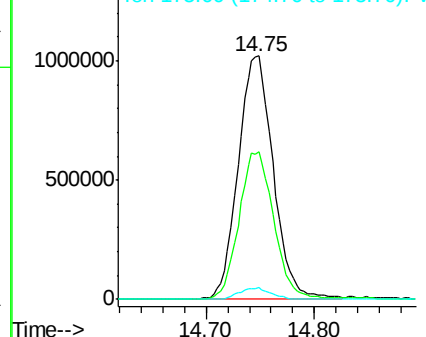

#80

Naphthalene, 2-methyl-

Concen: 0.04 ppbv

RT: 25.27 min Scan# 7522

Delta R.T. 0.03 min

Lab File: VL031425.D

Acq: 22 Jan 2018 21:14


Tgt Ion: 142 Resp: 2610

Ion Ratio Lower Upper

142 100

141 0.0 68.7 103.1#

115 30.3 36.3 54.5#

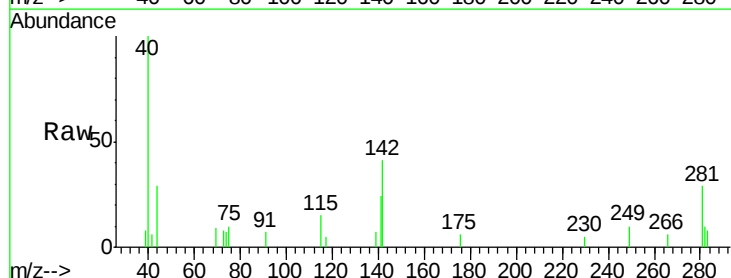

Abundance Ion 142.00 (141.70 to 142.70): V

Ion 141.00 (140.70 to 141.70): V

Ion 115.00 (114.70 to 115.70): V

