

Data Path : W:\HPCHEM1\MSVOA L\DATA\VL012218\
 Data File : VL031439.D
 Acq On : 23 Jan 2018 5:41
 Operator : SY/AP
 Sample : J1089-14
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 MDL-AIR-7

Manual Integrations
 APPROVED

MMDadoda
 1/24/2018 5:10:38 PM

Quant Time: Jan 23 07:26:34 2018
 Quant Method : W:\HPCHEM1\MSVOA L\METHODS\VL012218AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Jan 22 17:52:32 2018
 QLast Update : Mon Jan 22 17:52:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.91	49	1207298	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.45	114	2580151	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.41	117	2540078	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.75	95	2094791	10.30	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	103.00%

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
5) Vinyl Chloride	3.40	62	2482m	0.04	ppbv	
32) 1,1,1-Trichloroethane	6.77	97	7004m	0.03	ppbv	
35) Carbon Tetrachloride	7.29	117	6880m	0.03	ppbv	
38) Trichloroethene	8.13	130	3332m	0.04	ppbv	
52) Tetrachloroethene	11.55	164	2968m	0.03	ppbv	
63) 1,1,2,2-Tetrachloroethane	14.01	83	6820m	0.03	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : W:\HPCHEM1\MSVOA L\DATA\VL012218\
Data File : VL031439.D
Acq On : 23 Jan 2018 5:41
Operator : SY/AP
Sample : J1089-14
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
MDL-AIR-7

Manual Integrations
APPROVED

MMDadoda
1/24/2018 5:10:38 PM

Quant Time: Jan 23 07:26:34 2018
Quant Method : W:\HPCHEM1\MSVOA L\METHODS\VL012218AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Jan
QLast Update : Mon Jan 22 17:52:32 2018
Response via : Initial Calibration

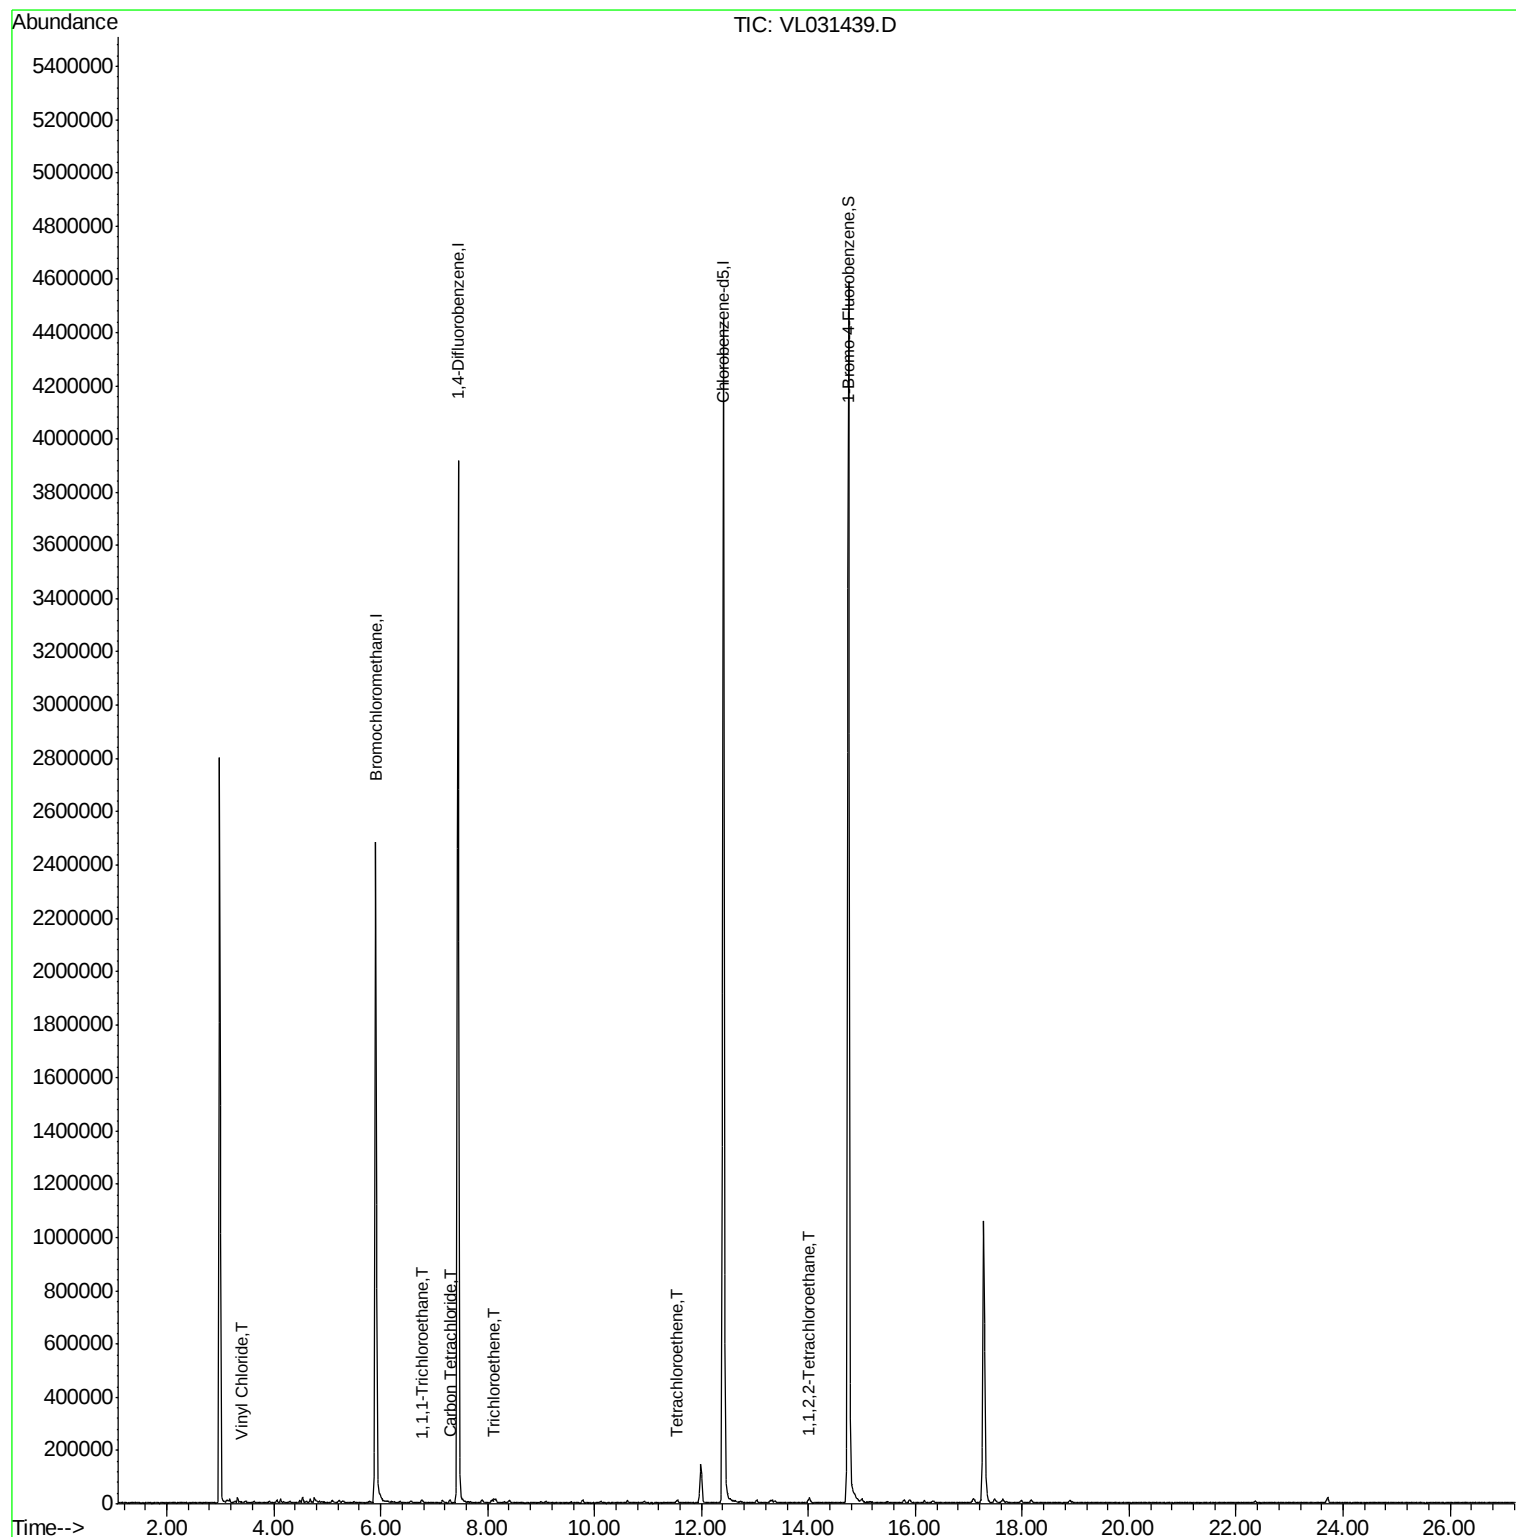

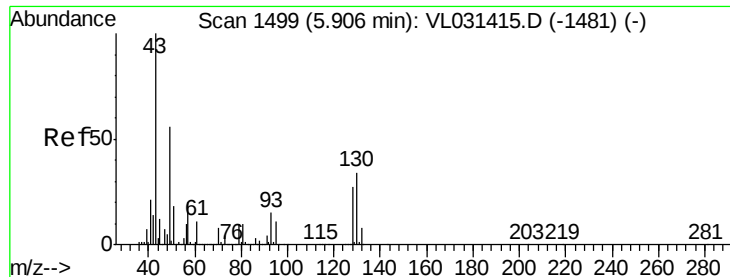

#1

Bromochloromethane

Concen: 10.00 ppbv

RT: 5.91 min Scan# 1499

Delta R.T. -0.00 min

Lab File: VL031439.D

Acq: 23 Jan 2018 5:41

Instrument :

MSVOA_L

ClientSampleId :

MDL-AIR-7

Tot Ion: 49 Resp: 1207298

Ion Ratio Lower Upper

49 100


128 44.6 23.5 70.6

130 57.0 29.9 89.7

Manual Integrations
APPROVED

MMDadoda

1/24/2018 5:10:38 PM

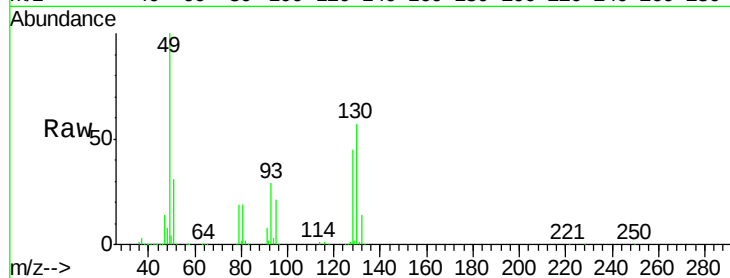

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

5.91

800000

600000



400000

200000

0

5.80 5.85 5.90 5.95 6.00

Time-->

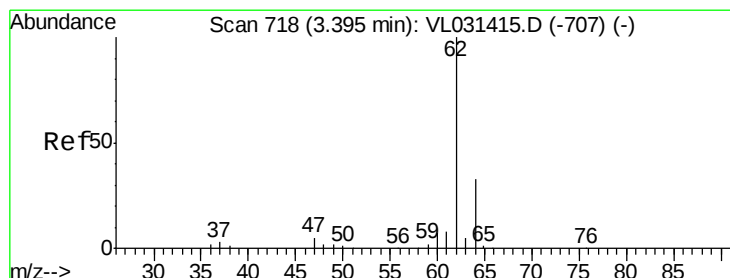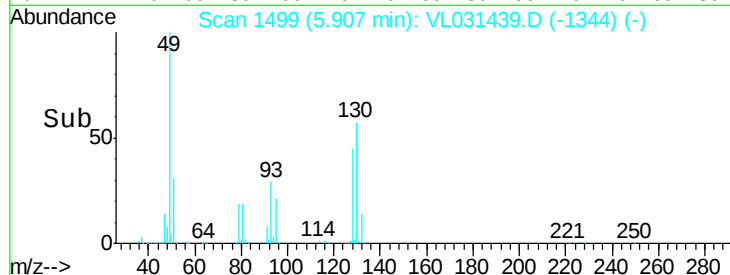

#5

Vinyl Chloride

Concen: 0.04 ppbv m

RT: 3.40 min Scan# 719

Delta R.T. 0.00 min

Lab File: VL031439.D


Acq: 23 Jan 2018 5:41

Tgt Ion: 62 Resp: 2482

Ion Ratio Lower Upper

62 100

64 0.0 25.4 38.0#

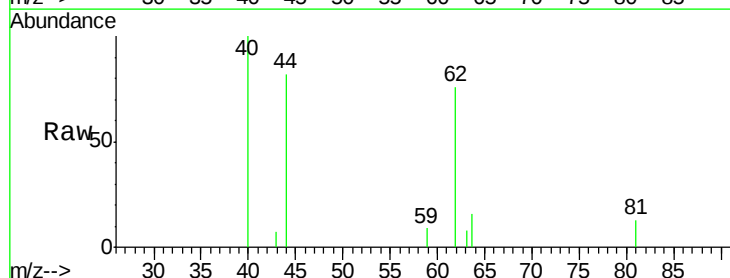

Abundance Ion 62.10 (61.80 to 62.80): VL0

Ion 64.10 (63.80 to 64.80): VL0

3.40

2000

1500


1000


500

0

3.35 3.40

Time-->

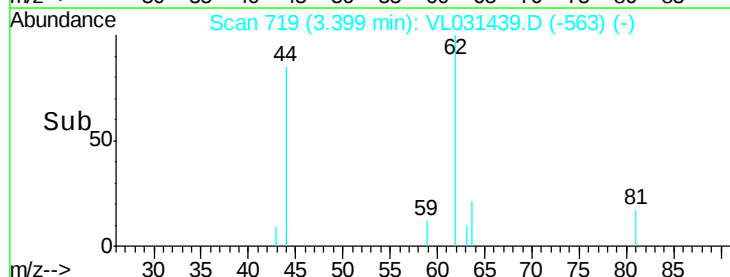

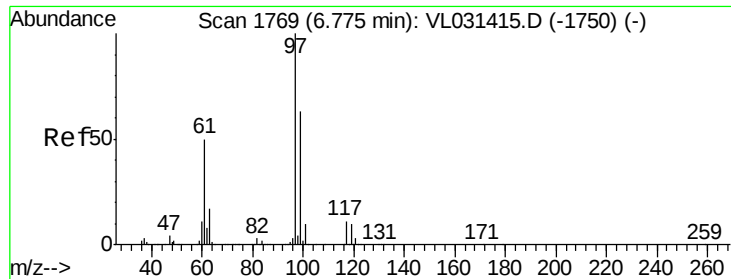





#32
 1,1,1-Trichloroethane
 Concen: 0.03 ppbv m
 RT: 6.77 min Scan# 1769
 Delta R.T. 0.00 min
 Lab File: VL031439.D
 Acq: 23 Jan 2018 5:41

Instrument :
 MSVOA_L
 ClientSampleId :
 MDL-AIR-7

Tot Ion	Ratio	Lower	Upper
97	100		
99	62.5	51.9	77.9
61	54.4	40.6	61.0




Manual Integrations
 APPROVED


MMDadoda
 1/24/2018 5:10:38 PM

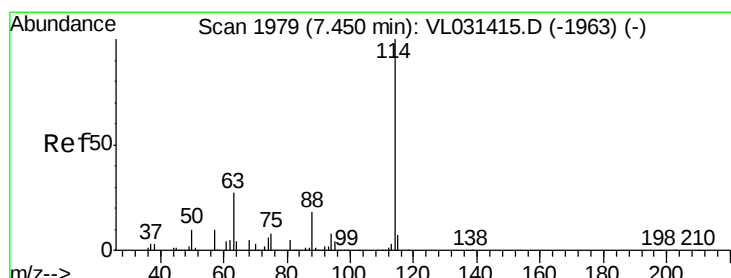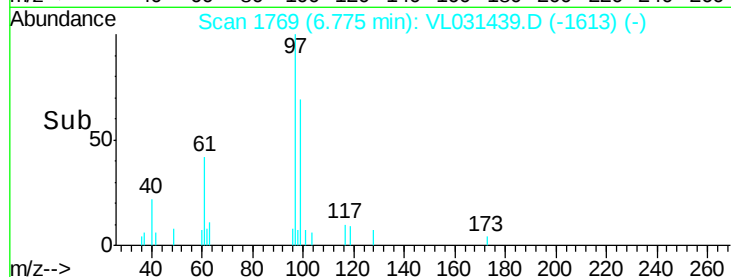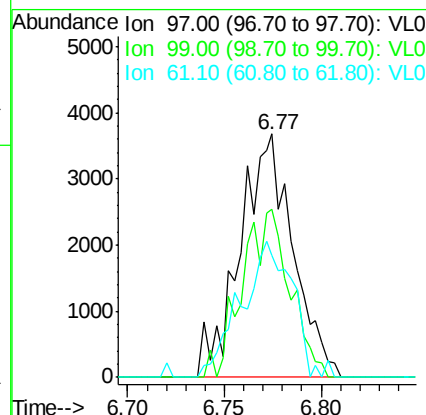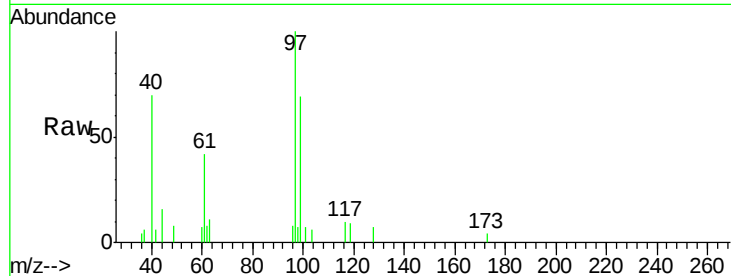

#33
 1,4-Difluorobenzene
 Concen: 10.00 ppbv
 RT: 7.45 min Scan# 1978
 Delta R.T. -0.00 min
 Lab File: VL031439.D
 Acq: 23 Jan 2018 5:41

Tgt Ion	Ratio	Lower	Upper
114	100		
63	28.6	22.5	33.7
88	18.5	14.6	22.0

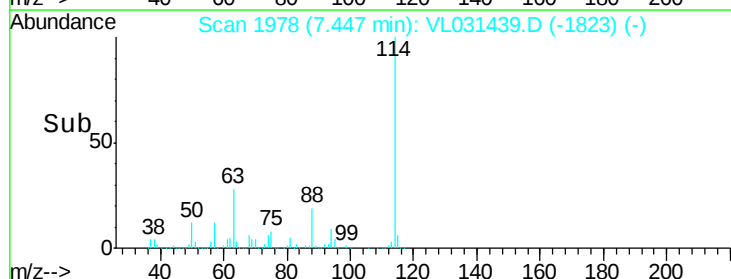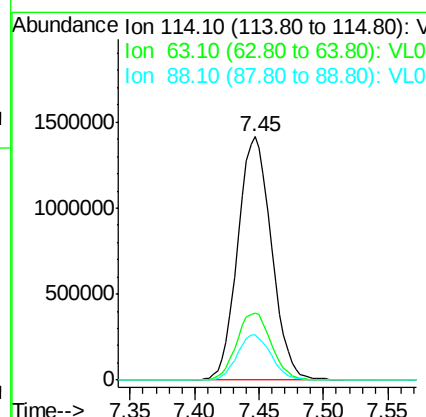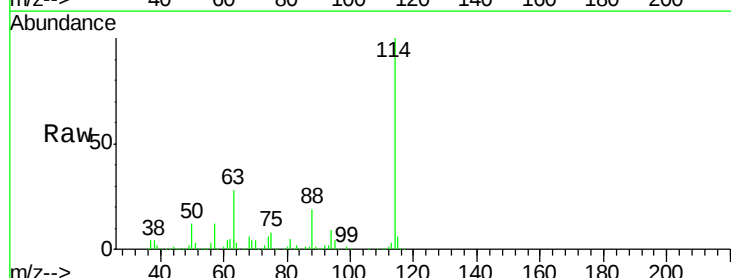

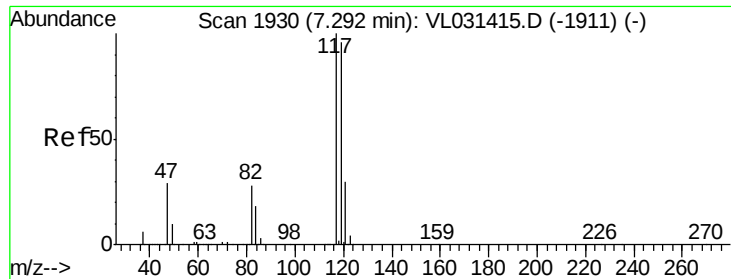





#35
Carbon Tetrachloride
Concen: 0.03 ppbv m
RT: 7.29 min Scan# 1928
Delta R.T. -0.01 min
Lab File: VL031439.D
Acq: 23 Jan 2018 5:41

Instrument :
MSVOA_L
ClientSampled :
MDL-AIR-7

Tot Ion	Ratio	Lower	Upper
117	100		
119	89.4	74.2	111.4
121	18.5	24.2	36.4




Manual Integrations
APPROVED


MMDadoda
1/24/2018 5:10:38 PM

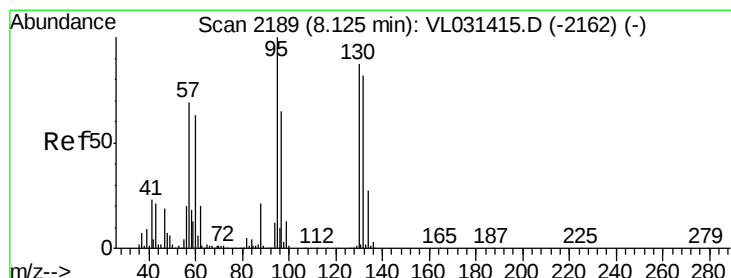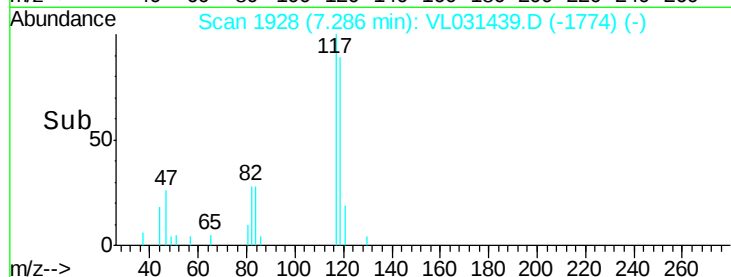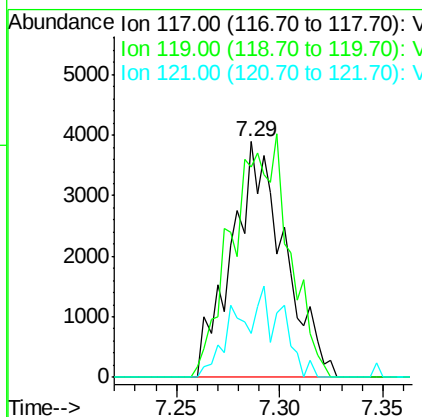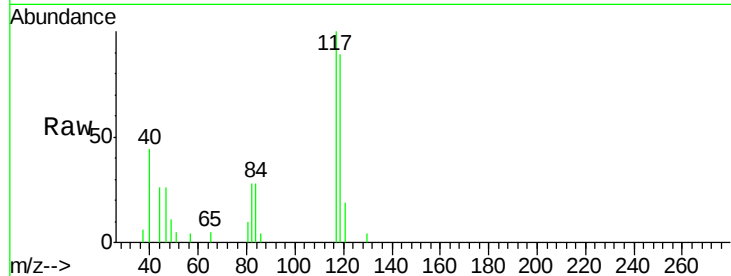

#38
Trichloroethene
Concen: 0.04 ppbv m
RT: 8.13 min Scan# 2189
Delta R.T. 0.00 min
Lab File: VL031439.D
Acq: 23 Jan 2018 5:41

Tgt Ion	Ratio	Lower	Upper
130	100		
95	52.4	92.9	139.3
132	50.5	74.9	112.3
97	42.2	60.2	90.4

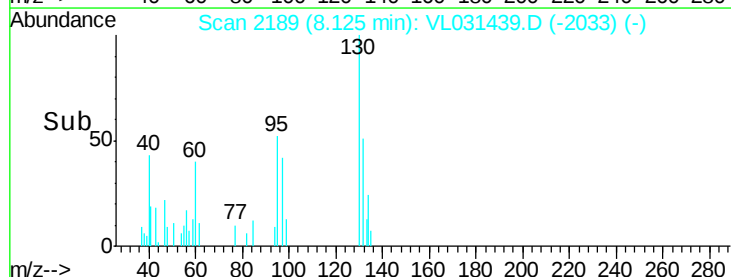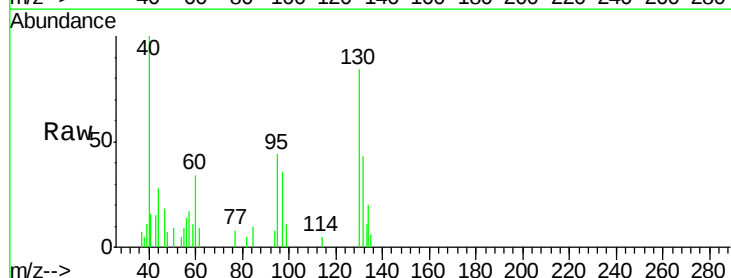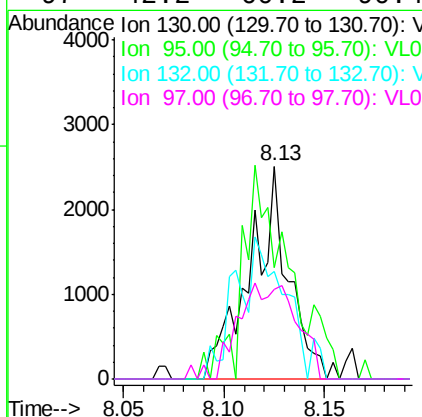

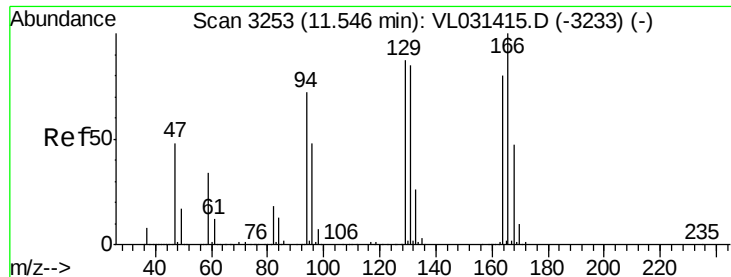





#52
Tetrachloroethene
Concen: 0.03 ppbv m
RT: 11.55 min Scan# 3253
Delta R.T. 0.00 min
Lab File: VL031439.D
Acq: 23 Jan 2018 5:41

Instrument :
MSVOA_L
ClientSampleId :
MDL-AIR-7

Tot Ion	Ratio	Lower	Upper
164	100		
166	71.4	100.2	150.2#
129	71.7	91.4	137.0#
131	51.8	87.4	131.0#




Manual Integrations
APPROVED


MMDadoda
1/24/2018 5:10:38 PM

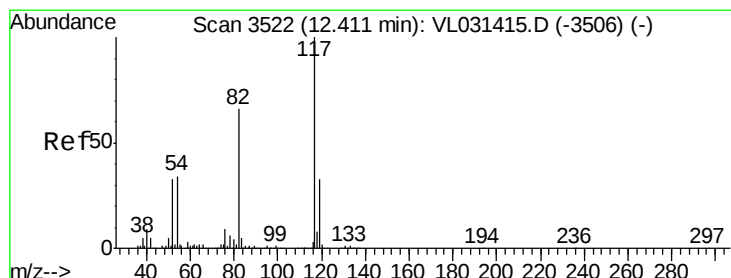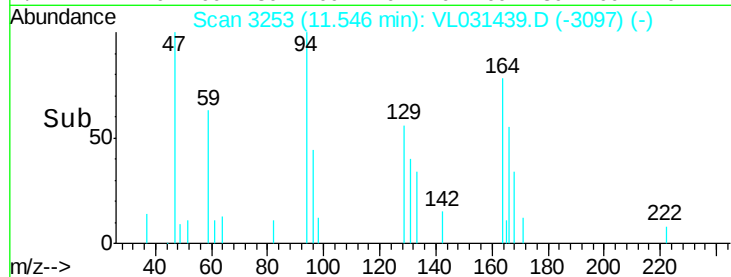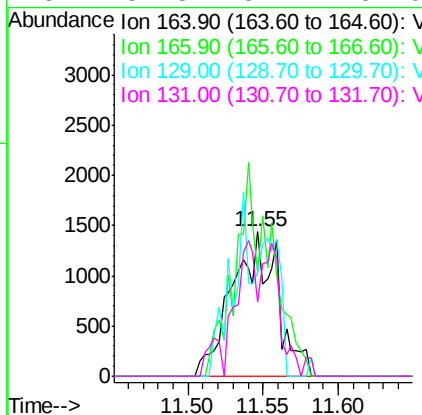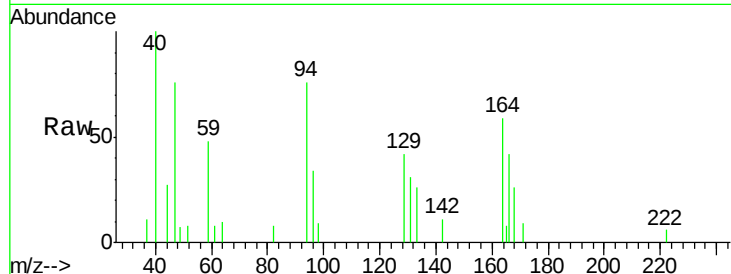

#55
Chlorobenzene-d5
Concen: 10.00 ppbv
RT: 12.41 min Scan# 3521
Delta R.T. -0.01 min
Lab File: VL031439.D
Acq: 23 Jan 2018 5:41

Tgt Ion	Ratio	Lower	Upper
117	100		
82	69.5	51.8	77.6
119	32.8	24.2	36.2

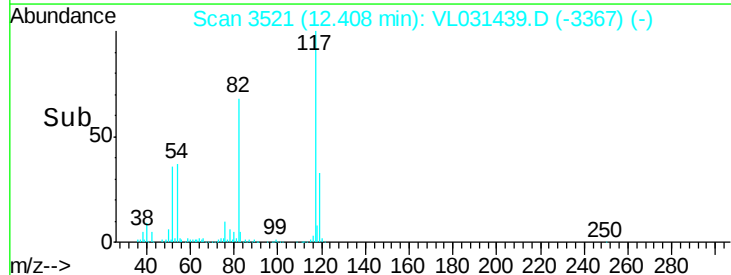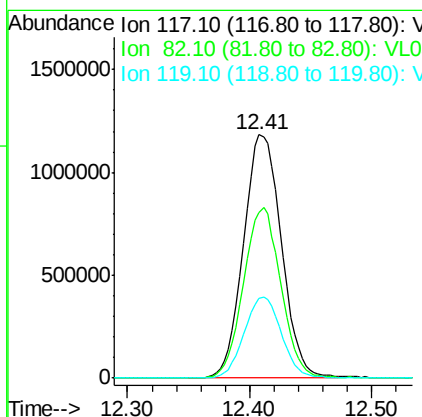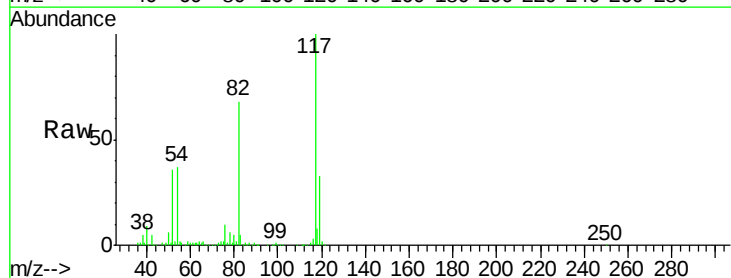

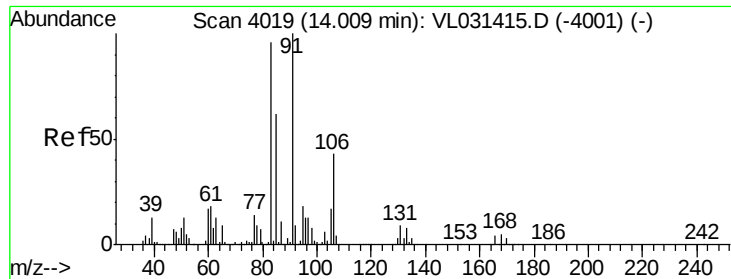





#63
 1,1,2,2-Tetrachloroethane
 Concen: 0.03 ppbv m
 RT: 14.01 min Scan# 4018
 Delta R.T. -0.00 min
 Lab File: VL031439.D
 Acq: 23 Jan 2018 5:41

Instrument :
 MSVOA_L
 ClientSampleId :
 MDL-AIR-7

Tot Ion	Ratio	Lower	Upper
83	100		
131	0.0	4.8	14.3#
85	0.0	32.4	97.0#

Manual Integrations
 APPROVED

MMDadoda
 1/24/2018 5:10:38 PM

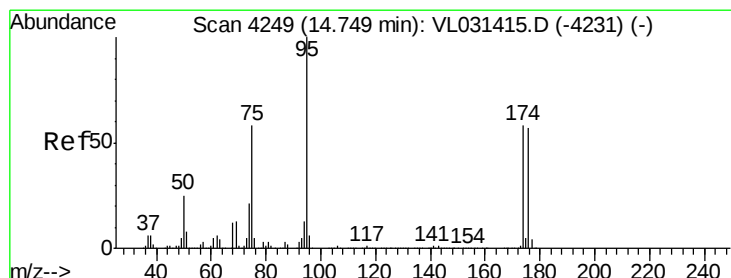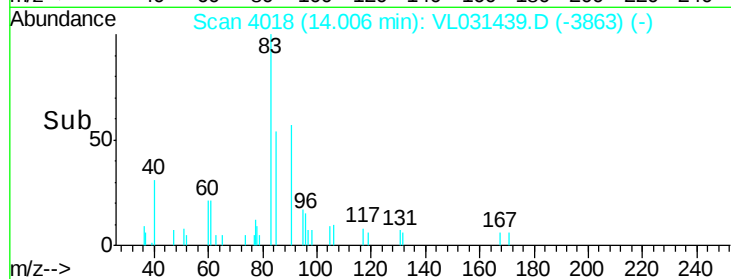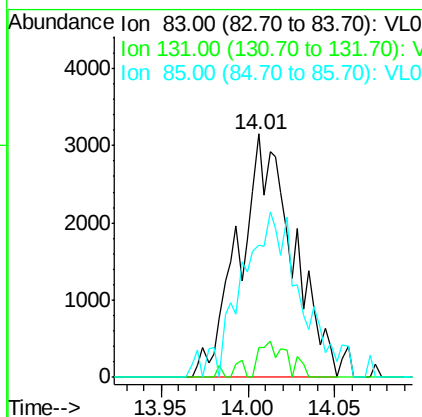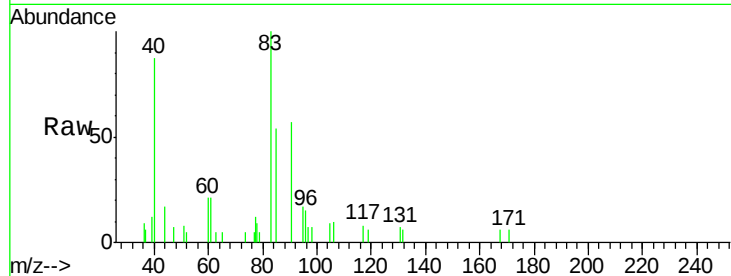

#68
 1-Bromo-4-Fluorobenzene
 Concen: 10.30 ppbv
 RT: 14.75 min Scan# 4249
 Delta R.T. 0.00 min
 Lab File: VL031439.D
 Acq: 23 Jan 2018 5:41

Tgt Ion	Ratio	Lower	Upper
95	100		
174	60.4	48.2	72.4
175	4.4	3.6	5.4

