


Data Path : W:\HPCHEM1\MSVOA L\DATA\VL012218\
 Data File : VL031414.D
 Acq On : 22 Jan 2018 12:35
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL012218AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Jan 22 17:52:32 2018
 Last Update : Mon Jan 22 17:52:32 2018

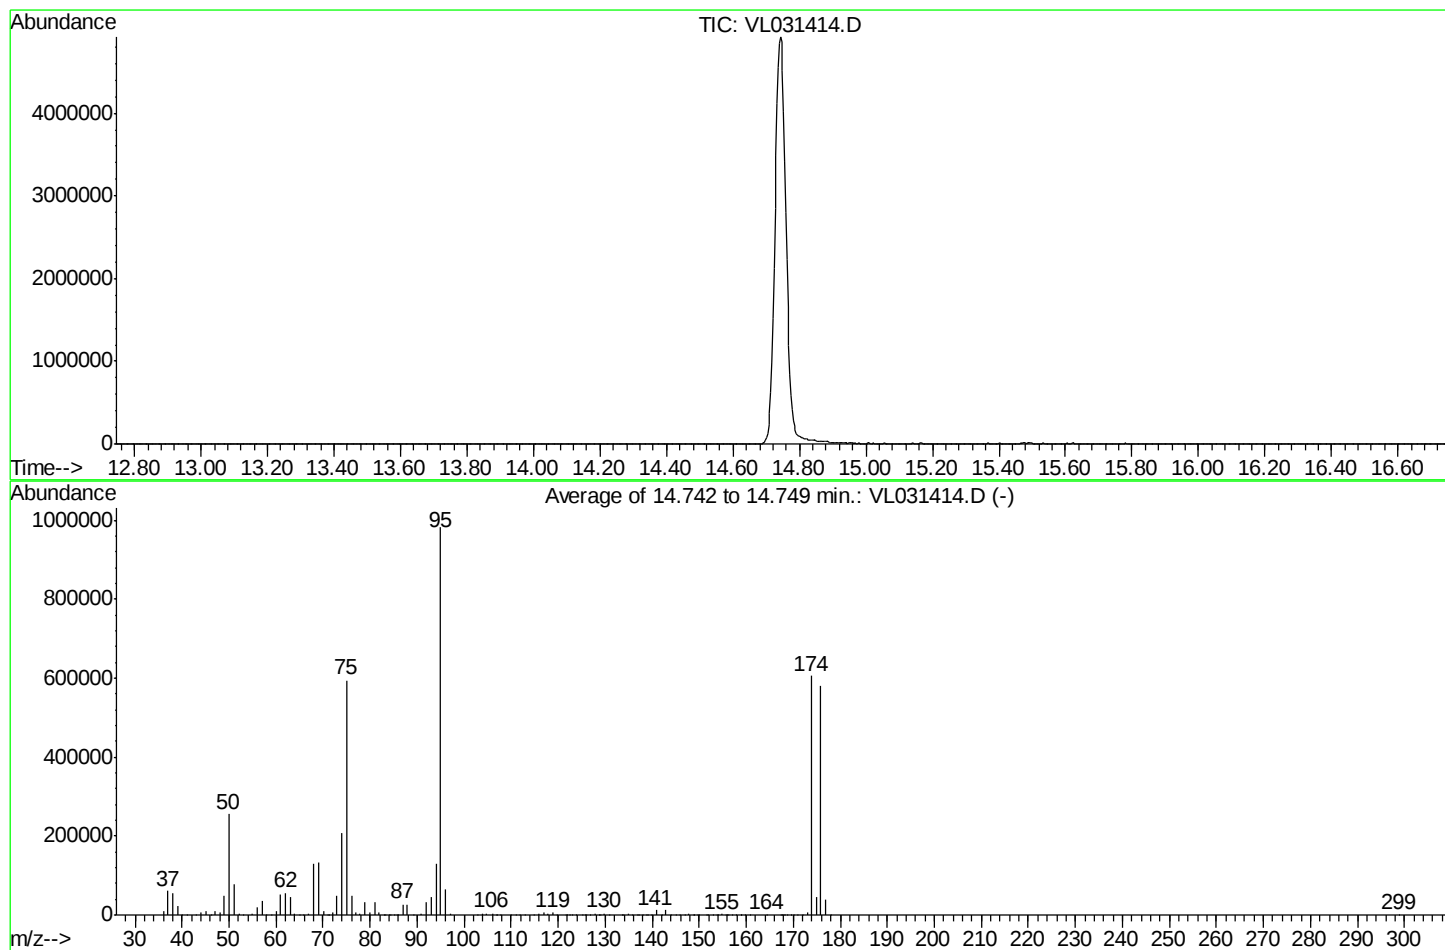

AutoFind: Scans 4247, 4248, 4249; Background Corrected with Scan 4221

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.0	255701	PASS
75	95	30	66	60.6	595157	PASS
95	95	100	100	100.0	982634	PASS
96	95	5	9	6.5	63602	PASS
173	174	0.00	2	1.1	6666	PASS
174	95	50	120	61.7	606528	PASS
175	174	4	9	7.3	44445	PASS
176	174	93	101	95.6	579968	PASS
177	176	5	9	6.6	38221	PASS