


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL012324\
Data File : VL040988.D
Acq On : 23 Jan 2024 8:27
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL012324AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Jan 24 00:50:15 2024

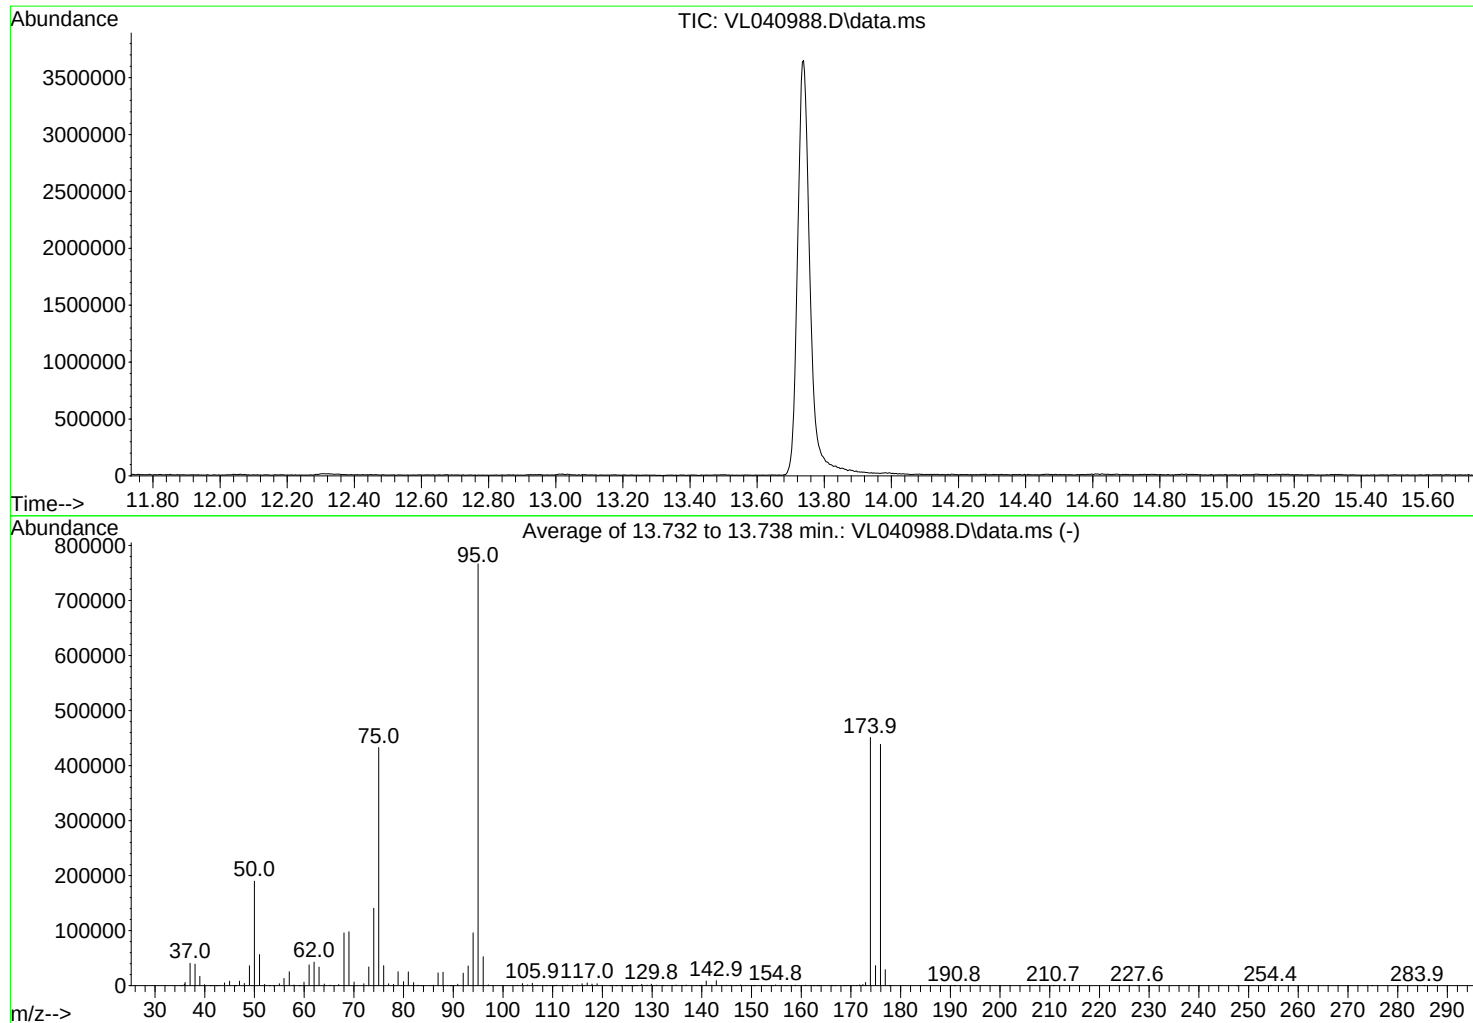

AutoFind: Scans 3461, 3462, 3463; Background Corrected with Scan 3429

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.8	189824	PASS
75	95	30	66	56.5	432896	PASS
95	95	100	100	100.0	766741	PASS
96	95	5	9	6.9	52637	PASS
173	174	0.00	2	1.3	5796	PASS
174	95	50	120	58.8	451136	PASS
175	174	4	9	8.1	36453	PASS
176	174	93	101	97.2	438549	PASS
177	176	5	9	6.6	28979	PASS

Average of 13.732 to 13.738 min.: VL040988.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.20	63	43.95	4898	53.80	95	65.20	93
35.90	2893	45.00	8120	55.00	3384	66.95	199
36.05	5732	46.00	588	55.95	13211	68.00	9611
37.05	40853	46.20	135	57.00	25245	69.00	9811
38.05	39387	47.00	8164	57.95	1128	70.05	6799
39.00	16975	47.95	4251	59.00	61	70.80	169
39.95	1822	49.00	36051	59.95	6429	72.00	3506
41.10	82	50.00	189824	61.00	37899	73.00	34030
41.60	162	51.00	56309	62.00	42824	74.00	140642
42.40	56	52.05	2277	63.00	33744	75.00	432896
43.00	601	53.00	62	64.05	2850	76.00	36339

Average of 13.732 to 13.738 min.: VL040988.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.00	3642	86.95	23160	97.05	1440	110.70	970
78.00	2242	87.95	24352	102.85	482	111.80	198
78.90	25437	88.80	292	103.90	3665	112.05	402
80.00	7252	89.45	132	104.95	1373	112.60	217
80.95	25080	90.00	100	105.90	4296	113.00	785
82.00	5640	90.90	2624	106.90	652	114.95	1191
82.75	466	92.00	22763	108.00	301	115.90	3385
83.05	625	93.00	35912	108.70	96	116.95	5069
83.60	60	94.00	95984	109.55	185	117.90	2991
85.30	223	95.00	766741	109.90	316	118.95	3444
86.00	995	96.00	52637	110.20	131	119.85	371

Average of 13.732 to 13.738 min.: VL040988.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
121.60	51	127.90	2321	139.60	63	147.80	1215
122.75	141	128.75	621	139.95	822	148.85	750
123.60	81	129.05	897	140.90	8459	149.90	719
123.95	472	129.85	2783	141.70	557	150.50	88
124.60	90	130.90	1029	142.00	914	152.10	286
124.80	171	132.10	103	142.90	8999	152.60	160
125.10	64	134.05	338	143.85	682	152.95	349
125.70	123	134.85	1062	144.90	777	153.85	245
126.20	96	135.95	196	145.70	493	154.20	69
126.70	162	136.85	1185	145.90	566	154.85	1508
126.90	57	138.95	306	146.90	648	155.70	194

Average of 13.732 to 13.738 min.: VL040988.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.75	433	166.80	113	173.90	451136	254.40	71
156.90	367	168.60	105	174.95	36453	274.80	98
157.10	164	169.10	243	175.95	438549	283.95	180
157.85	211	169.40	247	176.90	28979	285.30	56
158.85	776	169.75	326	177.70	69		
160.90	885	170.20	302	178.00	577		
161.90	90	170.60	359	190.00	70		
162.50	54	171.15	737	190.80	77		
163.20	72	171.75	1387	210.70	59		
163.55	136	172.40	2095	227.60	62		
166.10	109	172.95	5796	247.60	65		