

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL012422\
 Data File : VL038268.D
 Acq On : 24 Jan 2022 20:29
 Operator : SY/AP
 Sample : N1211-01
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA L
 ClientSampleId :
 SVE-INFLUENT

Manual Integrations
 APPROVED

Quant Time: Jan 25 14:36:09 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL012422A

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument:

QLast Update : Mon Jan 24 14:12:48 2022

Response via : Initial Calibration

Reviewed By : Semsettin Yesilyurt 01/26/2022
 Supervised By : Mahesh Dadoda 01/26/2022

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.68	49	799401	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.19	114	1984987	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.09	117	1686561	10.00	ppbv	0.00


System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.42	95	1353318	10.57	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	105.70%

Target Compounds

						Ovalue
2) Dichlorodifluoromethane	3.06	85	66519	0.391	ppbv	95
3) Chlorodifluoromethane	3.00	51	31135m	0.196	ppbv	
4) Chloromethane	3.16	50	10538m	0.192	ppbv	
10) Heptane	8.13	43	75972m	0.570	ppbv	
11) Trichlorofluoromethane	3.96	101	37016m	0.279	ppbv	
13) Ethanol	3.62	45	4435776	797.603	ppbv	98
15) Acetone	3.86	43	1137857	16.147	ppbv	98
17) tert-Butyl alcohol	4.31	59	23151m	0.299	ppbv	
19) Isopropyl Alcohol	3.99	45	492315	11.168	ppbv	100
20) Methylene Chloride	4.36	84	19998	0.488	ppbv	97
25) Ethyl Acetate	5.68	43	677240	3.432	ppbv #	92
29) Chloroform	5.76	83	26748	0.179	ppbv	96
30) Cyclohexane	7.15	84	16631m	0.208	ppbv	
31) cis-1,2-Dichloroethene	5.56	61	100621	1.257	ppbv	93
32) 1,1,1-Trichloroethane	6.52	97	22539m	0.151	ppbv	
34) 2-Butanone	5.25	43	661271	10.187	ppbv	98
35) Carbon Tetrachloride	7.03	117	15452	0.111	ppbv #	78
36) Benzene	6.91	78	99154	0.565	ppbv	96
38) Trichloroethene	7.84	130	58375m	0.893	ppbv	
41) Tetrahydrofuran	6.06	42	875130	20.055	ppbv	99
44) 2,2,4-Trimethylpentane	7.88	57	125352	0.405	ppbv #	82
50) 4-Methyl-2-Pentanone	8.75	43	190285	1.643	ppbv	100
52) Tetrachloroethene	11.23	164	104004	1.719	ppbv	94
53) Toluene	9.81	91	4781536	24.604	ppbv	96
58) Ethyl Benzene	12.72	91	209117	0.844	ppbv	90
59) m/p-Xylene	12.97	91	649808	3.073	ppbv	97
60) o-Xylene	13.70	91	275398	1.400	ppbv	98
64) n-propylbenzene	15.56	120	16691m	0.265	ppbv	
70) n-Butylbenzene	18.56	91	38301m	0.170	ppbv	
72) 4-Ethyltoluene	15.85	105	105349m	0.512	ppbv	
73) 1,3,5-Trimethylbenzene	16.00	105	84335m	0.456	ppbv	
74) 1,2,4-Trimethylbenzene	16.77	105	361141m	1.853	ppbv	
79) Naphthalene	22.20	128	53853m	0.591	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

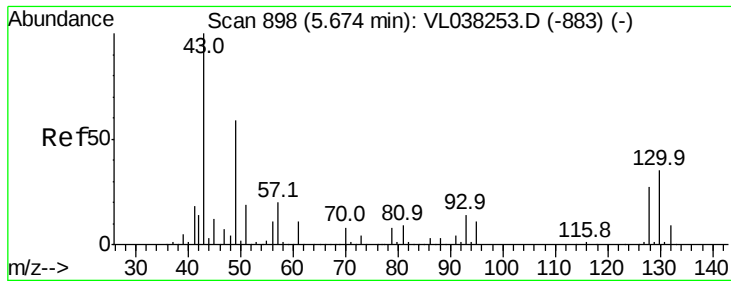

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.68 Instrument: MSVOA_1

Delta R.T. ClientSampleId:

Lab File: SVE-INFLUENT

Acq: 24 Jan 2022 20:29

Tot Ion:

Ion Ratio

49 100

128 46.


130 58.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 01/26/2022




Supervised By :Mahesh Dadoda 01/26/2022



Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

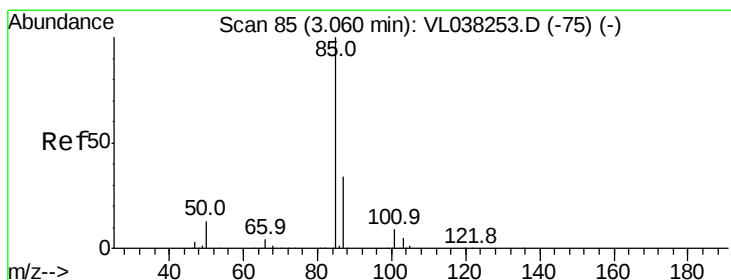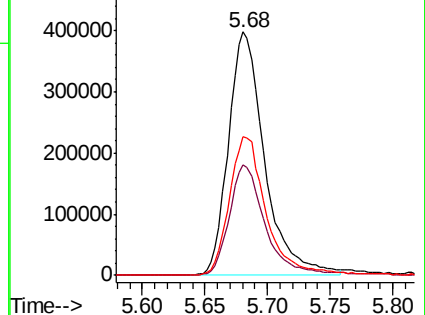

#2

Dichlorodifluoromethane

Concen: 0.391 ppbv

RT: 3.06 min Scan# 84

Delta R.T. -0.00 min

Lab File: VL038268.D


Acq: 24 Jan 2022 20:29

Tgt Ion: 85 Resp: 66519

Ion Ratio Lower Upper



85 100


87 30.7 27.0 40.6



Abundance Ion 85.00 (84.70 to 85.70): VL0

Ion 87.00 (86.70 to 87.70): VL0

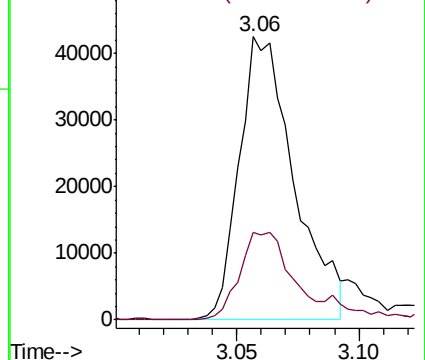

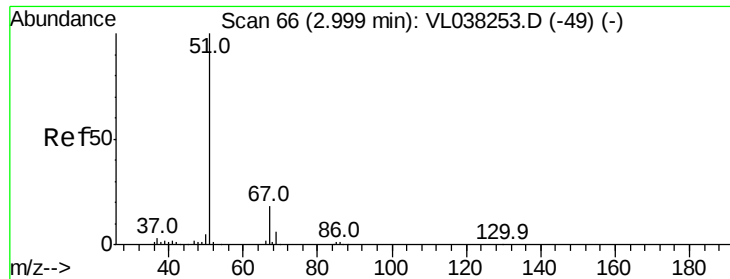

#3

Chlorodifluoromethane

Concen: 0.196 ppbv m

RT: 3.00 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 24 Jan 2022 20:29 SVE-INFLUENT

Tot Ion:

Ion Ratio

51 100





67 15.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 01/26/2022

Supervised By :Mahesh Dadoda 01/26/2022

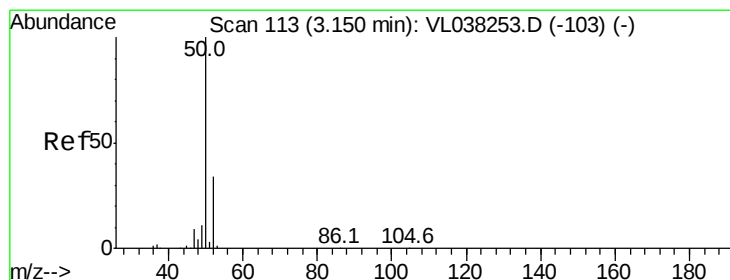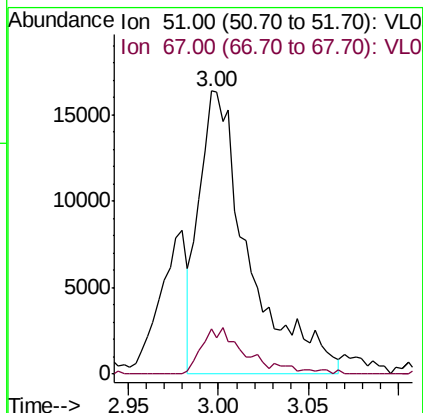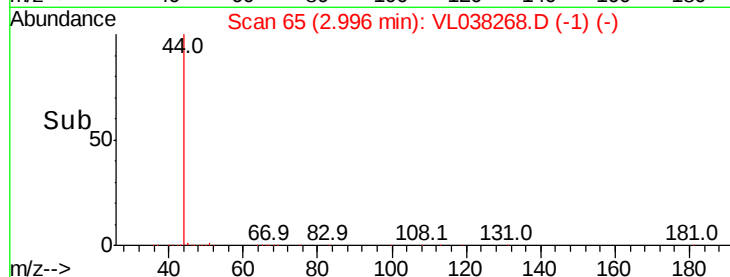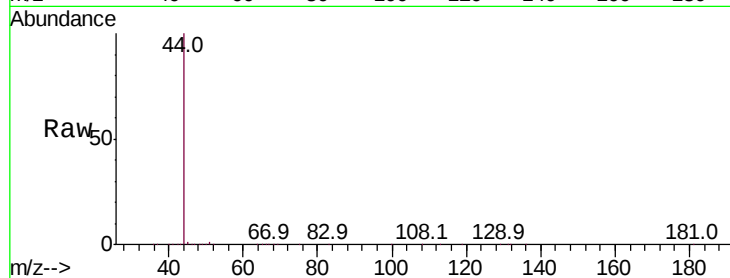

#4

Chloromethane

Concen: 0.192 ppbv m

RT: 3.16 min Scan# 115

Delta R.T. 0.01 min

Lab File: VL038268.D




Acq: 24 Jan 2022 20:29


Tgt Ion: 50 Resp: 10538

Ion Ratio Lower Upper

50 100

52 26.6 27.1 40.7#

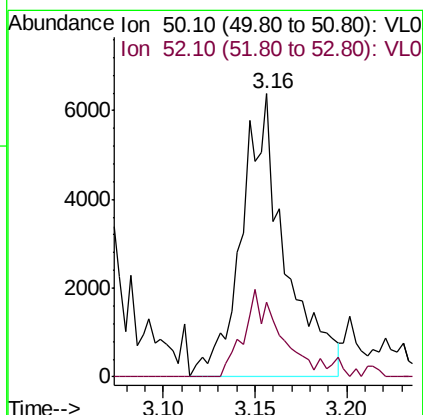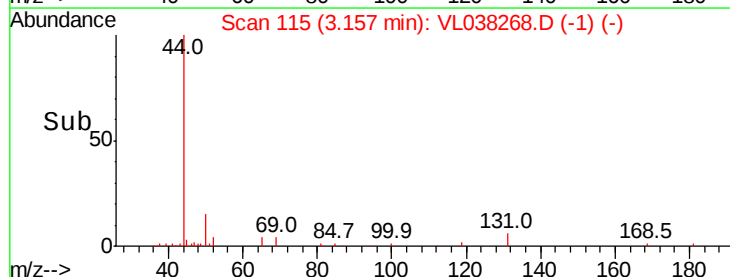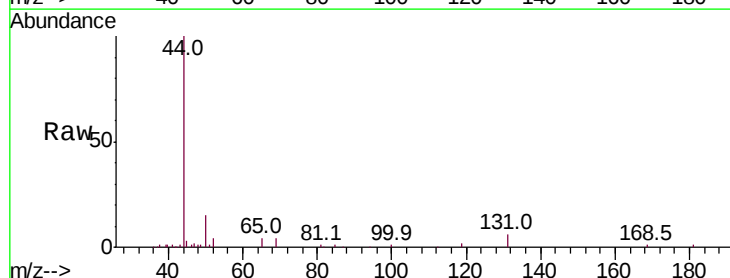




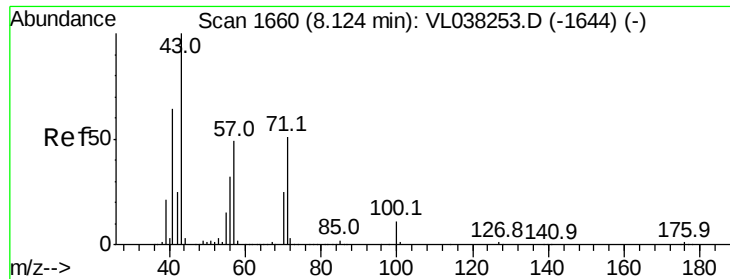


#10
Heptane
Concen: 0.570 ppbv m
RT: 8.13
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId:
Acq: 24 Jan 2022 20:29 SVE-INFLUENT

Tot Ion:
Ion Ratio
43 100
57 47.




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 01/26/2022
Supervised By :Mahesh Dadoda 01/26/2022

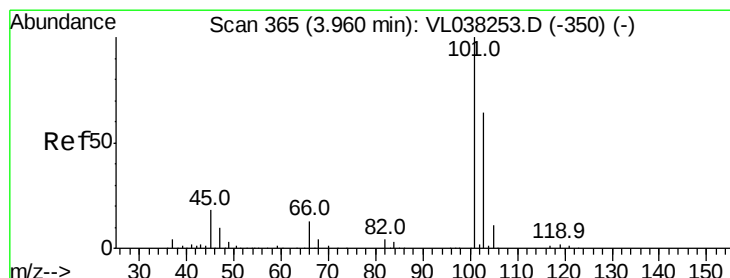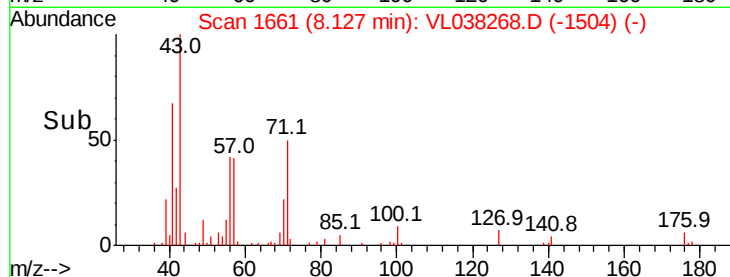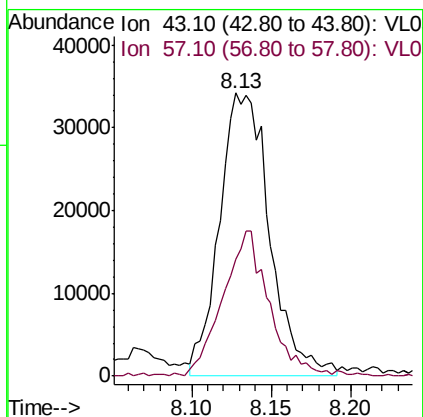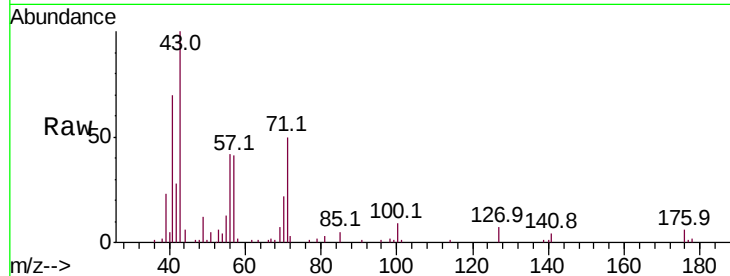

#11
Trichlorofluoromethane
Concen: 0.279 ppbv m
RT: 3.96 min Scan# 365
Delta R.T. 0.00 min
Lab File: VL038268.D
Acq: 24 Jan 2022 20:29

Tgt Ion:101 Resp: 37016
Ion Ratio Lower Upper
101 100
103 57.3 51.2 76.8

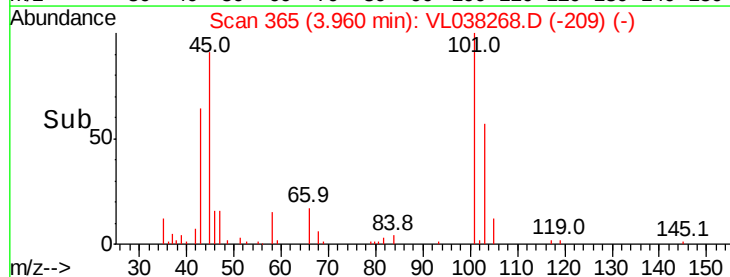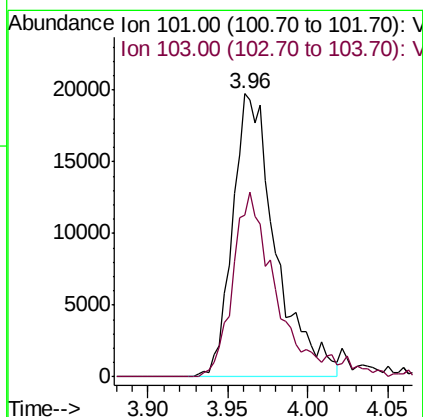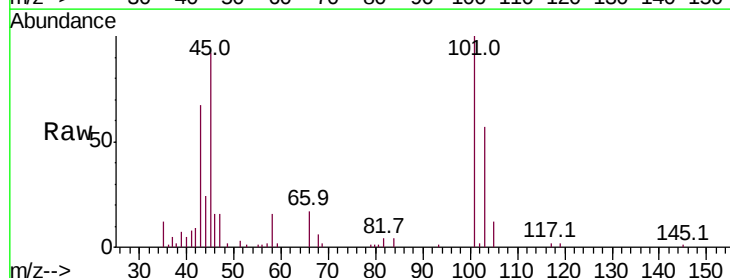

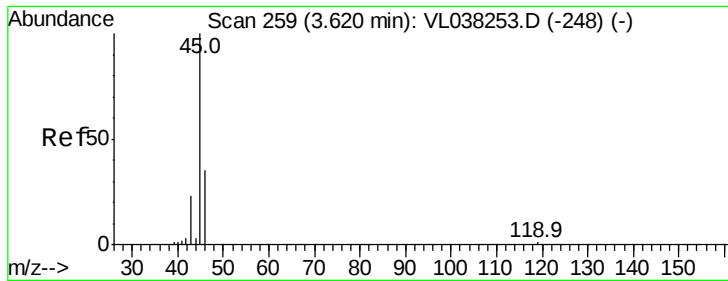

#13

Ethanol

Concen: 797.603 ppbv

RT: 3.62

Delta R.T.

Lab File:

Acq: 24 Jan 2022 20:29

Instrument :

MSVOA_L

ClientSampleId :

SVE-INFLUENT

Tot Ion:

Ion Ratio

45 100





46 37.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 01/26/2022

Supervised By :Mahesh Dadoda 01/26/2022

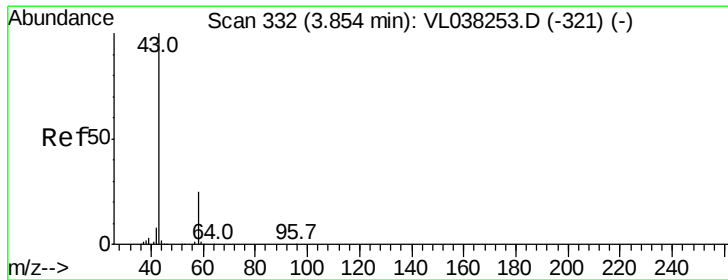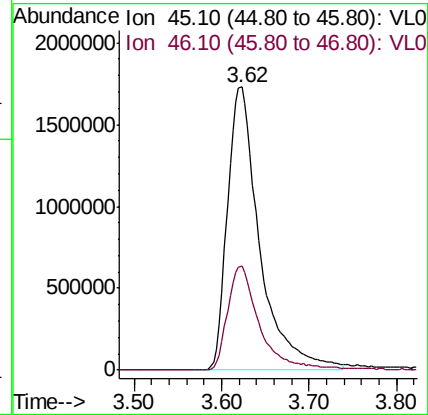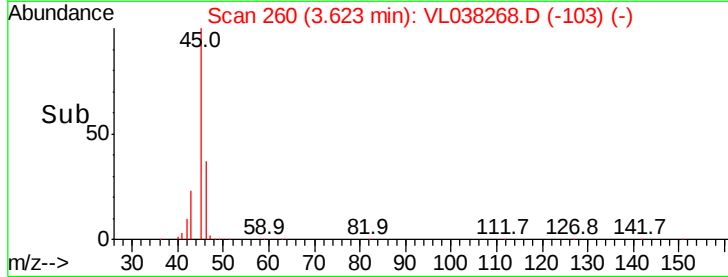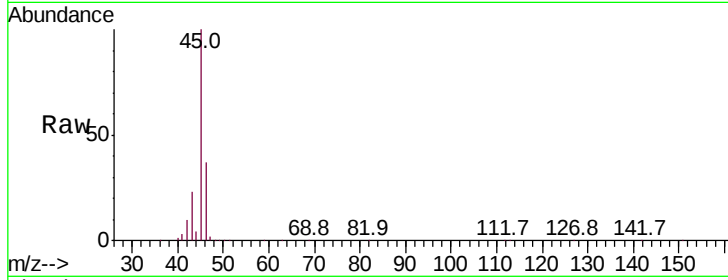

#15

Acetone

Concen: 16.147 ppbv

RT: 3.86 min Scan# 335

Delta R.T. 0.01 min

Lab File: VL038268.D




Acq: 24 Jan 2022 20:29


Tgt Ion: 43 Resp: 1137857

Ion Ratio Lower Upper

43 100

58 27.8 21.5 32.3

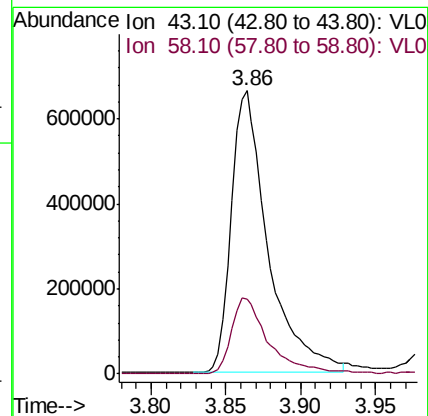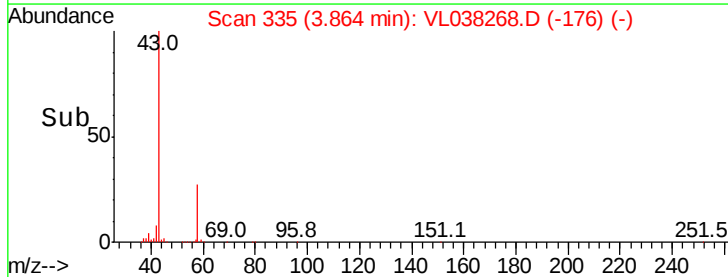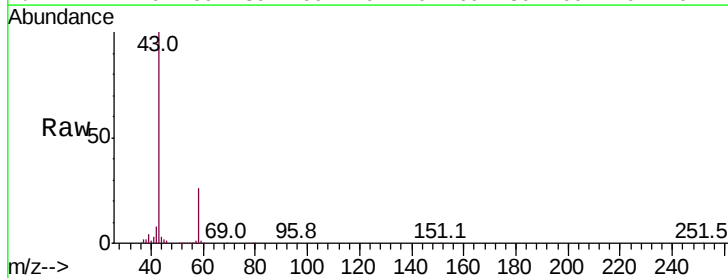

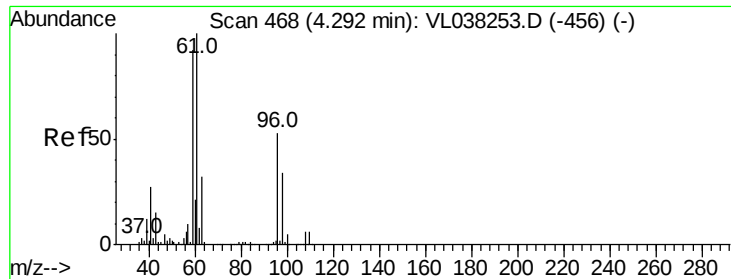

#17

tert-Butyl alcohol

Concen: 0.299 ppbv m

RT: 4.31

Delta R.T. MSVOA_L

Lab File: ClientSampleId :

Acq: 24 Jan 2022 20:29

Tot Ion:

Ion Ratio

59 100





57 0.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 01/26/2022

Supervised By :Mahesh Dadoda 01/26/2022

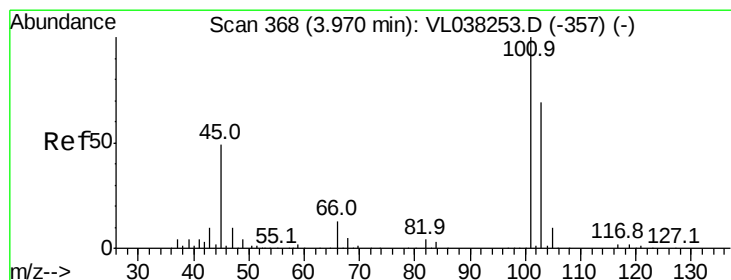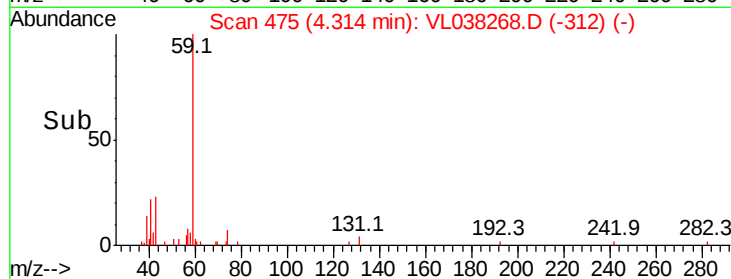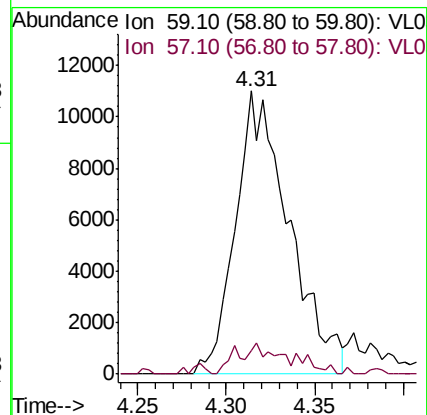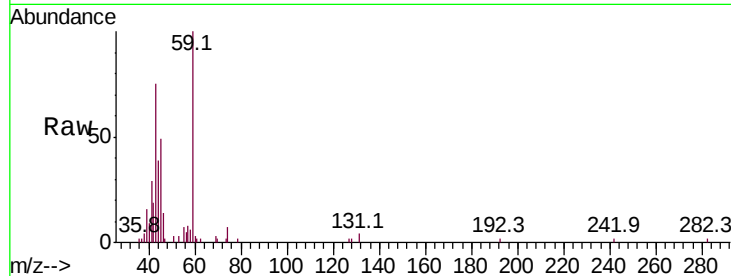

#19

Isopropyl Alcohol

Concen: 11.168 ppbv

RT: 3.99 min Scan# 374

Delta R.T. 0.02 min

Lab File: VL038268.D




Acq: 24 Jan 2022 20:29




Tgt Ion: 45 Resp: 492315

Ion Ratio Lower Upper

45 100

58 3.0 2.3 3.5

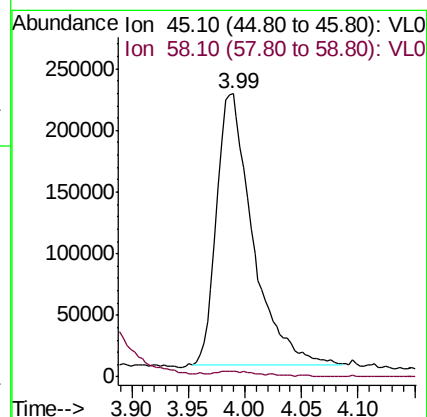


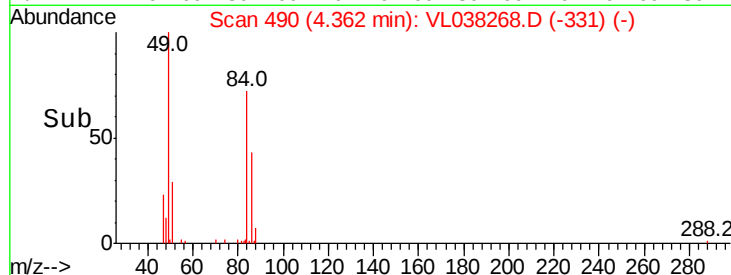
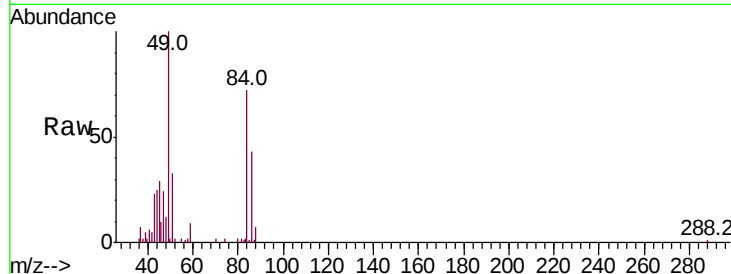



#20
Methvlene Chloride
Concen: 0.488 ppbv
RT: 4.36
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId :
Acq: 24 Jan 2022 20:29 SVE-INFLUENT

Tot Ion:
Ion Ratio
84 100
49 139.
51 42.
86 60.5 51.4 77.0


Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 01/26/2022
Supervised By :Mahesh Dadoda 01/26/2022

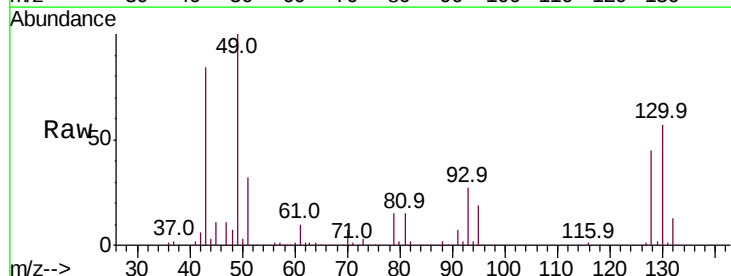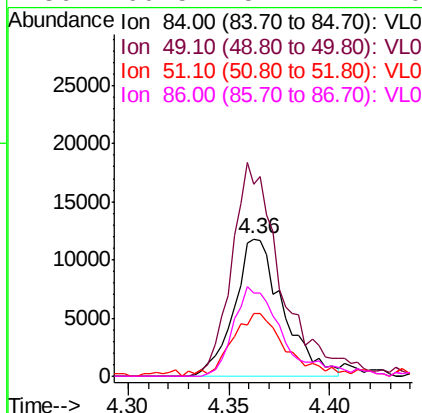

#25
Ethyl Acetate
Concen: 3.432 ppbv
RT: 5.68 min Scan# 900
Delta R.T. 0.00 min
Lab File: VL038268.D
Acq: 24 Jan 2022 20:29

Tgt Ion: 43 Resp: 677240
Ion Ratio Lower Upper
43 100
45 13.7 7.9 11.9#
61 12.7 7.8 11.8#
70 8.6 5.4 8.0#

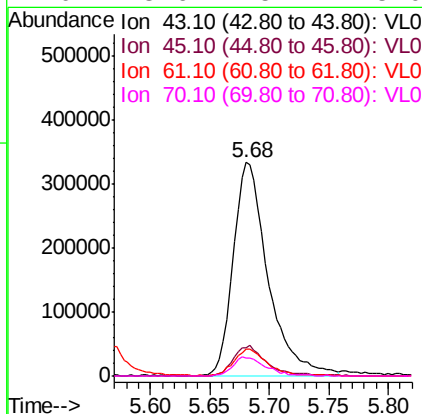




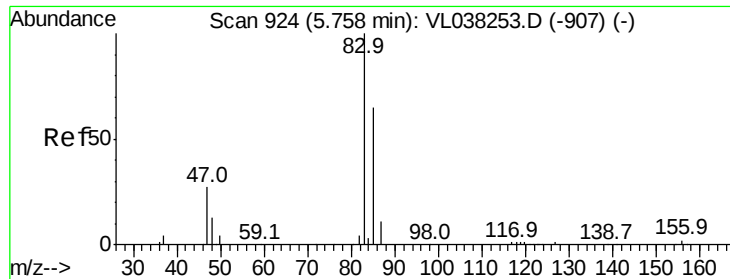


#29
Chloroform
Concen: 0.179 ppbv
RT: 5.76
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId :
SVE-INFLUENT
Acq: 24 Jan 2022 20:29

Tot Ion:
Ion Ratio
83 100
85 61.




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 01/26/2022
Supervised By :Mahesh Dadoda 01/26/2022

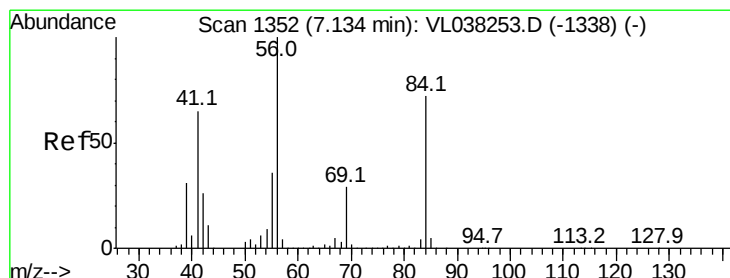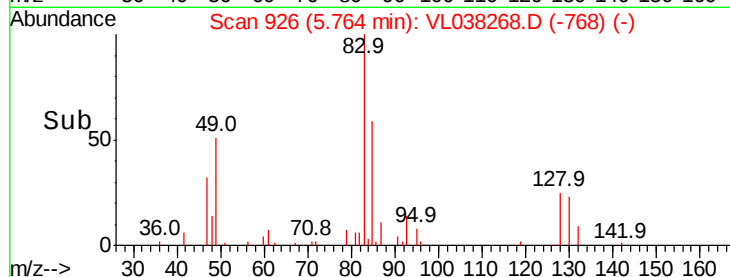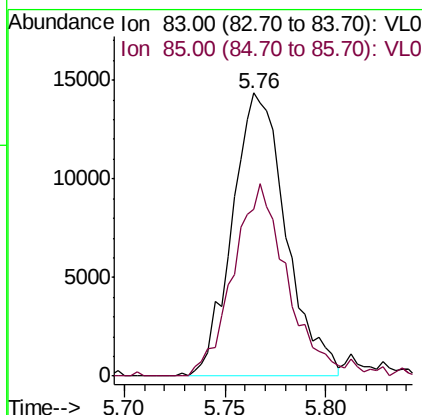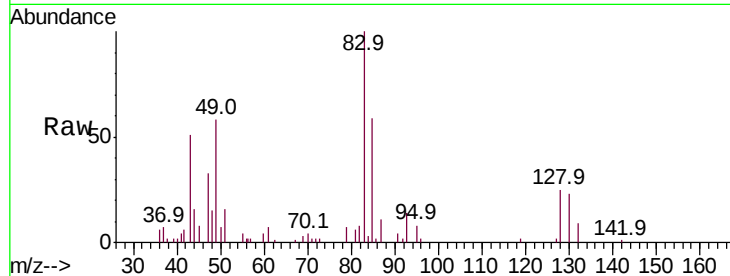

#30
Cyclohexane
Concen: 0.208 ppbv m
RT: 7.15 min Scan# 1356
Delta R.T. 0.01 min
Lab File: VL038268.D
Acq: 24 Jan 2022 20:29

Tgt Ion: 84 Resp: 16631
Ion Ratio Lower Upper
84 100
56 0.0 112.7 169.1#
41 92.8 71.1 106.7

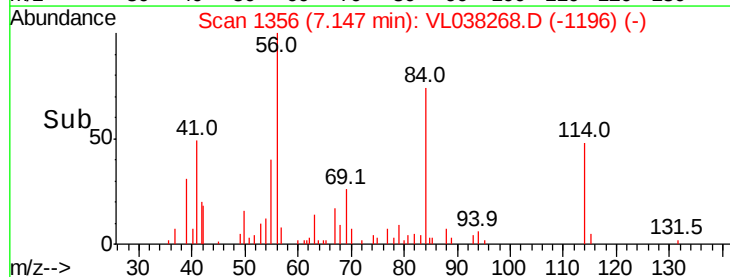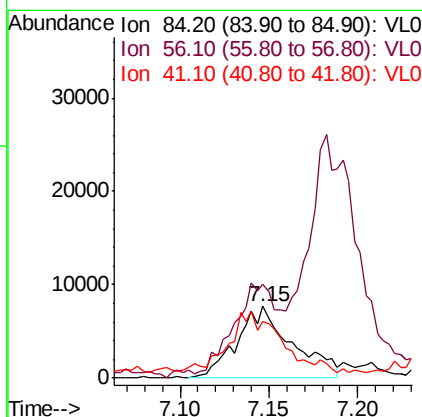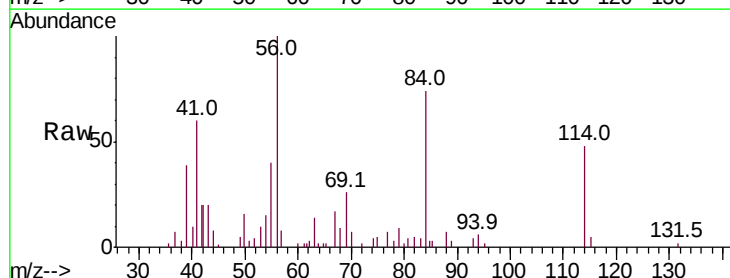




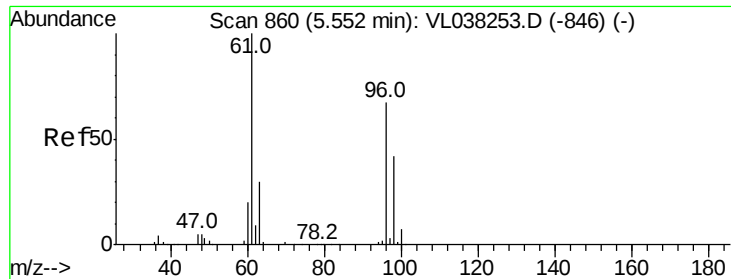


#31
 cis-1,2-Dichloroethene
 Concen: 1.257 ppbv
 RT: 5.56
 Instrument: MSVOA_1
 Delta R.T.:
 Lab File: ClientSampleId:
 Acq: 24 Jan 2022 20:29

Tot Ion:
 Ion Ratio
 61 100
 96 62.
 98 36.




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 01/26/2022
 Supervised By :Mahesh Dadoda 01/26/2022

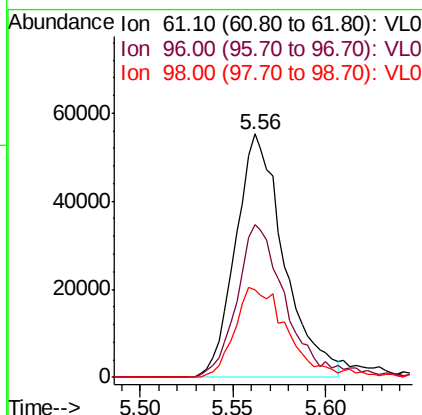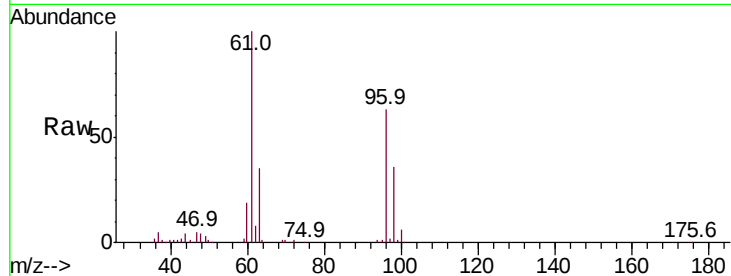

#32
 1,1,1-Trichloroethane
 Concen: 0.151 ppbv m
 RT: 6.52 min Scan# 1161
 Delta R.T. 0.00 min
 Lab File: VL038268.D
 Acq: 24 Jan 2022 20:29

Tgt Ion: 97 Resp: 22539
 Ion Ratio Lower Upper
 97 100
 99 62.0 51.5 77.3
 61 54.5 40.5 60.7

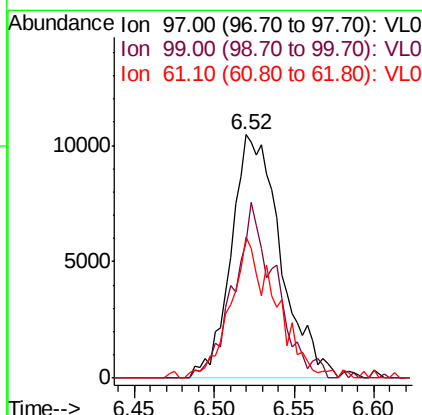







#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.19
 Instrument : MSVOA_1
 Delta R.T.:
 Lab File: ClientSampleId :
 SVE-INFLUENT
 Acq: 24 Jan 2022 20:29

Tot Ion:1
 Ion Rati
 114 100
 63 26.
 88 18.




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 01/26/2022
 Supervised By :Mahesh Dadoda 01/26/2022

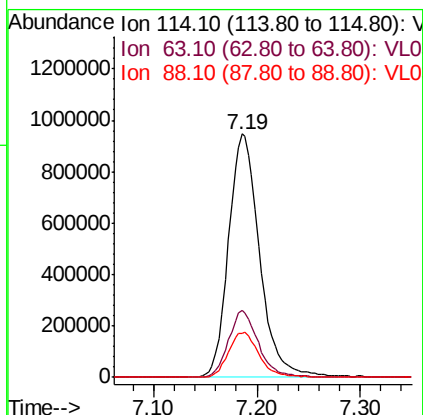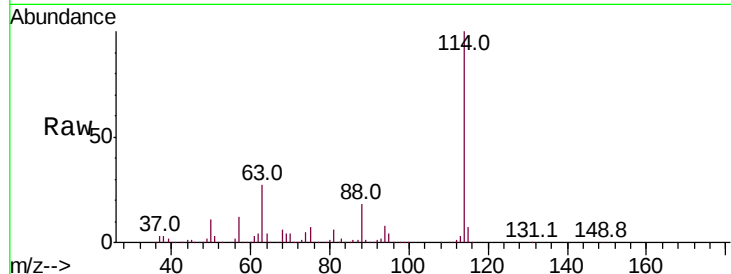

#34
 2-Butanone
 Concen: 10.187 ppbv
 RT: 5.25 min Scan# 767
 Delta R.T. 0.01 min
 Lab File: VL038268.D
 Acq: 24 Jan 2022 20:29

Tgt Ion: 43 Resp: 661271
 Ion Ratio Lower Upper
 43 100
 72 21.7 18.1 27.1

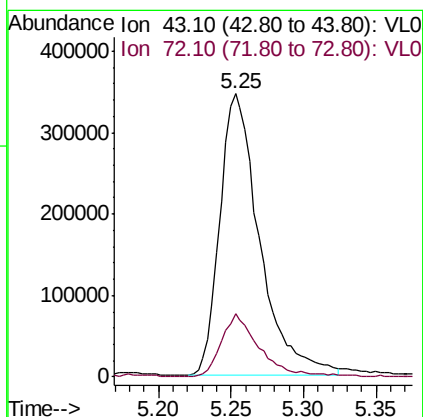




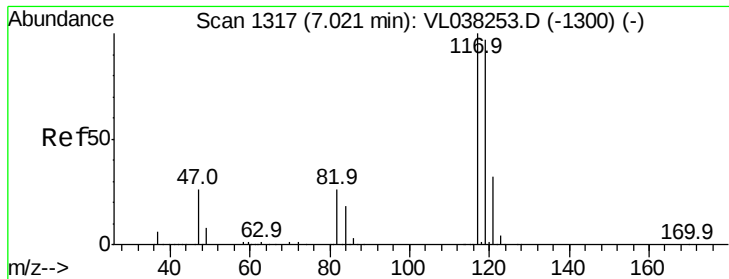


#35
Carbon Tetrachloride
Concen: 0.111 ppbv
RT: 7.03
Instrument: MSVOA_L
Delta R.T.:
Lab File: ClientSampleId :
Acq: 24 Jan 2022 20:29

Tot Ion:1
Ion Rati
117 100
119 72.
121 24.




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 01/26/2022
Supervised By :Mahesh Dadoda 01/26/2022

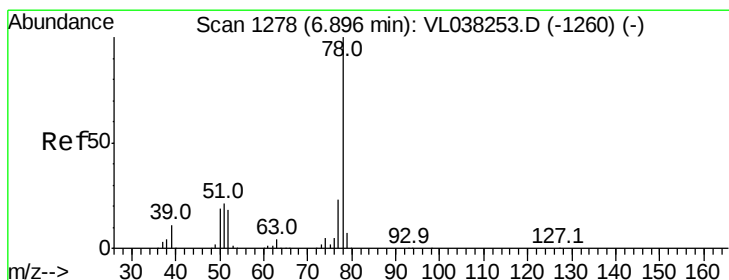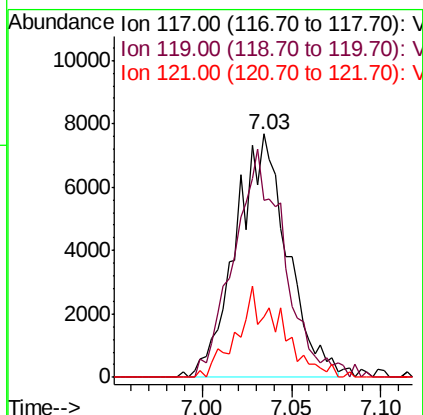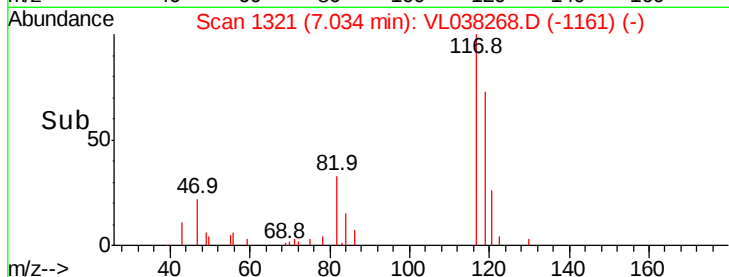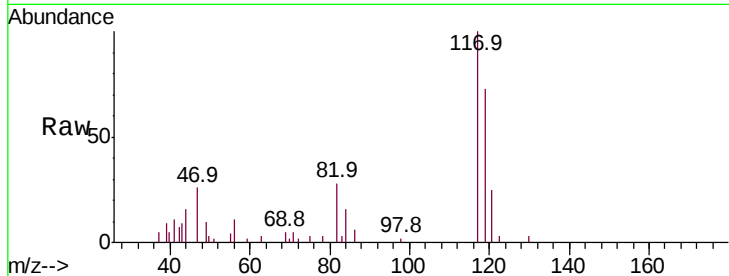

#36
Benzene
Concen: 0.565 ppbv
RT: 6.91 min Scan# 1281
Delta R.T. 0.01 min
Lab File: VL038268.D
Acq: 24 Jan 2022 20:29

Tgt Ion: 78 Resp: 99154
Ion Ratio Lower Upper
78 100
77 20.5 18.2 27.2
50 20.8 15.1 22.7

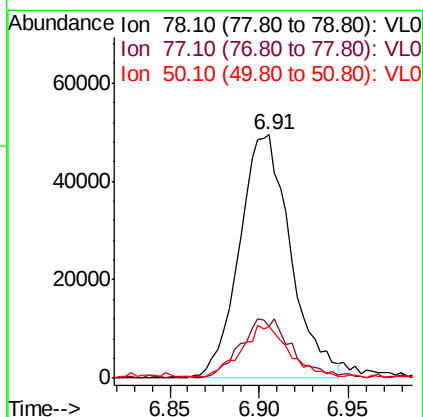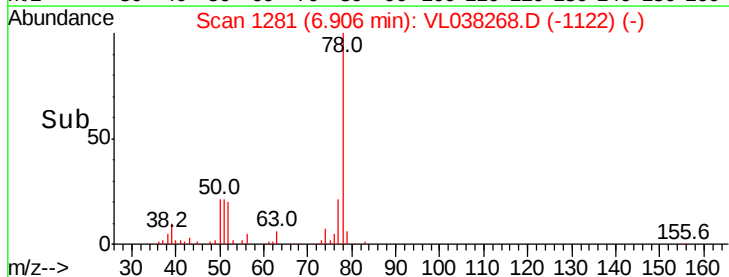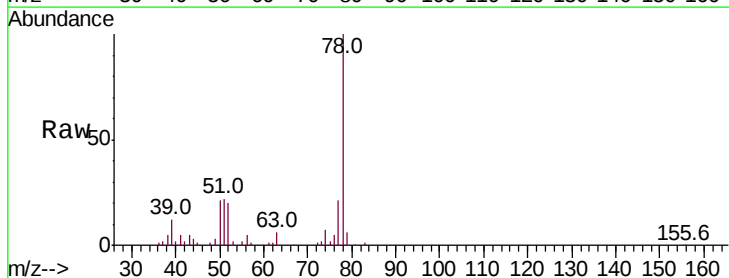

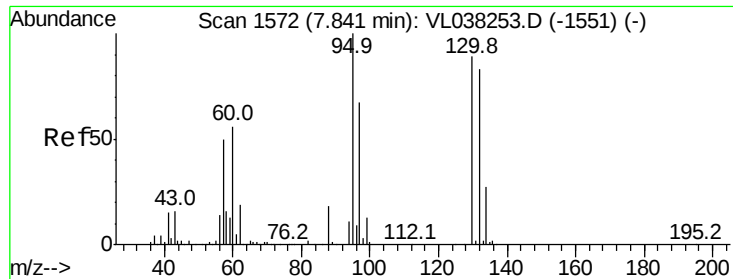

#38

Trichloroethene

Concen: 0.893 ppbv m

RT: 7.84 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 24 Jan 2022 20:29 SVE-INFLUENT

Tot Ion:1

Ion Rati

130 100

95 108.

132 87.

97 64.2

59.6





89.4

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 01/26/2022

Supervised By :Mahesh Dadoda 01/26/2022

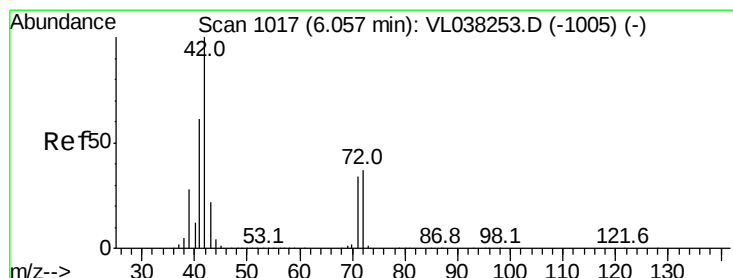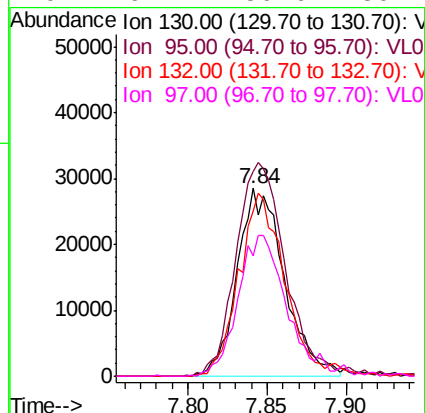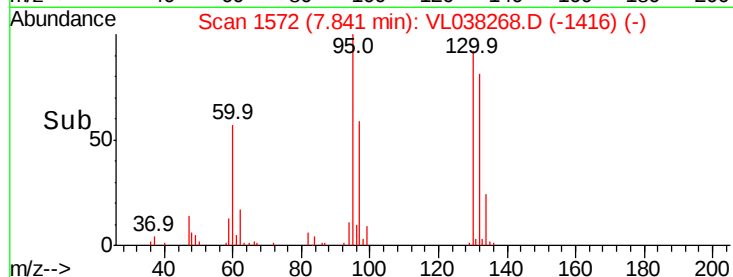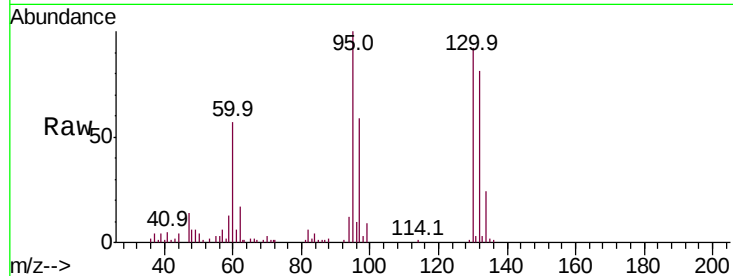

#41

Tetrahydrofuran

Concen: 20.055 ppbv

RT: 6.06 min Scan# 1017

Delta R.T. 0.00 min

Lab File: VL038268.D

Acq: 24 Jan 2022 20:29

Tgt Ion: 42 Resp: 875130

Ion Ratio Lower Upper




42 100


72 37.0

71 35.8

29.7 44.5

29.4 44.2

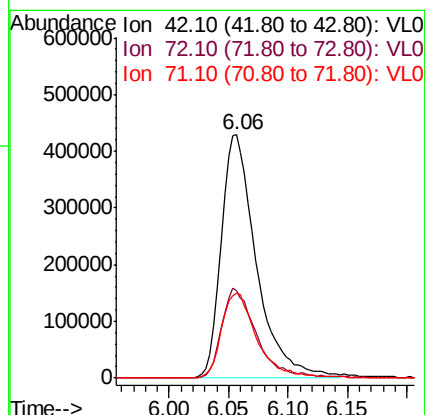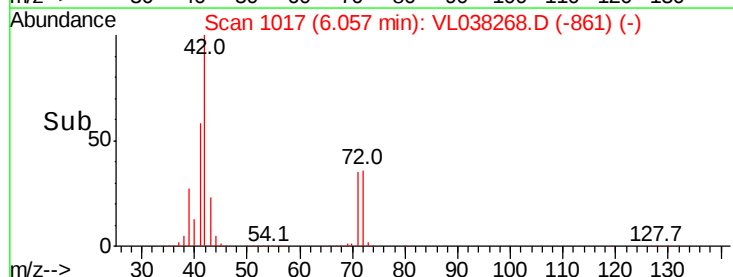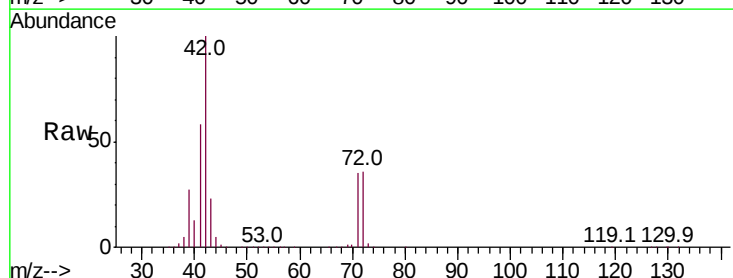




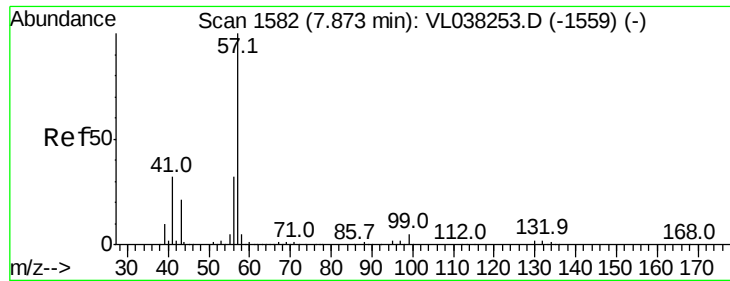


#44
 2,2,4-Trimethylpentane
 Concen: 0.405 ppbv
 RT: 7.88
 Instrument: MSVOA_1
 Delta R.T.:
 Lab File: ClientSampleId:
 SVE-INFLUENT
 Acq: 24 Jan 2022 20:29

Tot Ion:
 Ion Ratio
 57 100
 41 41.
 56 43.




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 01/26/2022
 Supervised By :Mahesh Dadoda 01/26/2022

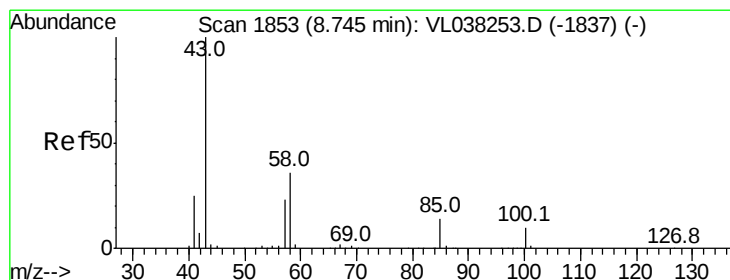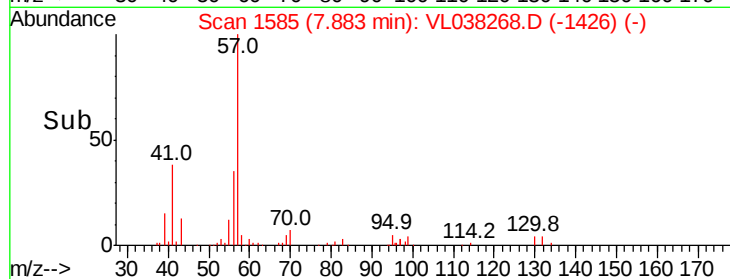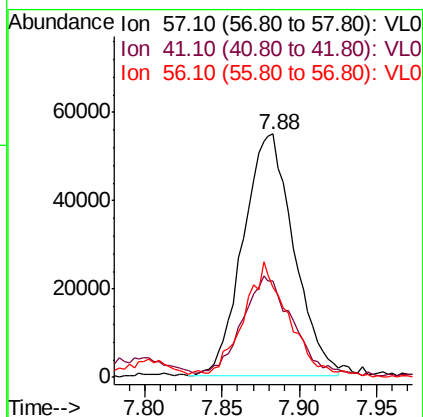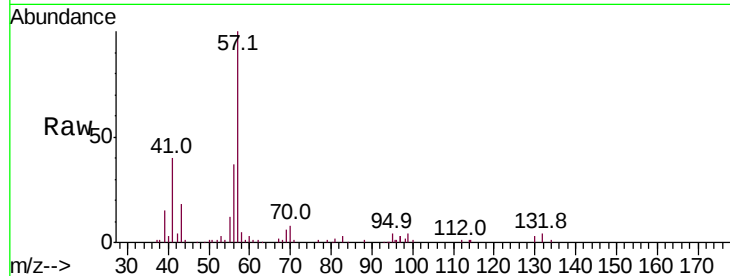

#50
 4-Methyl-2-Pentanone
 Concen: 1.643 ppbv
 RT: 8.75 min Scan# 1856
 Delta R.T. 0.01 min
 Lab File: VL038268.D
 Acq: 24 Jan 2022 20:29

Tgt Ion: 43 Resp: 190285
 Ion Ratio Lower Upper
 43 100
 58 35.2 28.2 42.4

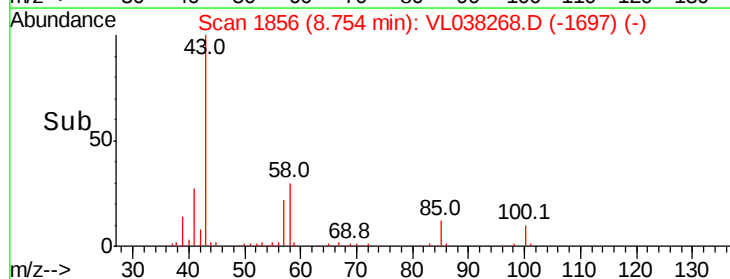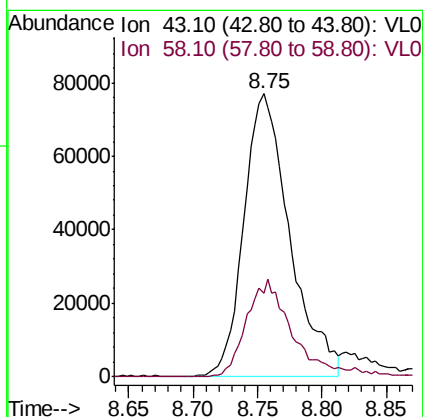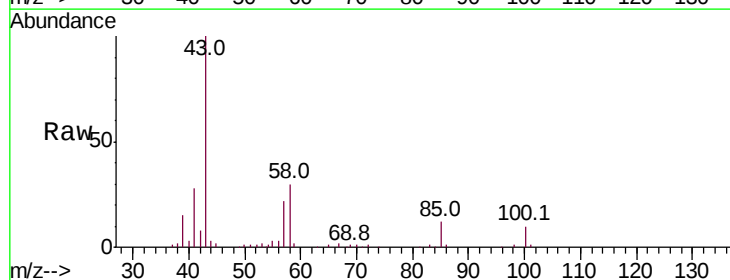

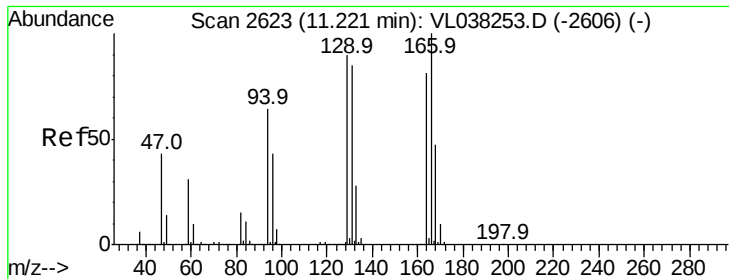

#52

Tetrachloroethene

Concen: 1.719 ppbv

RT: 11.23

Delta R.T. MSVOA_1





Lab File: ClientSampleId :

Acq: 24 Jan 2022 20:29 SVE-INFLUENT

Tot Ion:1
Ion Rati
164 100
166 134.
129 109.
131 109.6 83.6 125.4

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 01/26/2022
Supervised By :Mahesh Dadoda 01/26/2022

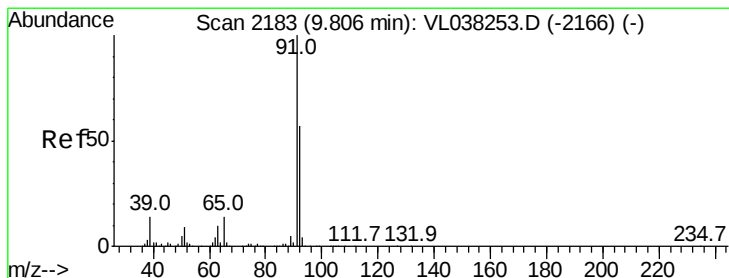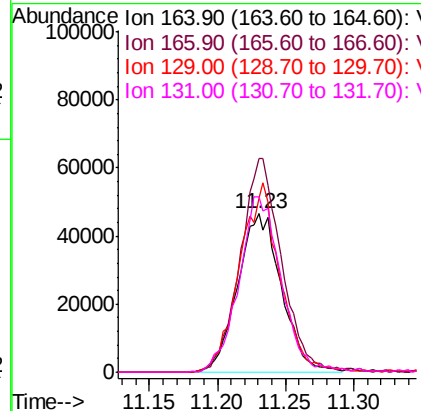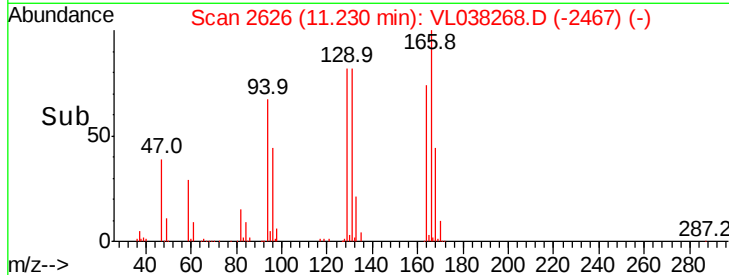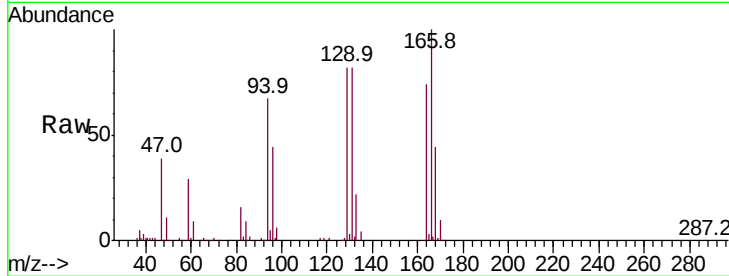

#53

Toluene

Concen: 24.604 ppbv




RT: 9.81 min Scan# 2185


Delta R.T. 0.01 min

Lab File: VL038268.D

Acq: 24 Jan 2022 20:29

Tgt Ion: 91 Resp: 4781536
Ion Ratio Lower Upper
91 100
92 61.9 47.4 71.0

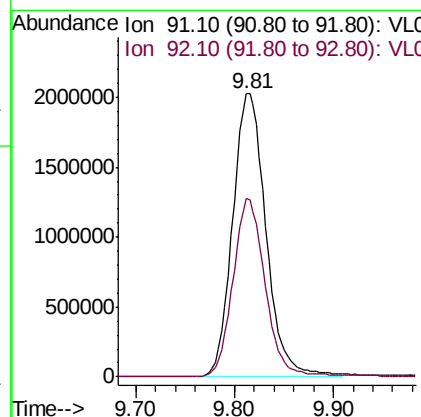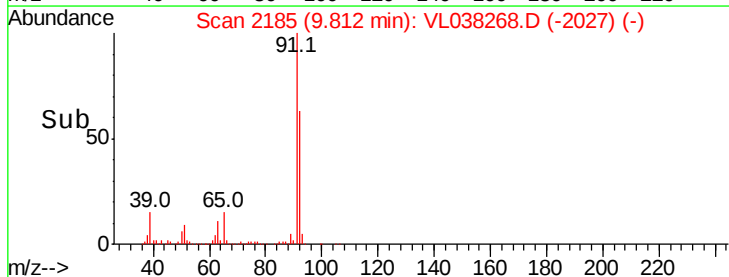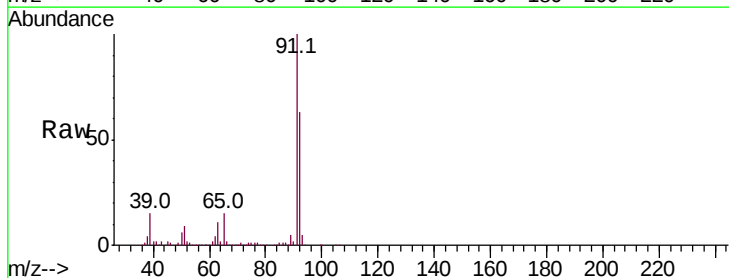




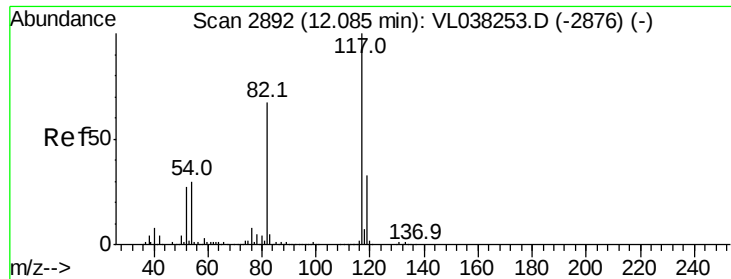


#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.09 min
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId :
Acq: 24 Jan 2022 20:29 SVE-INFLUENT

Tot Ion: 1
Ion Ratio
117 100
82 69.
119 33.




Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 01/26/2022
Supervised By : Mahesh Dadoda 01/26/2022

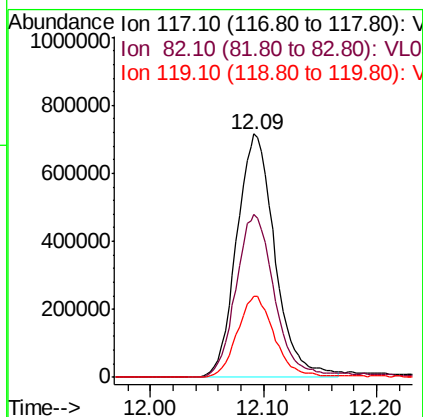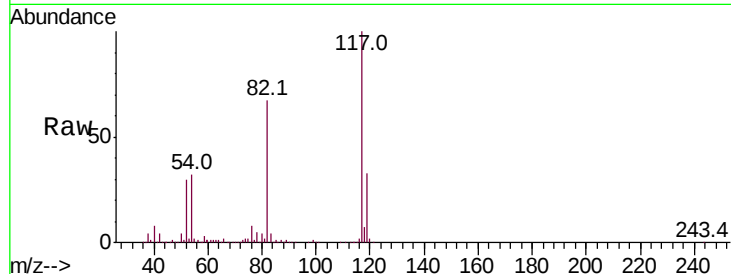

#58
Ethyl Benzene
Concen: 0.844 ppbv
RT: 12.72 min Scan# 3089
Delta R.T.: 0.01 min
Lab File: VL038268.D
Acq: 24 Jan 2022 20:29

Tgt Ion: 91 Resp: 209117
Ion Ratio Lower Upper
91 100
106 24.8 24.1 36.1

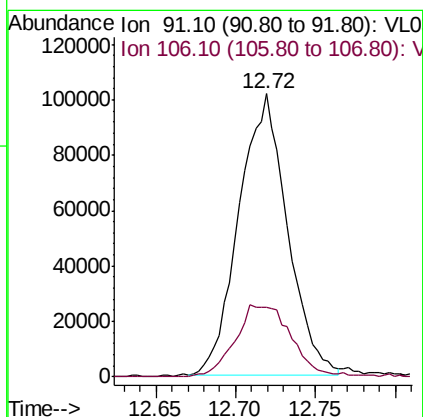




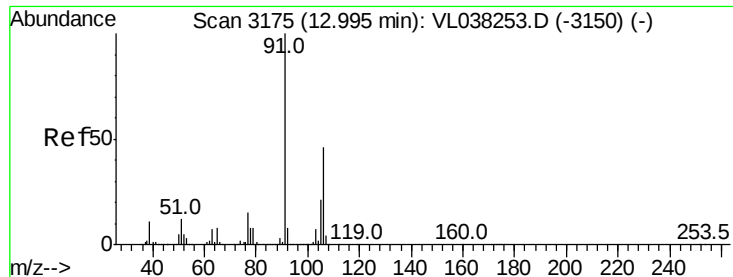


#59
m/p-Xylene
Concen: 3.073 ppbv
RT: 12.97 min
Instrument: MSVOA_1
Delta R.T.: 0.01 min
Lab File: ClientSampleId : SVE-INFLUENT
Acq: 24 Jan 2022 20:29

Tot Ion:
Ion Ratio
91 100
106 45.




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 01/26/2022
Supervised By :Mahesh Dadoda 01/26/2022

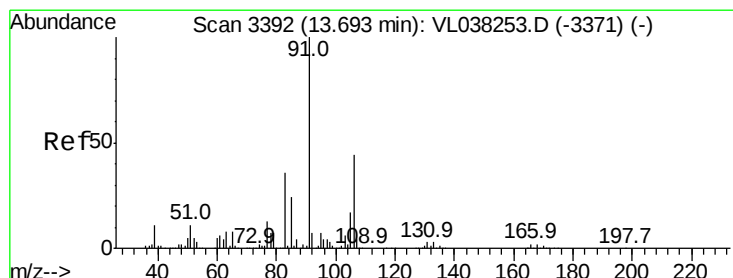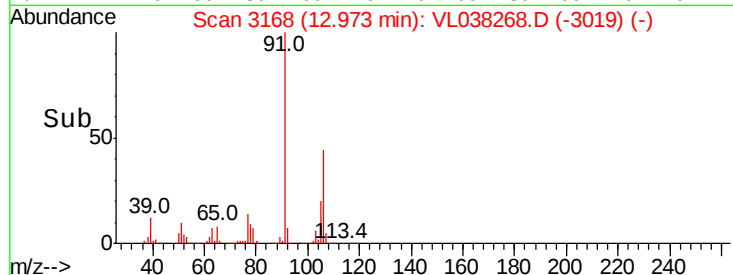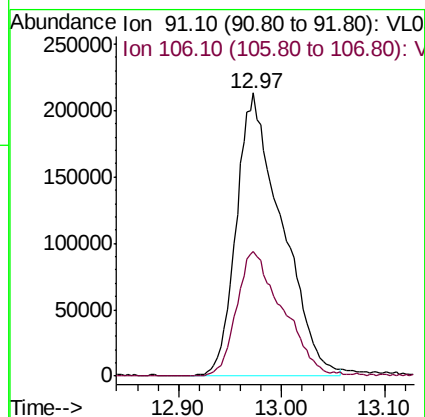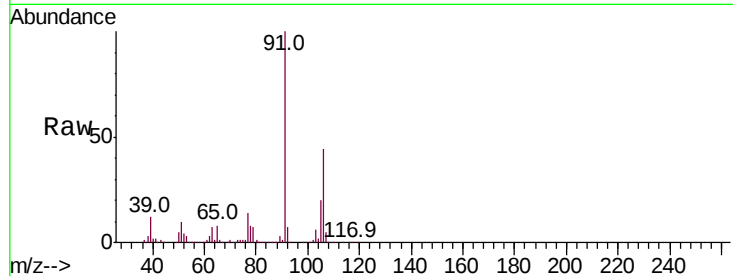

#60
o-Xylene
Concen: 1.400 ppbv
RT: 13.70 min Scan# 3394
Delta R.T.: 0.01 min
Lab File: VL038268.D
Acq: 24 Jan 2022 20:29

Tgt Ion: 91 Resp: 275398
Ion Ratio Lower Upper
91 100
106 43.2 22.2 66.6

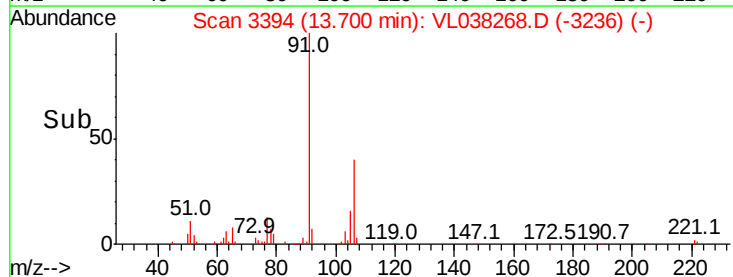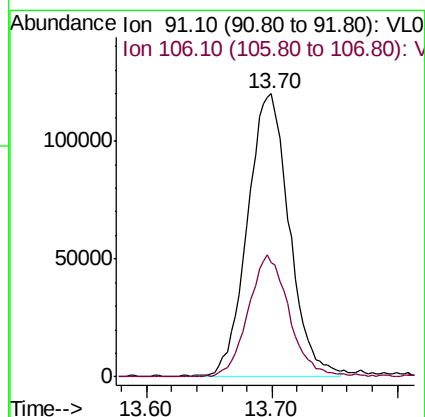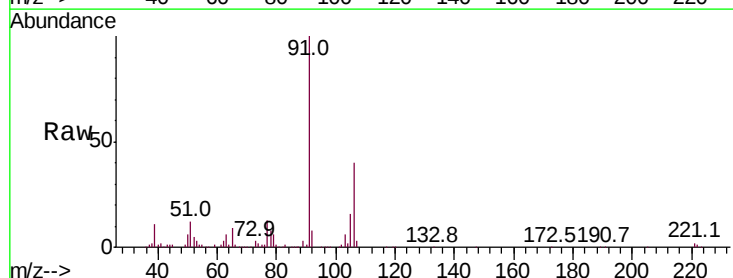

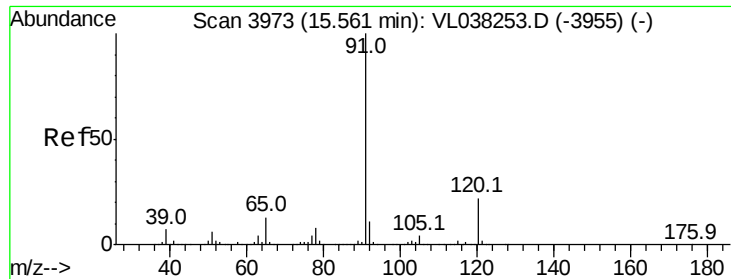

#64

n-propylbenzene

Concen: 0.265 ppbv m

RT: 15.56

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 24 Jan 2022 20:29

Tot Ion:1

Ion Ratio

120 100





91 0.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 01/26/2022

Supervised By :Mahesh Dadoda 01/26/2022

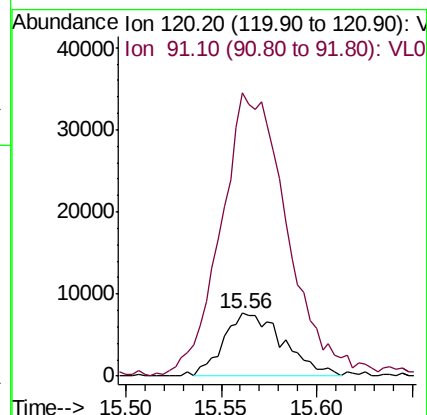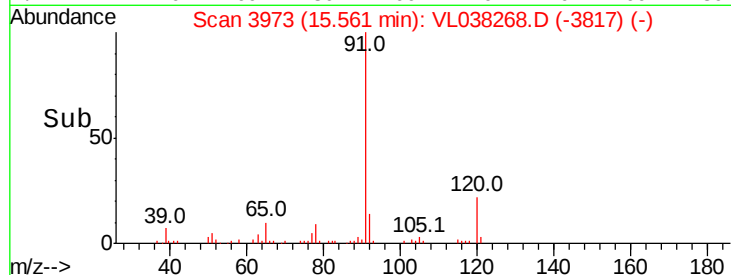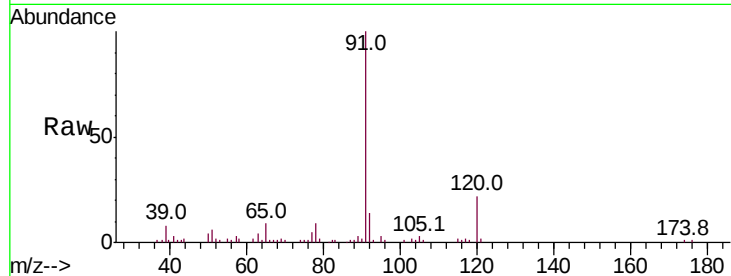

#68

1-Bromo-4-Fluorobenzene

Concen: 10.572 ppbv

RT: 14.42 min Scan# 3619

Delta R.T. 0.01 min

Lab File: VL038268.D

Acq: 24 Jan 2022 20:29




Tgt Ion: 95 Resp: 1353318


Ion Ratio Lower Upper

95 100

174 59.6 48.3 72.5

175 4.4 3.5 5.3

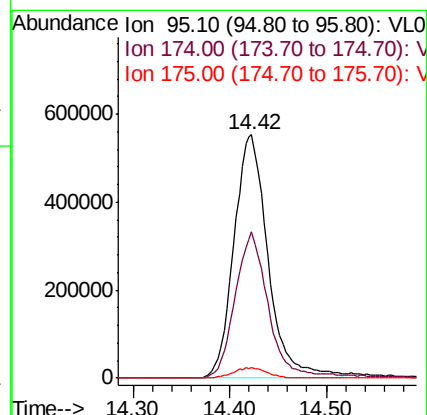




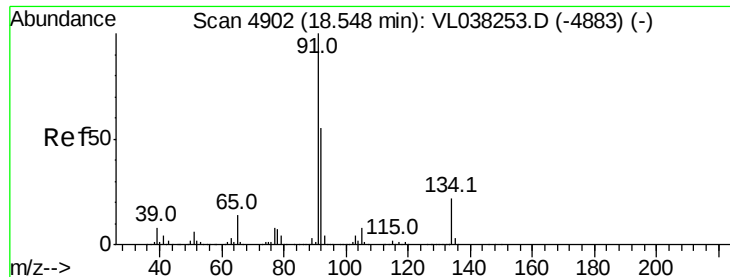


#70
n-Butylbenzene
Concen: 0.170 ppbv m
RT: 18.56
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId :
Acq: 24 Jan 2022 20:29 SVE-INFLUENT

Tot Ion:
Ion Ratio
91 100
92 34.
134 70.




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 01/26/2022
Supervised By :Mahesh Dadoda 01/26/2022

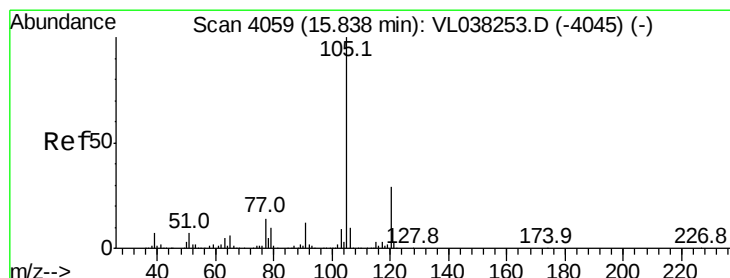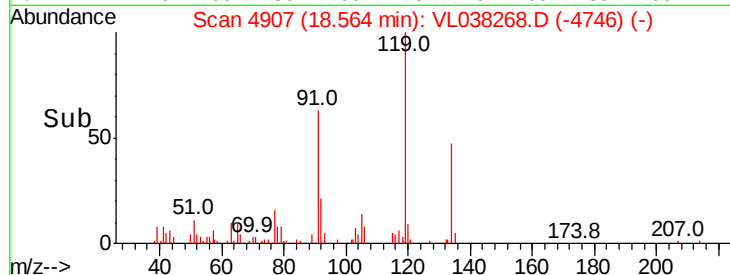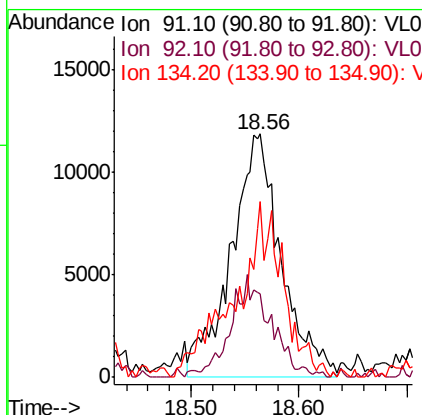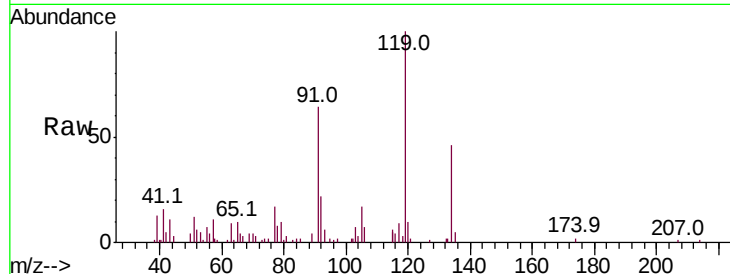

#72
4-Ethyltoluene
Concen: 0.512 ppbv m
RT: 15.85 min Scan# 4062
Delta R.T. 0.01 min
Lab File: VL038268.D
Acq: 24 Jan 2022 20:29

Tgt Ion:105 Resp: 105349
Ion Ratio Lower Upper
105 100
120 0.0 23.8 35.8#
91 0.0 10.2 15.4#
77 0.0 11.7 17.5#

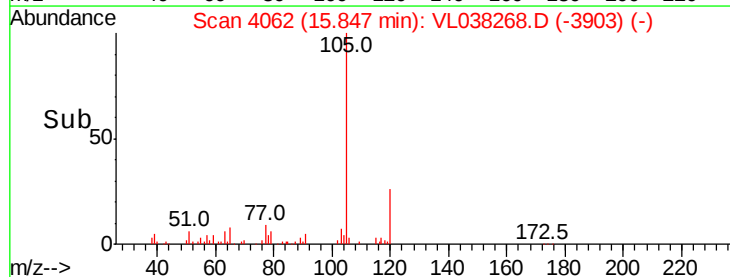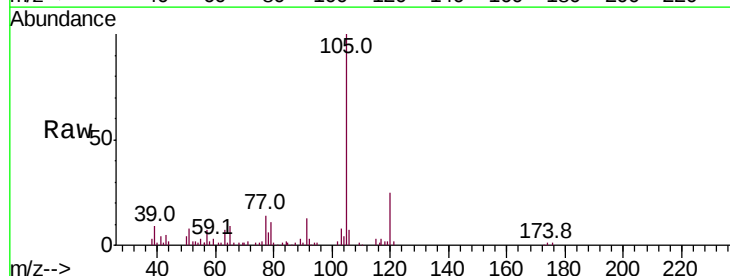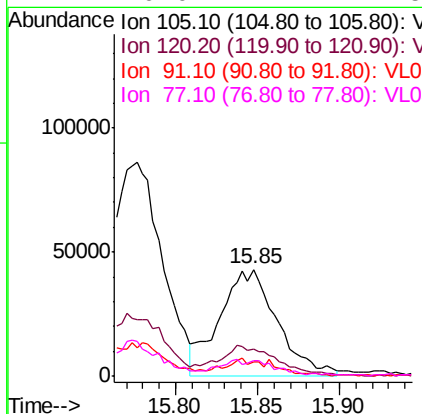

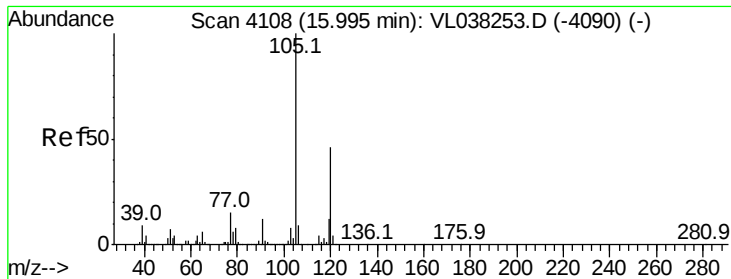

#73

1,3,5-Trimethylbenzene

Concen: 0.456 ppbv m

RT: 16.00

Delta R.T. MSVOA_L

Lab File: ClientSampleId :

Acq: 24 Jan 2022 20:29

Tot Ion:1

Ion Rati

105 100





120 32.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 01/26/2022

Supervised By :Mahesh Dadoda 01/26/2022

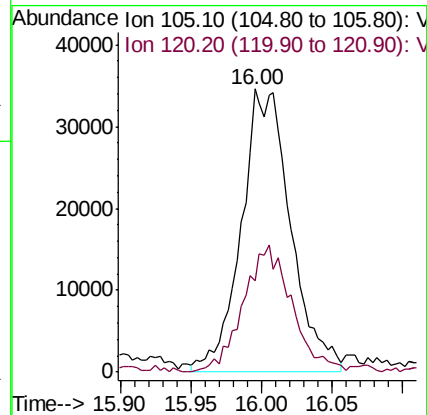

#74

1,2,4-Trimethylbenzene

Concen: 1.853 ppbv m

RT: 16.77 min Scan# 4350

Delta R.T. 0.01 min

Lab File: VL038268.D

Acq: 24 Jan 2022 20:29

Tgt Ion:105 Resp: 361141




Ion Ratio Lower Upper


105 100

120 37.9 37.2 55.8

91 11.0 36.6 55.0#

77 13.1 16.9 25.3#

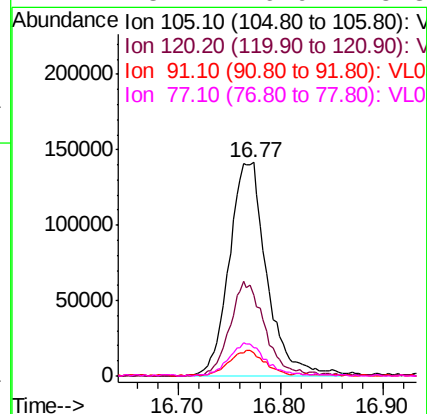

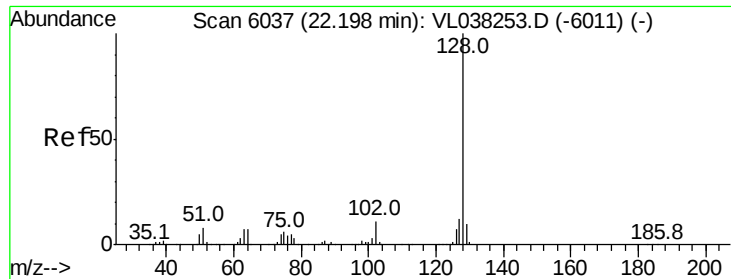

#79

Naphthalene

Concen: 0.591 ppbv m

RT: 22.20

Delta R.T

Lab File: ClientSampleId :

Acq: 24 Jan 2022 20.29

Tot Ion:1

Ion Rati

128 100

127 16.

129 8.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 01/26/2022

Supervised By :Mahesh Dadoda 01/26/2022

